

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042421\
 Data File : PP035262.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Apr 2021 15:09
 Operator : DD\AJ
 Sample : M2149-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-36-10.5-11.0

Manual Integrations
 APPROVED

Ankita
 4/27/2021 10:55:08 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 09:25:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.840	4.243	1563069	993439	19.182	19.291
2) SA Decachlor...	10.745	9.527	1498088	587662	23.706	24.733
Target Compounds						
41) L9 AR-1268-1	9.303	8.421	177714	84768	21.449	23.981
42) L9 AR-1268-2	9.396	8.486	155822	84994	19.504	25.130 #
43) L9 AR-1268-3	9.611	8.689	171020	82187	22.428m	26.510m
44) L9 AR-1268-4	10.035	8.981	99149	46674	41.478	44.266
45) L9 AR-1268-5	10.428	9.273	494012	209580	22.280	26.948

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042421\
Data File : PP035262.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Apr 2021 15:09
Operator : DD\AJ
Sample : M2149-03
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleID :
SB-36-10.5-11.0


Manual Integrations
APPROVED

Ankita
4/27/2021 10:55:08 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 09:25:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

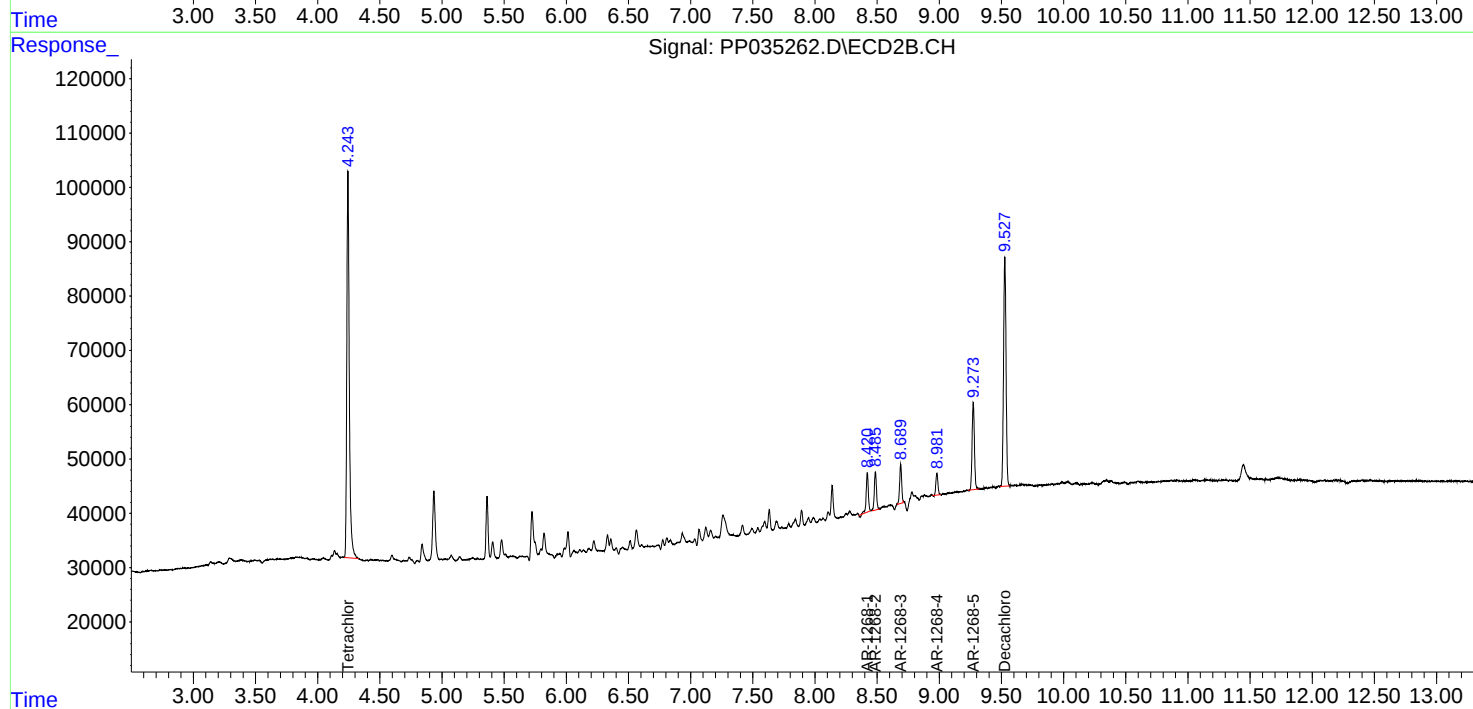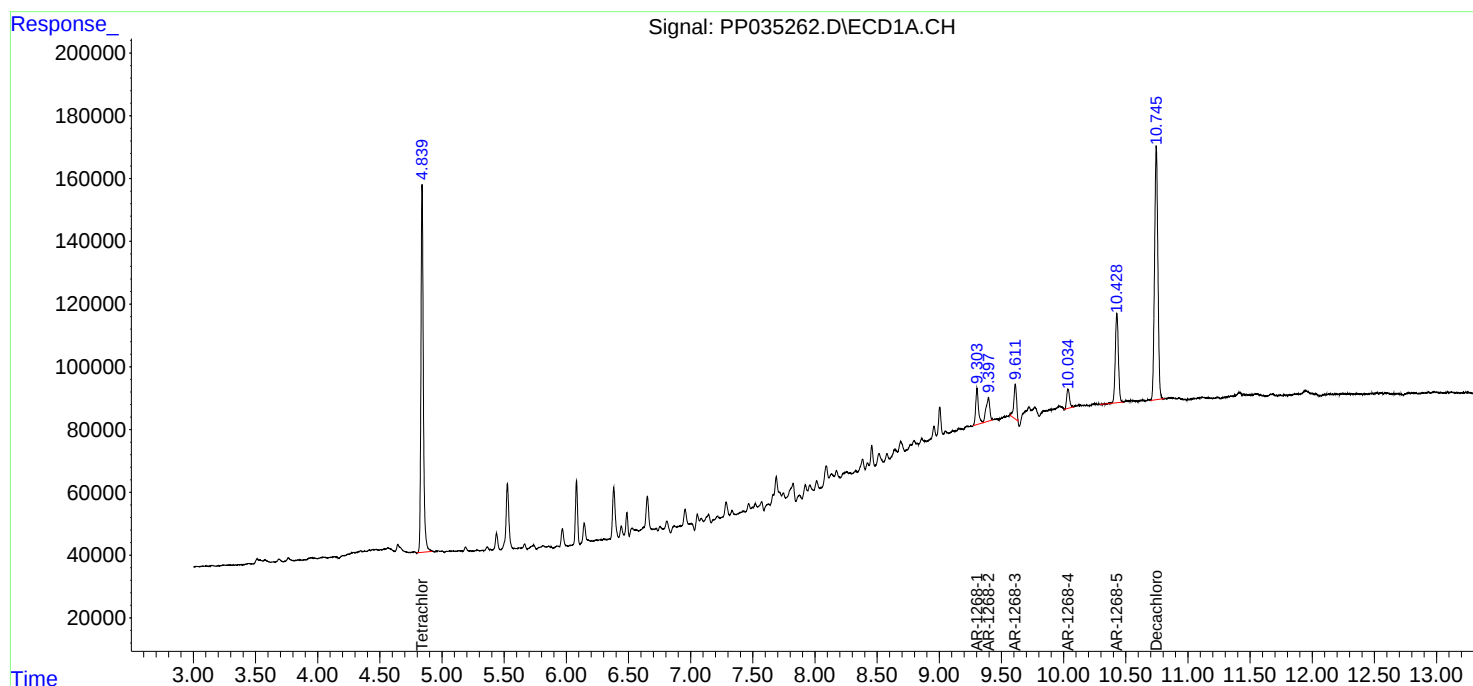

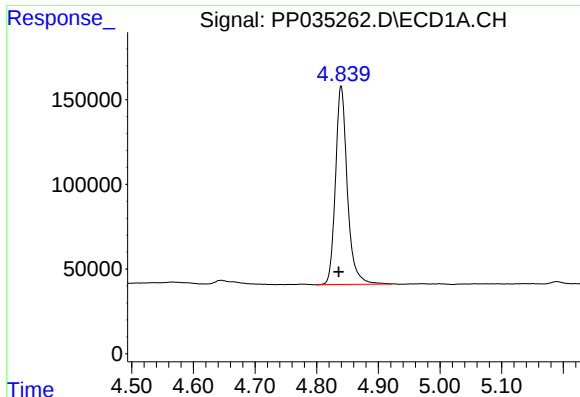


#1 Tetrachloro-m-xylene

R.T.: 4.840 min
Delta R.T.: 0.004 min
Response: 1563069
Conc: 19.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-36-10.5-11.0


Manual Integrations
APPROVED

Ankita
4/27/2021 10:55:08 AM

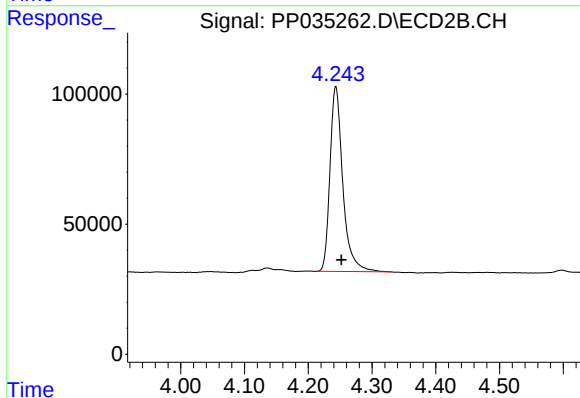


#1 Tetrachloro-m-xylene

R.T.: 4.243 min
Delta R.T.: -0.009 min
Response: 993439
Conc: 19.29 ng/ml

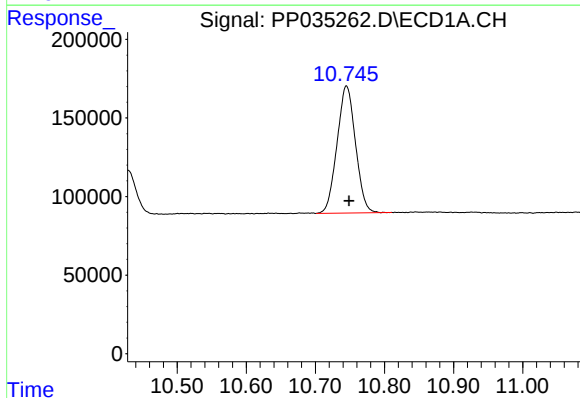


#2 Decachlorobiphenyl

R.T.: 10.745 min
Delta R.T.: -0.004 min
Response: 1498088
Conc: 23.71 ng/ml

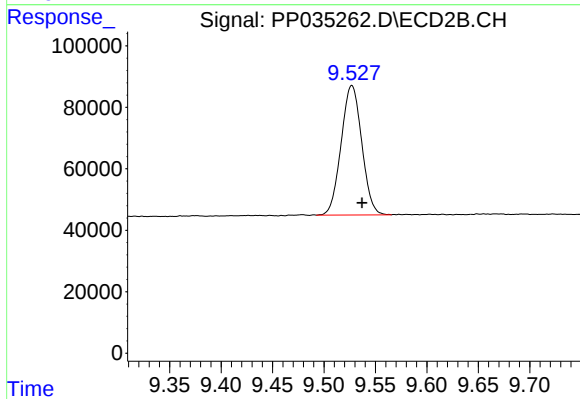

#2 Decachlorobiphenyl

R.T.: 9.527 min
Delta R.T.: -0.010 min
Response: 587662
Conc: 24.73 ng/ml

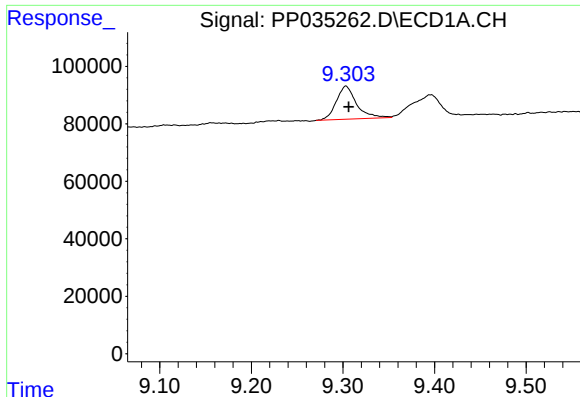


#41 AR-1268-1

R.T.: 9.303 min
Delta R.T.: -0.003 min
Response: 177714
Conc: 21.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-36-10.5-11.0


Manual Integrations
APPROVED

Ankita
4/27/2021 10:55:08 AM

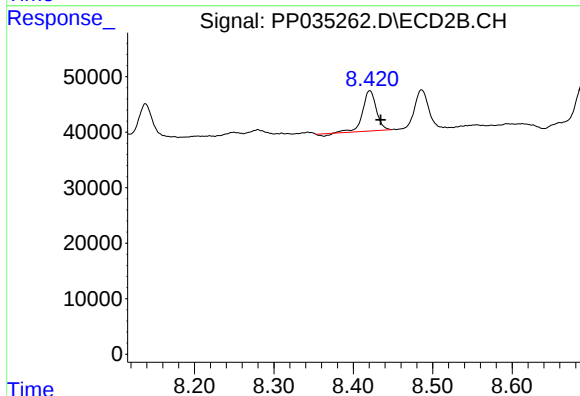


#41 AR-1268-1

R.T.: 8.421 min
Delta R.T.: -0.014 min
Response: 84768
Conc: 23.98 ng/ml

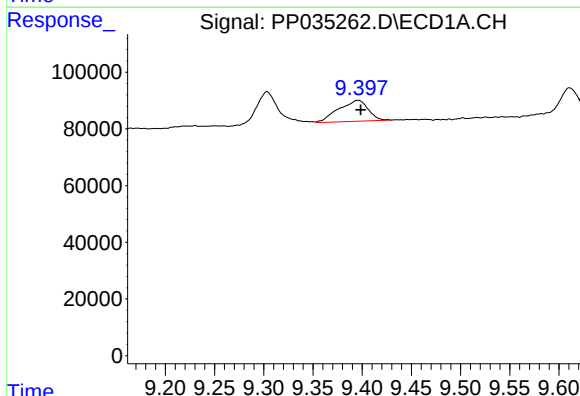


#42 AR-1268-2

R.T.: 9.396 min
Delta R.T.: -0.003 min
Response: 155822
Conc: 19.50 ng/ml

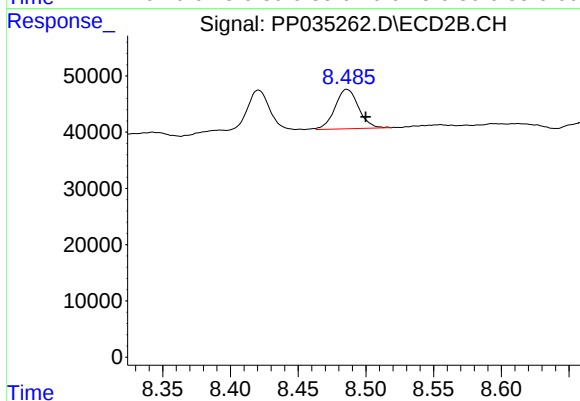

#42 AR-1268-2

R.T.: 8.486 min
Delta R.T.: -0.014 min
Response: 84994
Conc: 25.13 ng/ml

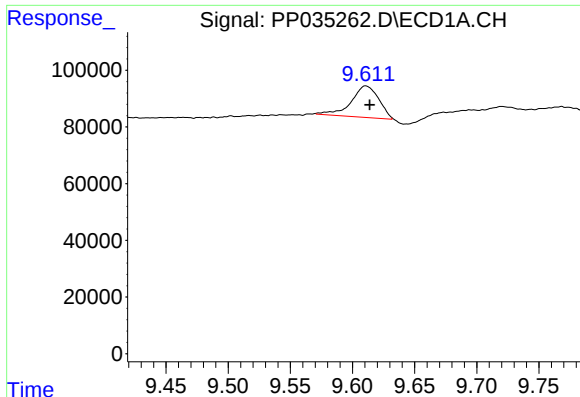


#43 AR-1268-3

R.T.: 9.611 min
Delta R.T.: -0.003 min
Response: 171020
Conc: 22.43 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SB-36-10.5-11.0


Manual Integrations
APPROVED

Ankita
4/27/2021 10:55:08 AM

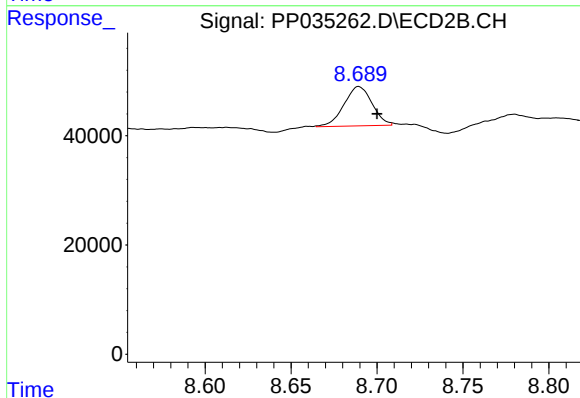


#43 AR-1268-3

R.T.: 8.689 min
Delta R.T.: -0.011 min
Response: 82187
Conc: 26.51 ng/ml m

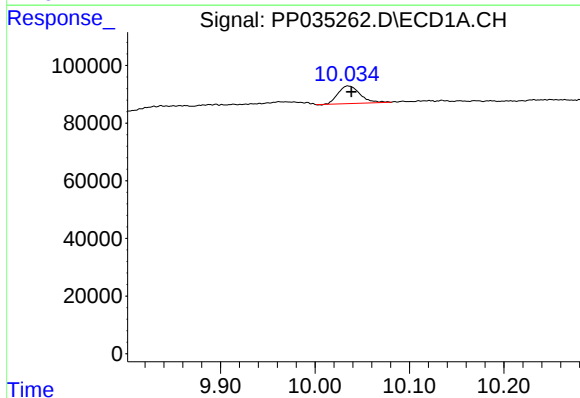


#44 AR-1268-4

R.T.: 10.035 min
Delta R.T.: -0.004 min
Response: 99149
Conc: 41.48 ng/ml

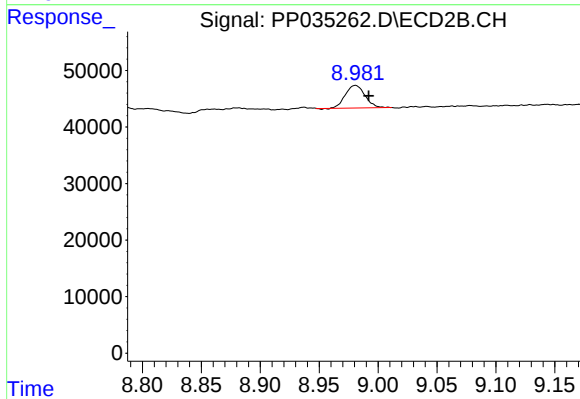

#44 AR-1268-4

R.T.: 8.981 min
Delta R.T.: -0.011 min
Response: 46674
Conc: 44.27 ng/ml

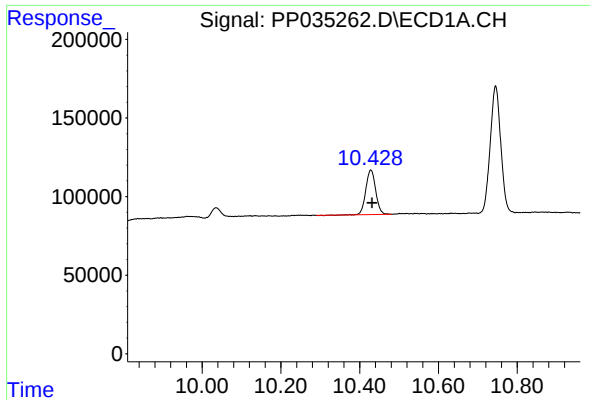


#45 AR-1268-5

R.T.: 10.428 min
Delta R.T.: -0.003 min
Response: 494012
Conc: 22.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-36-10.5-11.0

Manual Integrations
APPROVED

Ankita
4/27/2021 10:55:08 AM

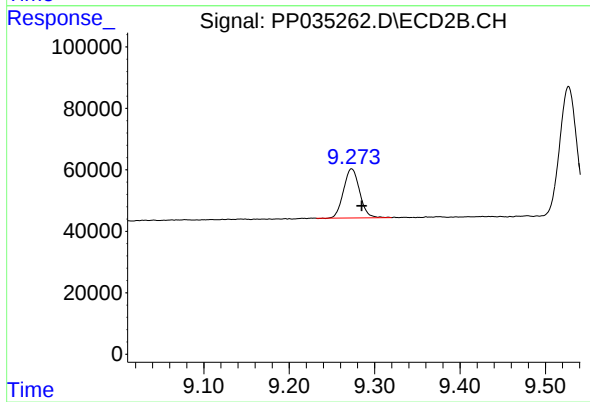

#45 AR-1268-5

R.T.: 9.273 min
Delta R.T.: -0.012 min
Response: 209580
Conc: 26.95 ng/ml