

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042424\
 Data File : PP064521.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2024 14:37
 Operator : YP\AJ
 Sample : P2246-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SAW-CUTTING-LIQUID

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/25/2024
 Supervised By :Ankita Jodhani 04/25/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 15:06:33 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042324.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 24 05:09:39 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.481	3.632	45518981	31929397	13.126m	12.901
2) SA Decachlor...	10.343	8.661	32866693	29331852	12.931	11.960
Target Compounds						
31) L7 AR-1260-1	7.281	6.212	1779692	1707718	13.260	13.803
32) L7 AR-1260-2	7.540	6.401	2550466	1941224	17.513	13.565
33) L7 AR-1260-3	7.903	6.555	3092039	2081572	26.892	15.215 #
34) L7 AR-1260-4	8.130	7.028	2175956	1930807	17.112m	16.699
35) L7 AR-1260-5	8.459	7.271	3786227	3480045	16.672	14.086

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042424\
Data File : PP064521.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2024 14:37
Operator : YP\AJ
Sample : P2246-03
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SAW-CUTTING-LIQUID


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/25/2024
Supervised By :Ankita Jodhani 04/25/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 15:06:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042324.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 24 05:09:39 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

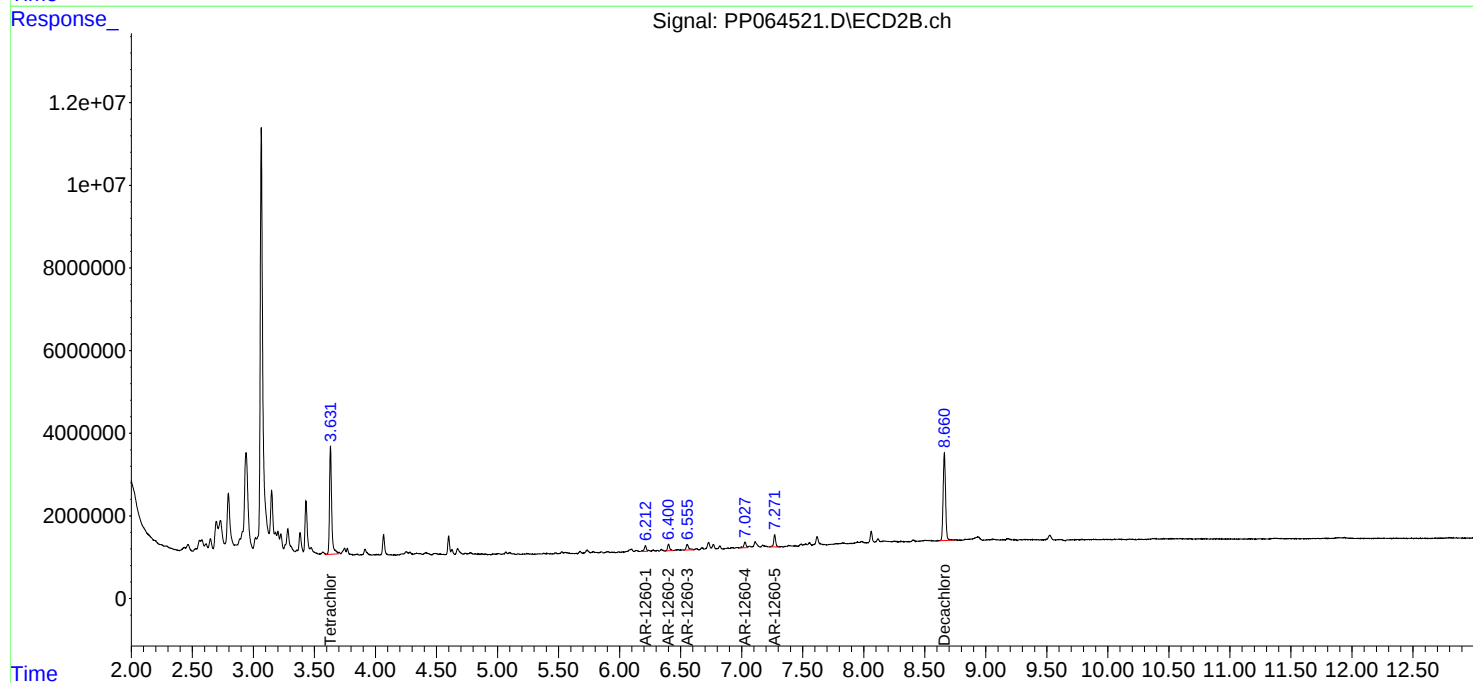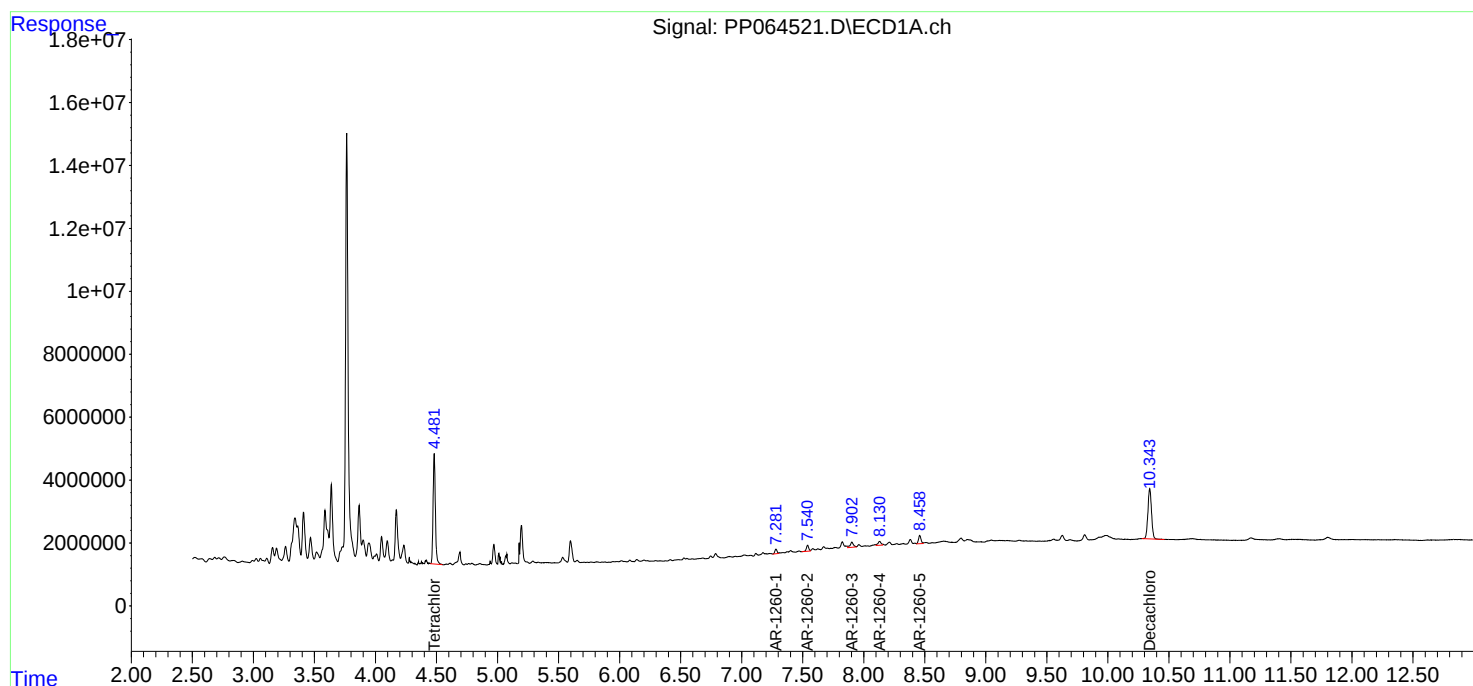

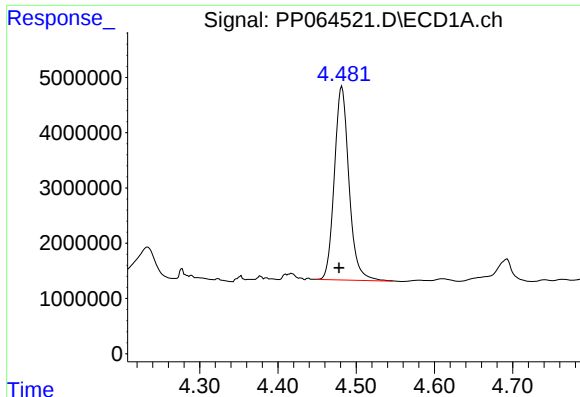


#1 Tetrachloro-m-xylene

R.T.: 4.481 min
Delta R.T.: 0.003 min
Response: 45518981
Conc: 13.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
SAW-CUTTING-LIQUID


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/25/2024
Supervised By :Ankita Jodhani 04/25/2024

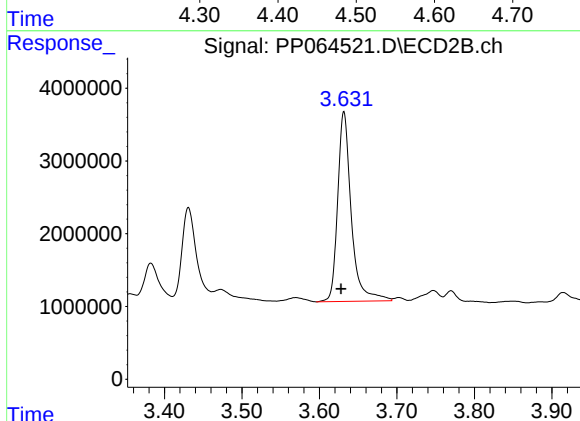


#1 Tetrachloro-m-xylene

R.T.: 3.632 min
Delta R.T.: 0.004 min
Response: 31929397
Conc: 12.90 ng/ml

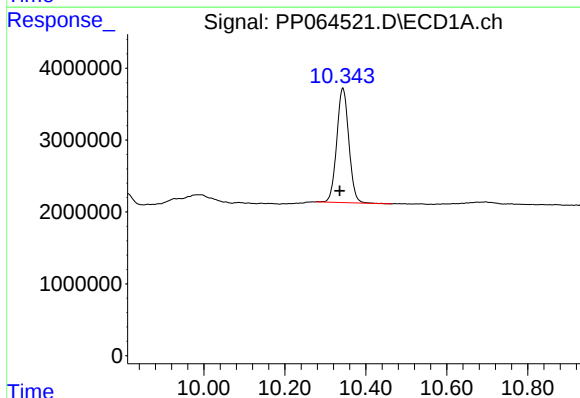


#2 Decachlorobiphenyl

R.T.: 10.343 min
Delta R.T.: 0.008 min
Response: 32866693
Conc: 12.93 ng/ml

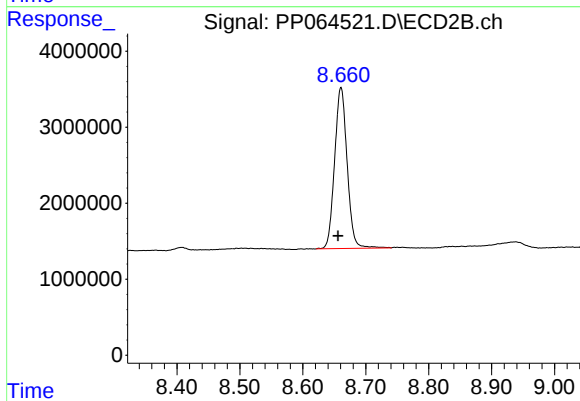

#2 Decachlorobiphenyl

R.T.: 8.661 min
Delta R.T.: 0.005 min
Response: 29331852
Conc: 11.96 ng/ml

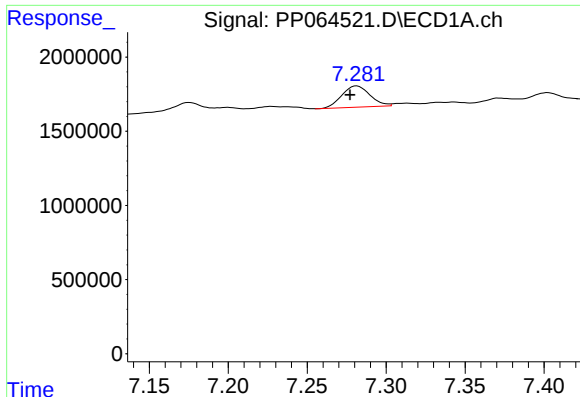


#31 AR-1260-1

R.T.: 7.281 min
Delta R.T.: 0.004 min
Response: 1779692
Conc: 13.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
SAW-CUTTING-LIQUID


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/25/2024
Supervised By :Ankita Jodhani 04/25/2024

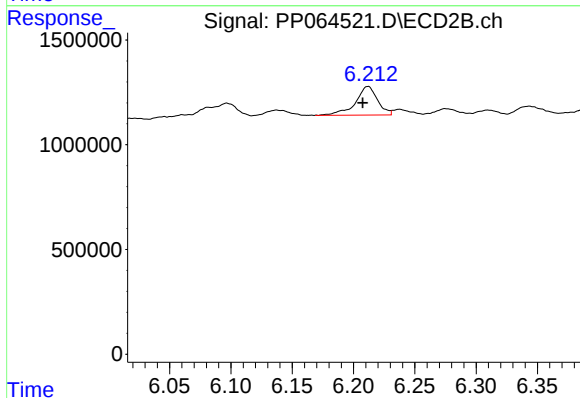


#31 AR-1260-1

R.T.: 6.212 min
Delta R.T.: 0.004 min
Response: 1707718
Conc: 13.80 ng/ml

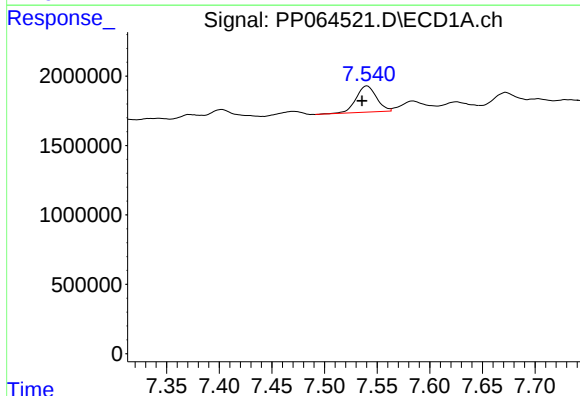


#32 AR-1260-2

R.T.: 7.540 min
Delta R.T.: 0.005 min
Response: 2550466
Conc: 17.51 ng/ml

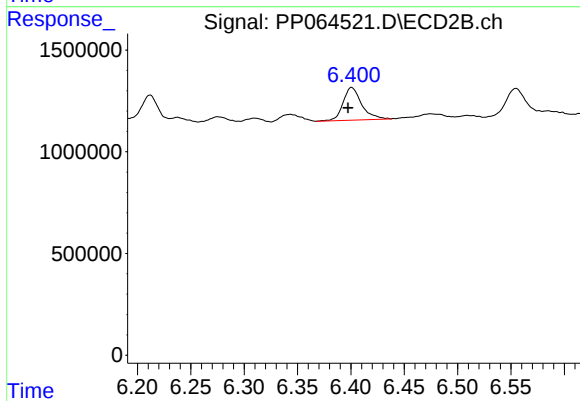

#32 AR-1260-2

R.T.: 6.401 min
Delta R.T.: 0.003 min
Response: 1941224
Conc: 13.57 ng/ml

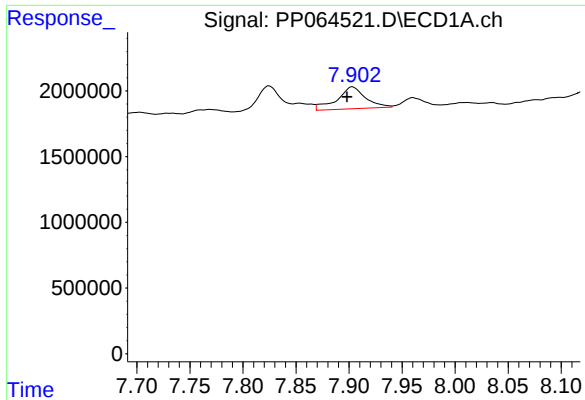


#33 AR-1260-3

R.T.: 7.903 min
Delta R.T.: 0.005 min
Response: 3092039
Conc: 26.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
SAW-CUTTING-LIQUID


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/25/2024
Supervised By :Ankita Jodhani 04/25/2024

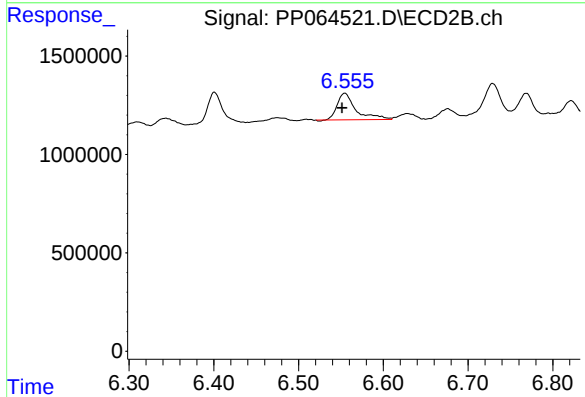


#33 AR-1260-3

R.T.: 6.555 min
Delta R.T.: 0.003 min
Response: 2081572
Conc: 15.22 ng/ml

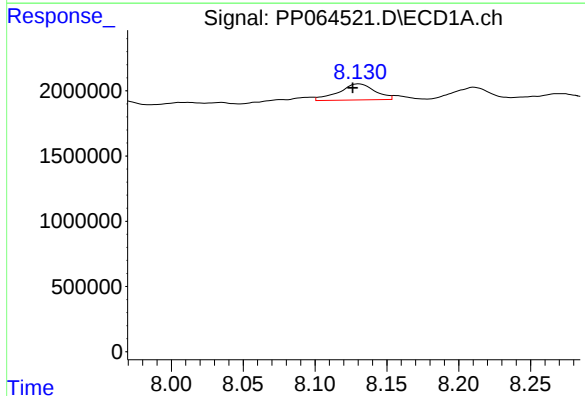


#34 AR-1260-4

R.T.: 8.130 min
Delta R.T.: 0.003 min
Response: 2175956
Conc: 17.11 ng/ml m

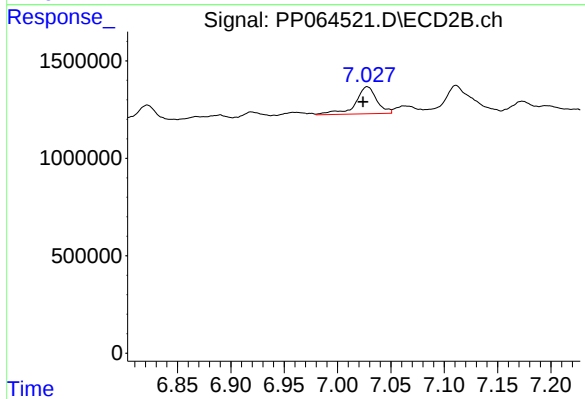

#34 AR-1260-4

R.T.: 7.028 min
Delta R.T.: 0.004 min
Response: 1930807
Conc: 16.70 ng/ml

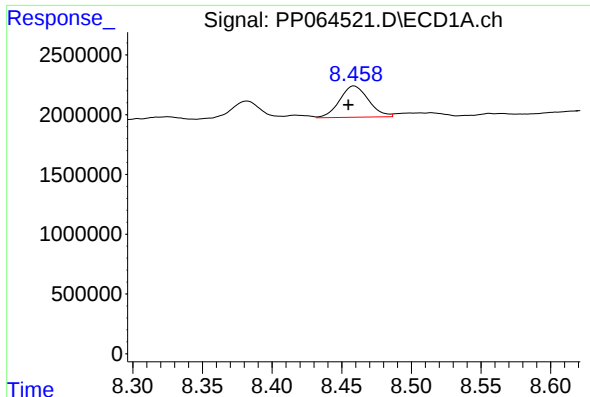


#35 AR-1260-5

R.T.: 8.459 min
Delta R.T.: 0.004 min
Response: 3786227
Conc: 16.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
SAW-CUTTING-LIQUID

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/25/2024
Supervised By :Ankita Jodhani 04/25/2024

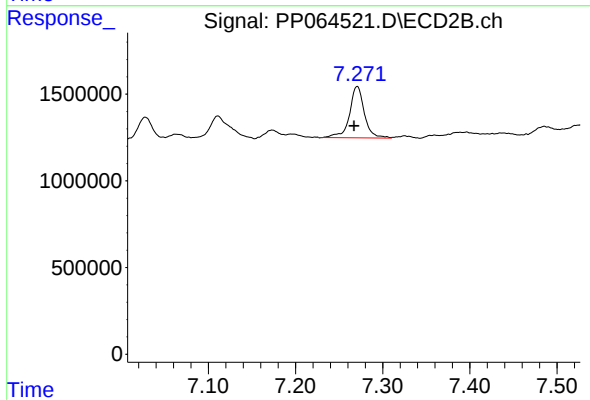

#35 AR-1260-5

R.T.: 7.271 min
Delta R.T.: 0.004 min
Response: 3480045
Conc: 14.09 ng/ml