

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042519\
 Data File : PP029991.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Apr 2019 11:49
 Operator : EI/SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 10:04:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042519.M
 Quant Title : 8080.M
 QLast Update : Fri Apr 26 10:04:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
9) T	2,4-D	14.058	0.000	788.8E6	0	1652.862	N.D. #
15) T	Picloram	17.799	18.383	1810000	2504013	0.511	0.930 #
16) T	DCPA	18.372	18.249	1510745	388465	0.425	0.143 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042519\
Data File : PP029991.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Apr 2019 11:49
Operator : EI/SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 10:04:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042519.M
Quant Title : 8080.M
QLast Update : Fri Apr 26 10:04:13 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

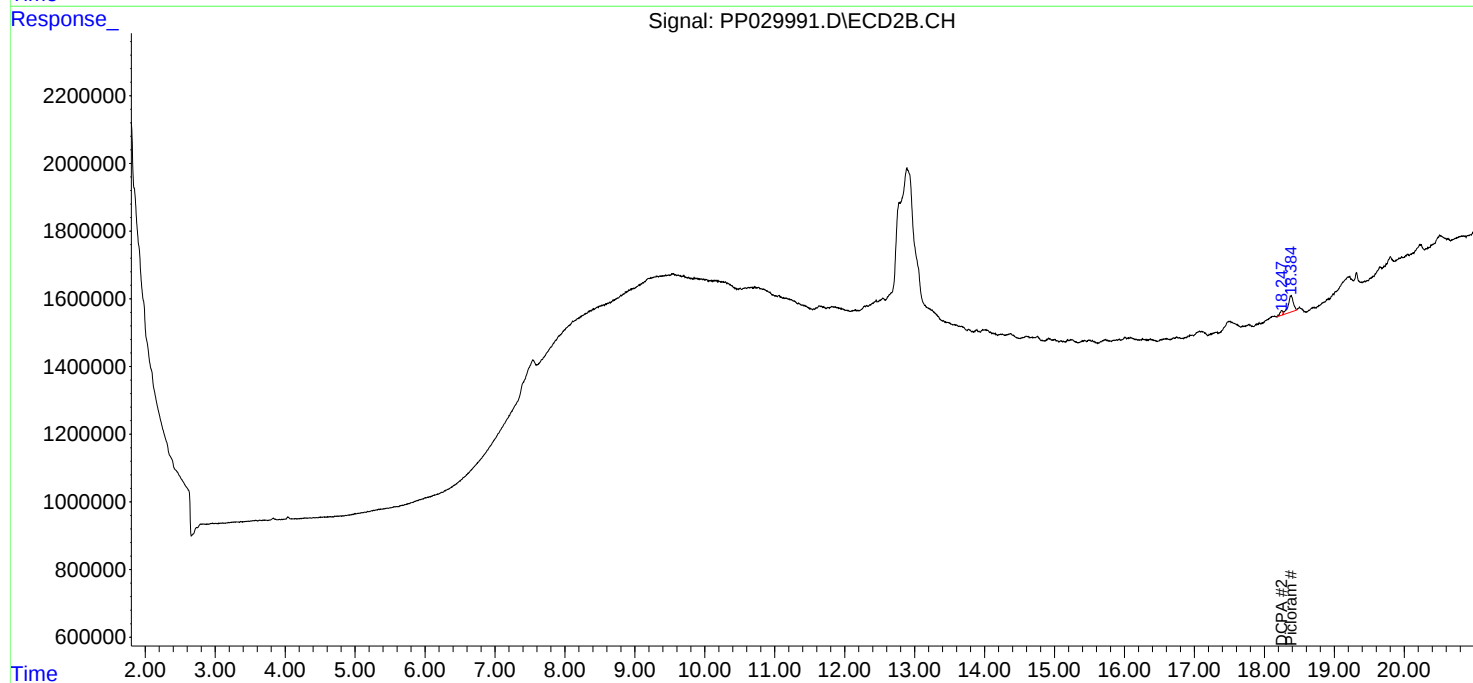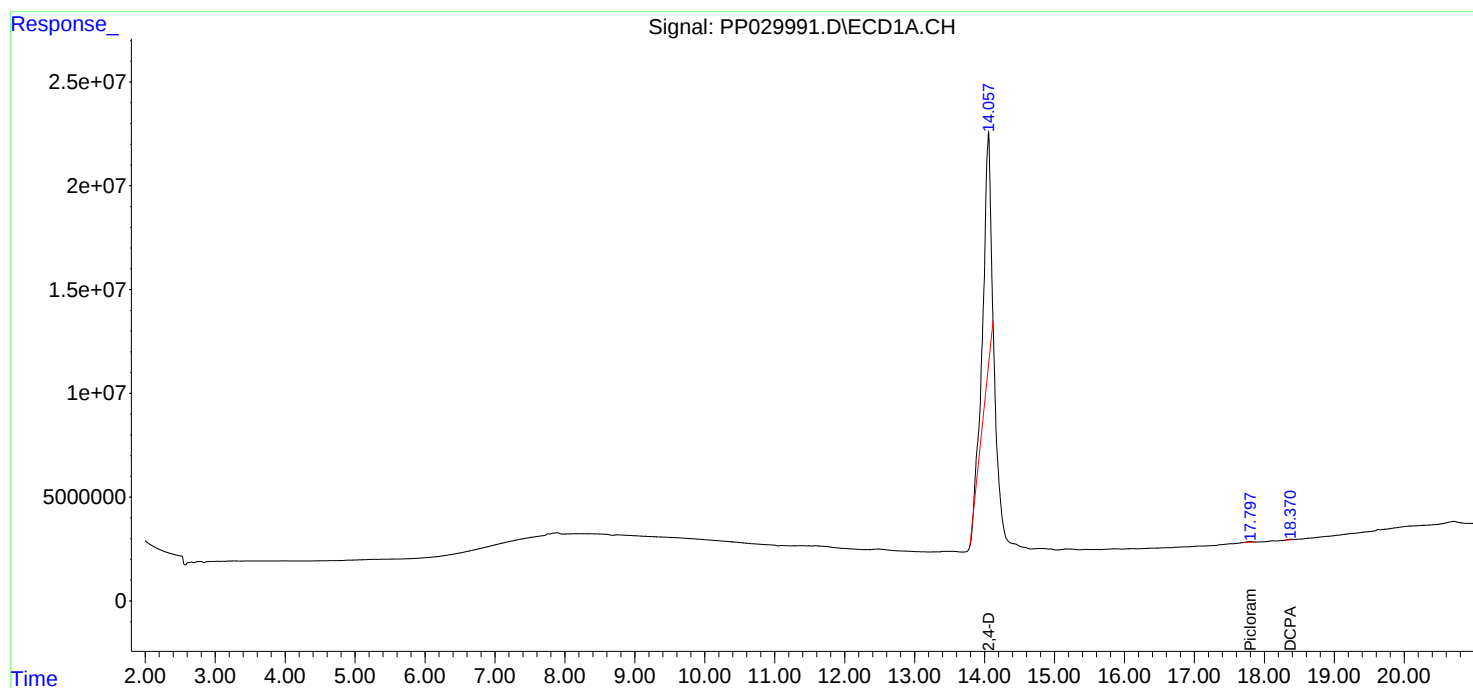


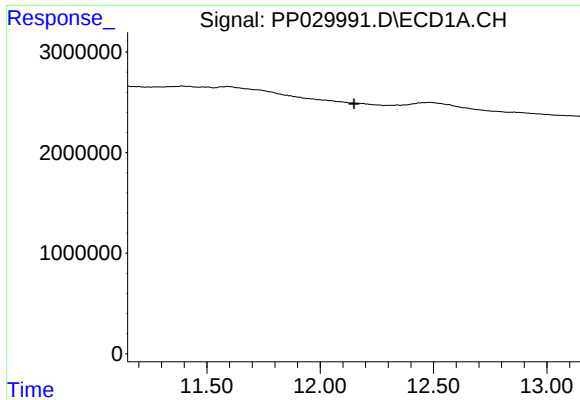

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 12.149 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

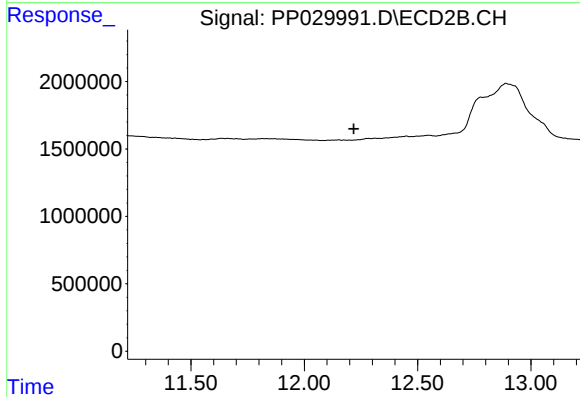


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 12.219 min
Response: 0
Conc: N.D.

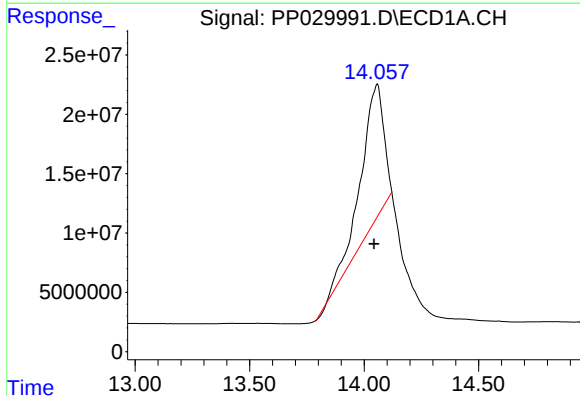


#9 2,4-D

R.T.: 14.058 min
Delta R.T.: 0.014 min
Response: 788816451
Conc: 1652.86 ng/ml

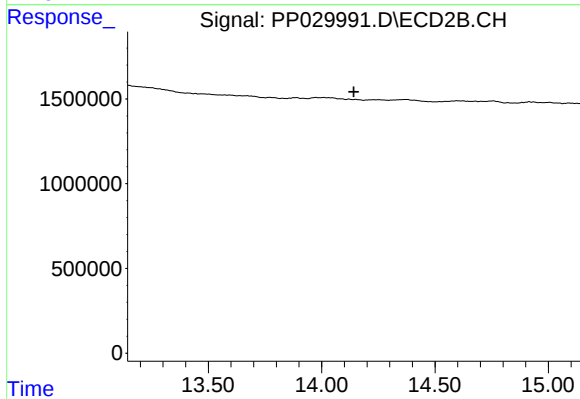

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 14.142 min
Response: 0
Conc: N.D.

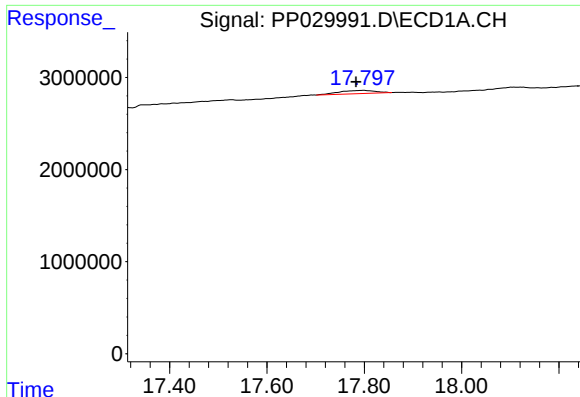

#15 Picloram


R.T.: 17.799 min
Delta R.T.: 0.016 min
Response: 1810000
Conc: 0.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

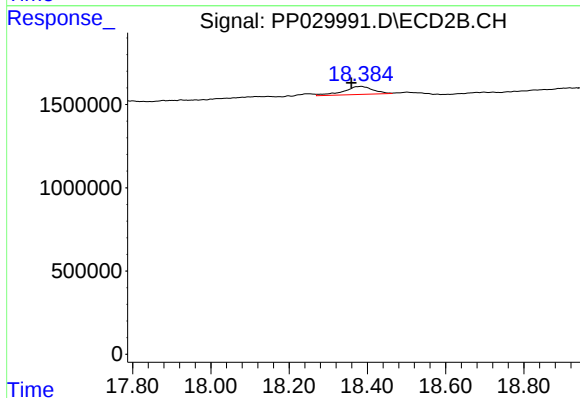


#15 Picloram

R.T.: 18.383 min
Delta R.T.: 0.024 min
Response: 2504013
Conc: 0.93 ng/ml

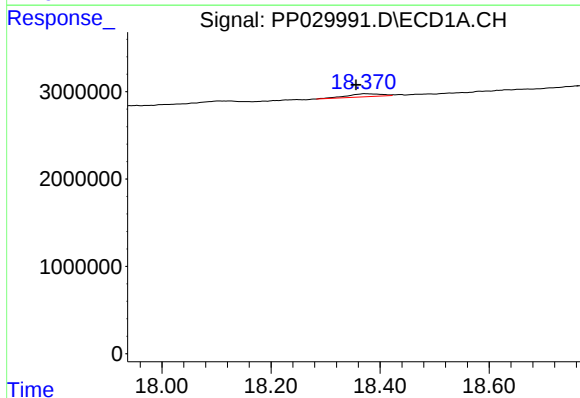

#16 DCPA

R.T.: 18.372 min
Delta R.T.: 0.016 min
Response: 1510745
Conc: 0.42 ng/ml

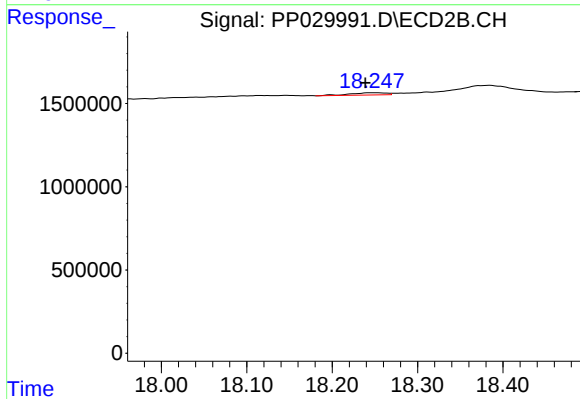

#16 DCPA

R.T.: 18.249 min
Delta R.T.: 0.010 min
Response: 388465
Conc: 0.14 ng/ml