

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042519\
 Data File : PP030012.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Apr 2019 3:09
 Operator : EI/SJ
 Sample : MDL-BL-WATER-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-BL-WATER-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 10:21:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042519.M
 Quant Title : 8080.M
 QLast Update : Fri Apr 26 10:04:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	12.148	12.219	262.4E6	186.0E6	590.136	464.500
Target Compounds							
7) T	MCPA	0.000	13.044	0	649382	N.D.	0.526 #
15) T	Picloram	17.808	18.399	1393867	789155	0.393	0.293 #
16) T	DCPA	18.356	18.243	394538	459299	0.111	0.169 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042519\
Data File : PP030012.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Apr 2019 3:09
Operator : EI/SJ
Sample : MDL-BL-WATER-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-BL-WATER-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 10:21:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042519.M
Quant Title : 8080.M
QLast Update : Fri Apr 26 10:04:13 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

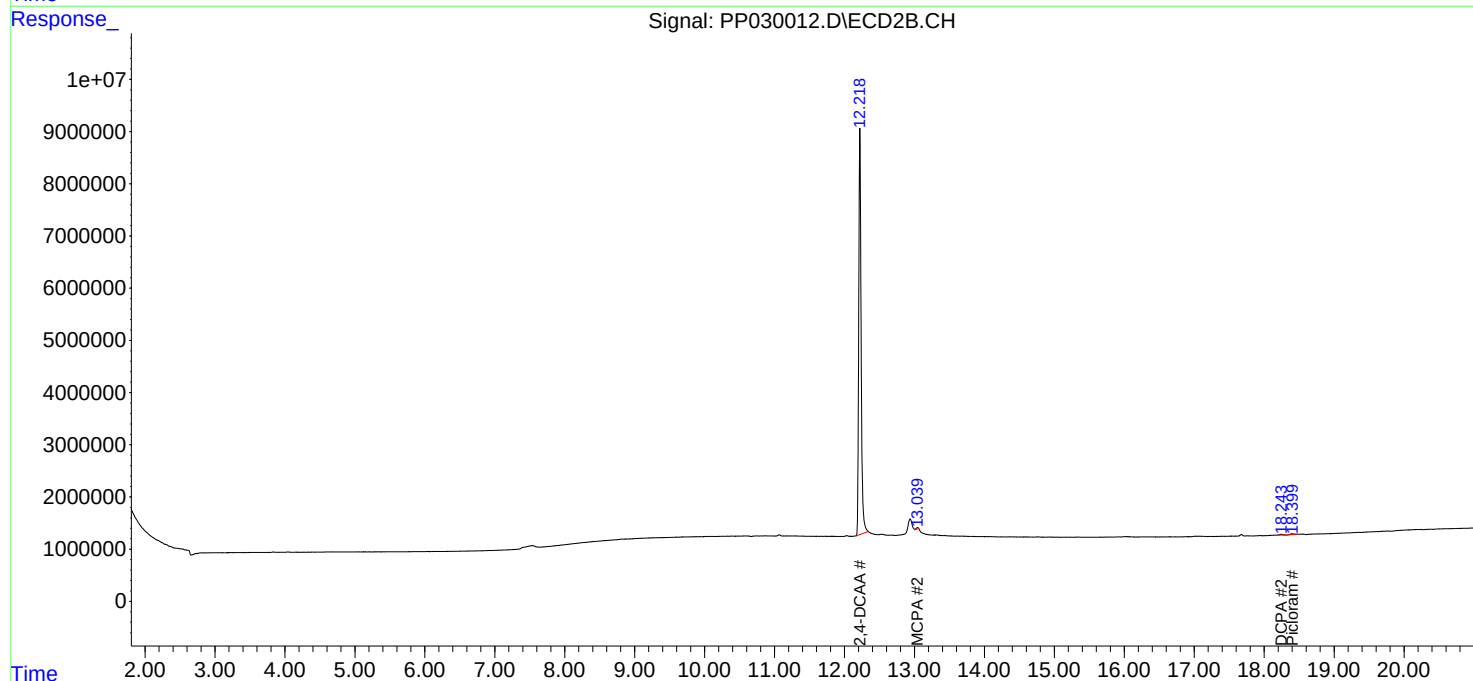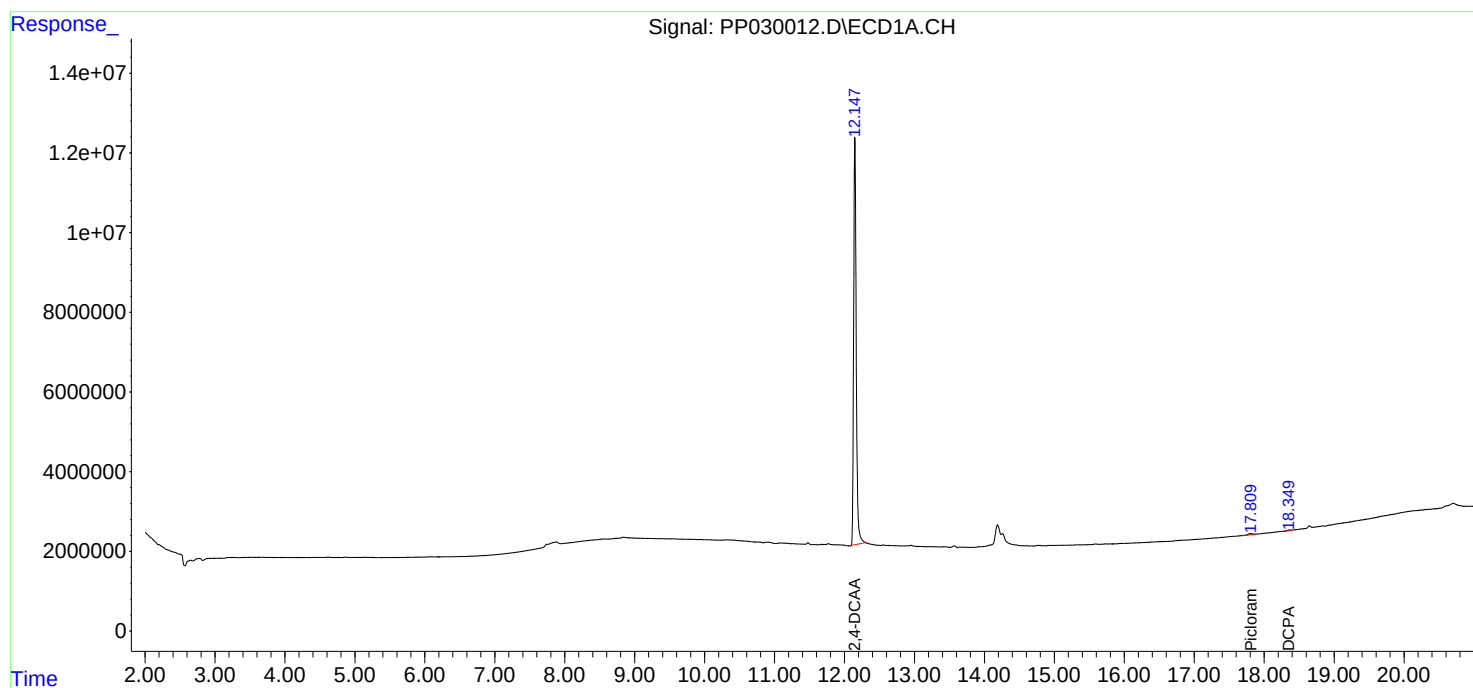


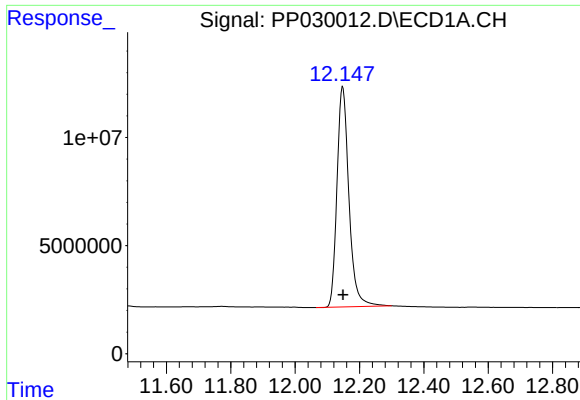

#4 2,4-DCAA


R.T.: 12.148 min
Delta R.T.: -0.001 min
Response: 262430414
Conc: 590.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-BL-WATER-01

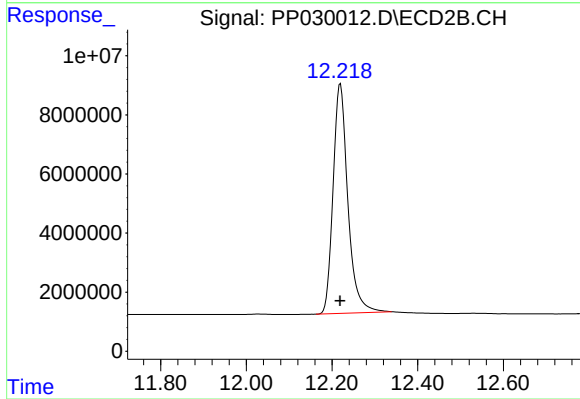


#4 2,4-DCAA

R.T.: 12.219 min
Delta R.T.: 0.000 min
Response: 185956189
Conc: 464.50 ng/ml

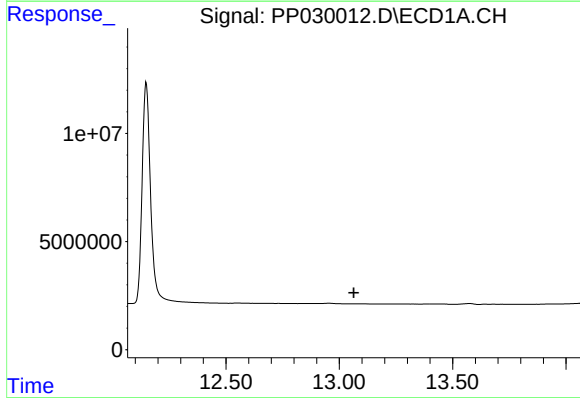


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 13.064 min
Response: 0
Conc: N.D.

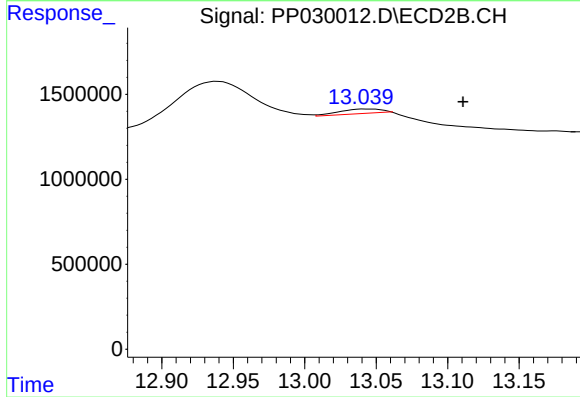

#7 MCPA


R.T.: 13.044 min
Delta R.T.: -0.066 min
Response: 649382
Conc: 0.53 ug/ml

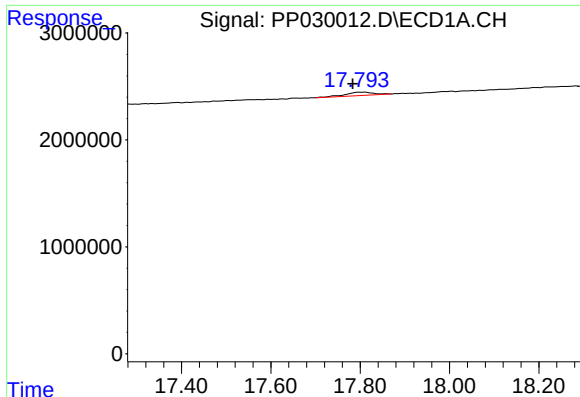

#15 Picloram


R.T.: 17.808 min
Delta R.T.: 0.025 min
Response: 1393867
Conc: 0.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-BL-WATER-01

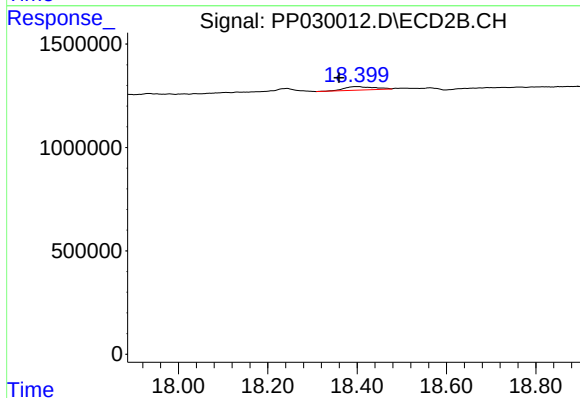


#15 Picloram

R.T.: 18.399 min
Delta R.T.: 0.040 min
Response: 789155
Conc: 0.29 ng/ml

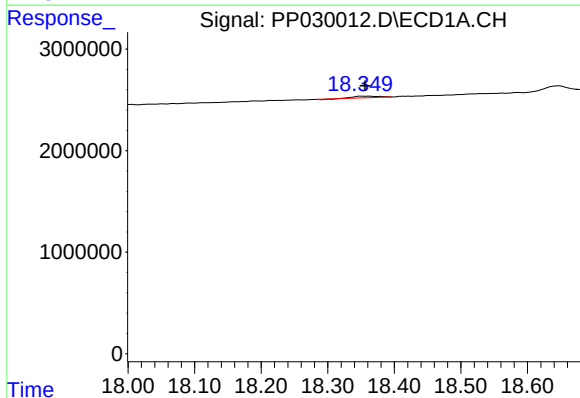

#16 DCPA

R.T.: 18.356 min
Delta R.T.: 0.000 min
Response: 394538
Conc: 0.11 ng/ml

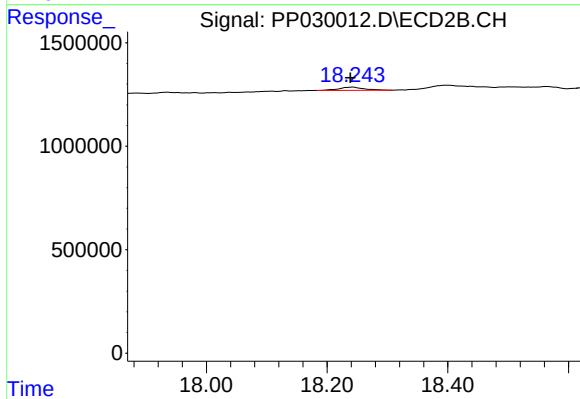

#16 DCPA

R.T.: 18.243 min
Delta R.T.: 0.005 min
Response: 459299
Conc: 0.17 ng/ml