

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042519\
 Data File : PP030013.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Apr 2019 3:34
 Operator : EI/SJ
 Sample : MDL-BL-WATER-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-BL-WATER-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 10:21:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042519.M
 Quant Title : 8080.M
 QLast Update : Fri Apr 26 10:04:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	12.150	12.222	160.4E6	109.7E6	360.585	274.049
Target Compounds							
7) T	MCPA	0.000	13.041	0	374701	N.D.	0.304 #
15) T	Picloram	17.810	18.422	515161	304635	0.145	0.113



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042519\
Data File : PP030013.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Apr 2019 3:34
Operator : EI/SJ
Sample : MDL-BL-WATER-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-BL-WATER-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 10:21:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042519.M
Quant Title : 8080.M
QLast Update : Fri Apr 26 10:04:13 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

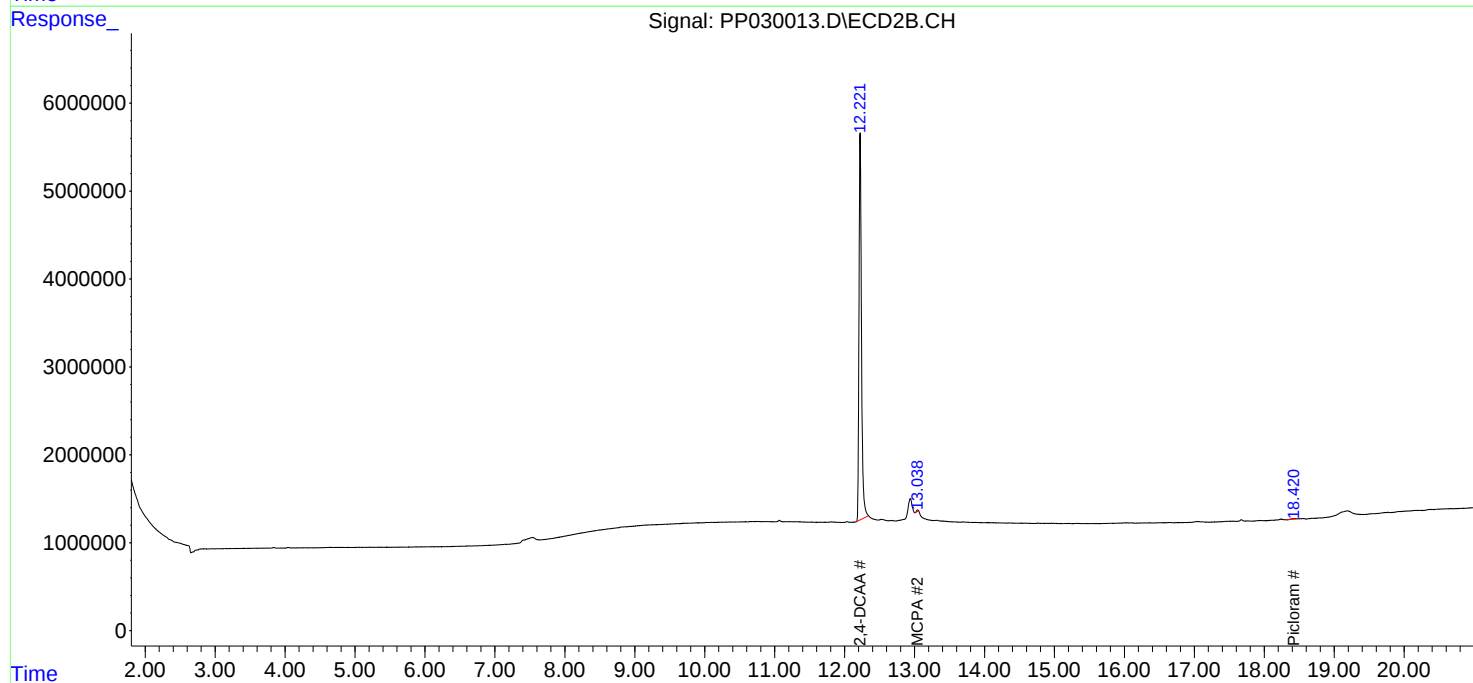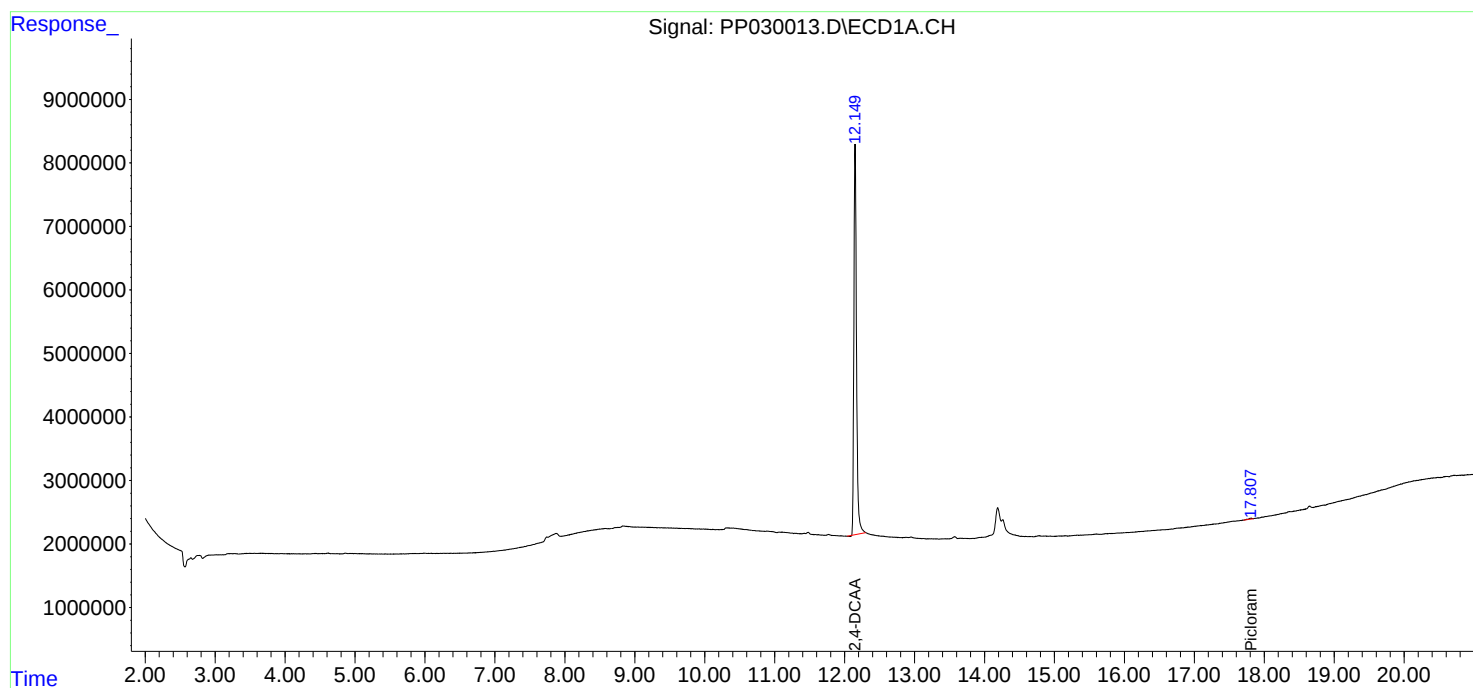


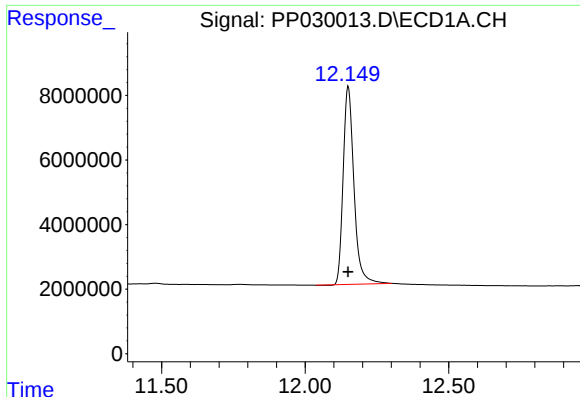

#4 2,4-DCAA


R.T.: 12.150 min
Delta R.T.: 0.000 min
Response: 160350557
Conc: 360.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-BL-WATER-02

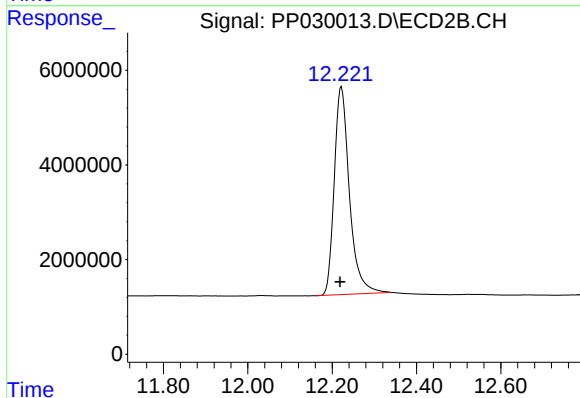


#4 2,4-DCAA

R.T.: 12.222 min
Delta R.T.: 0.003 min
Response: 109711891
Conc: 274.05 ng/ml

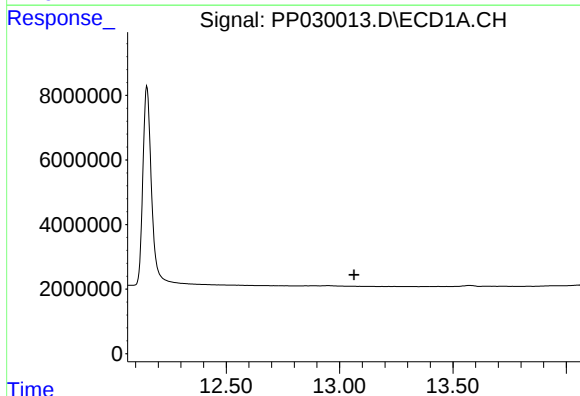


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 13.064 min
Response: 0
Conc: N.D.

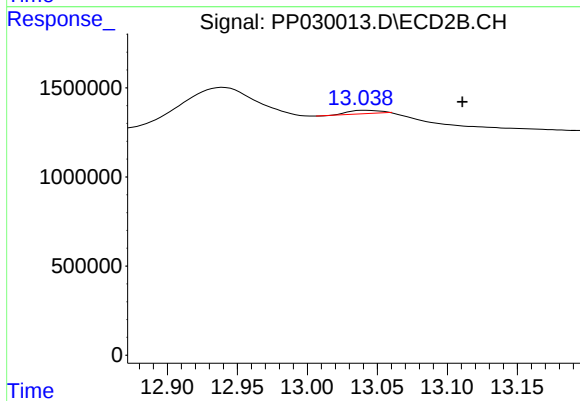

#7 MCPA


R.T.: 13.041 min
Delta R.T.: -0.069 min
Response: 374701
Conc: 0.30 ug/ml

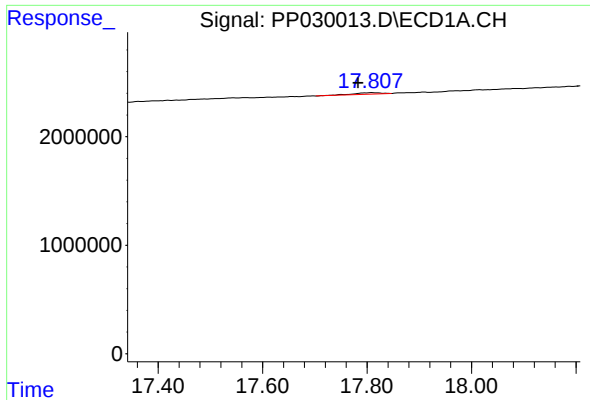

#15 Picloram

R.T.: 17.810 min
Delta R.T.: 0.027 min
Response: 515161
Conc: 0.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-BL-WATER-02

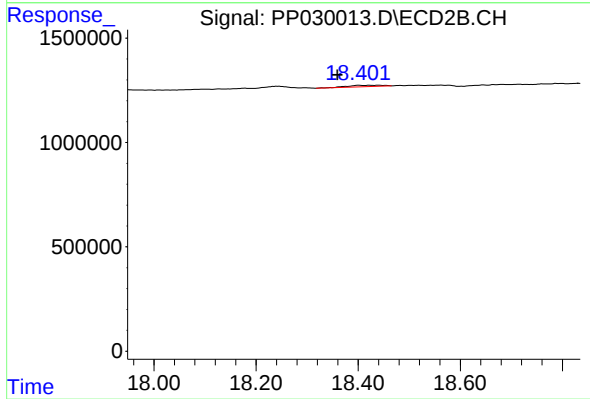

#15 Picloram

R.T.: 18.422 min
Delta R.T.: 0.062 min
Response: 304635
Conc: 0.11 ng/ml