

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042522\
 Data File : PP046604.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Apr 2022 14:56
 Operator : YP\AJ
 Sample : N2514-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WC-16-1A-5

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/26/2022
 Supervised By :mohammad ahmed 04/26/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 17:13:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 22 19:00:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.866	3.136	37626536	68710808	15.587m	20.946 #
2) SA Decachlor...	9.956	8.461	29186517	45579590	19.834	19.108

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042522\
Data File : PP046604.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Apr 2022 14:56
Operator : YP\AJ
Sample : N2514-03
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
WC-16-1A-5


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/26/2022
Supervised By :mohammad ahmed 04/26/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 17:13:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 22 19:00:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

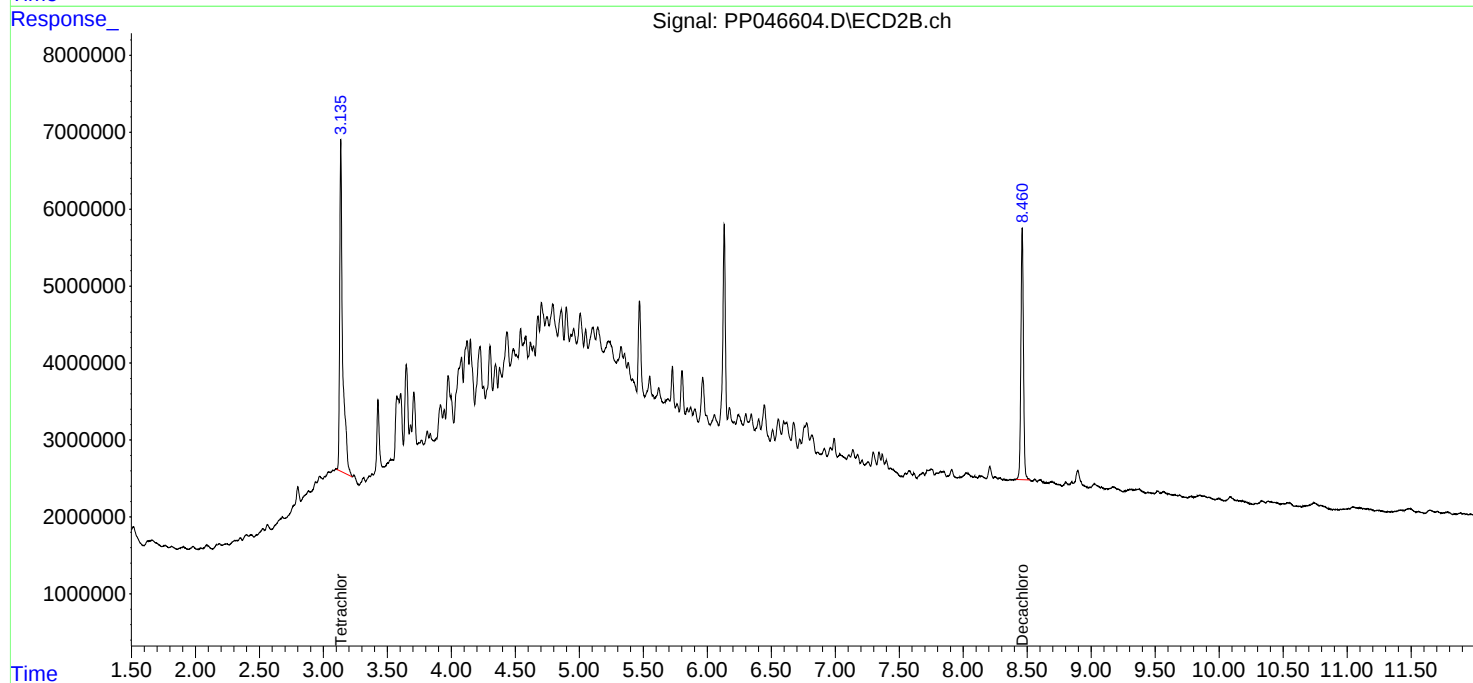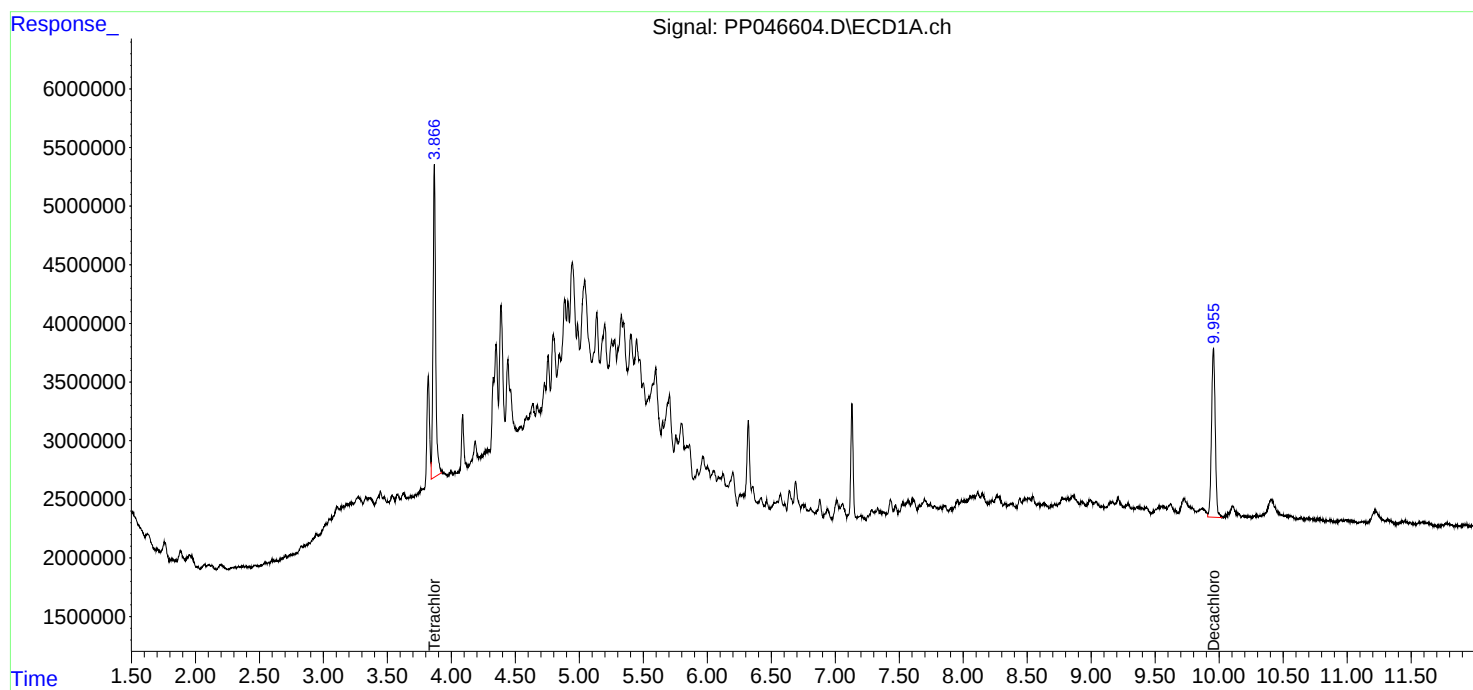

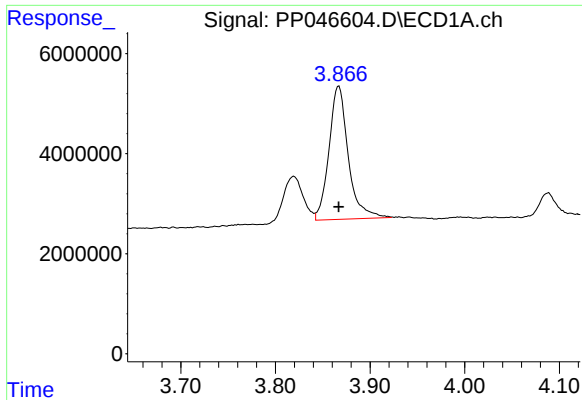


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 37626536
Conc: 15.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
WC-16-1A-5


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/26/2022
Supervised By :mohammad ahmed 04/26/2022

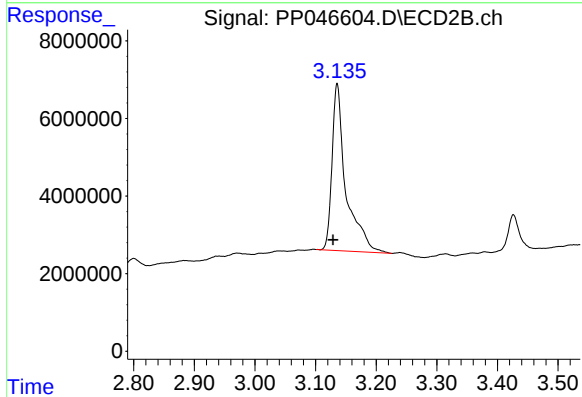


#1 Tetrachloro-m-xylene

R.T.: 3.136 min
Delta R.T.: 0.007 min
Response: 68710808
Conc: 20.95 ng/ml

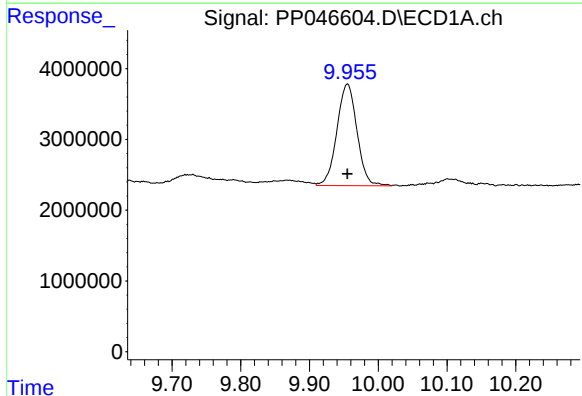

#2 Decachlorobiphenyl

R.T.: 9.956 min
Delta R.T.: 0.000 min
Response: 29186517
Conc: 19.83 ng/ml

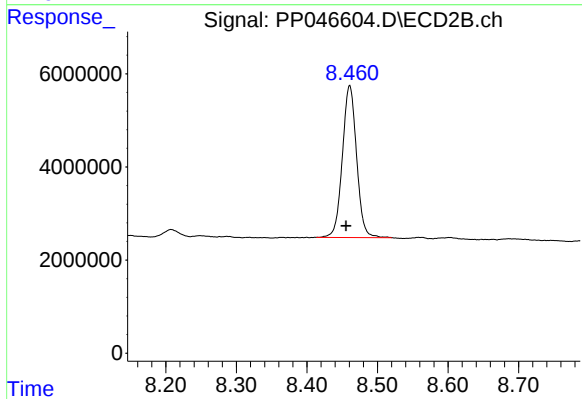

#2 Decachlorobiphenyl

R.T.: 8.461 min
Delta R.T.: 0.005 min
Response: 45579590
Conc: 19.11 ng/ml