

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042522\
Data File : PP046648.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2022 08:47
Operator : YP\AJ
Sample : N2550-01
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PUMP-STATION-207ST-TRAIN-FACILITY

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 11:38:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 22 19:00:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.862	3.127	50777425	74835941	21.035	22.813
2) SA Decachlor...	9.944	8.446	29323071	45375838	19.927	19.023

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042522\
Data File : PP046648.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2022 08:47
Operator : YP\AJ
Sample : N2550-01
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PUMP-STATION-207ST-TRAIN-FACILITY

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 11:38:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 22 19:00:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

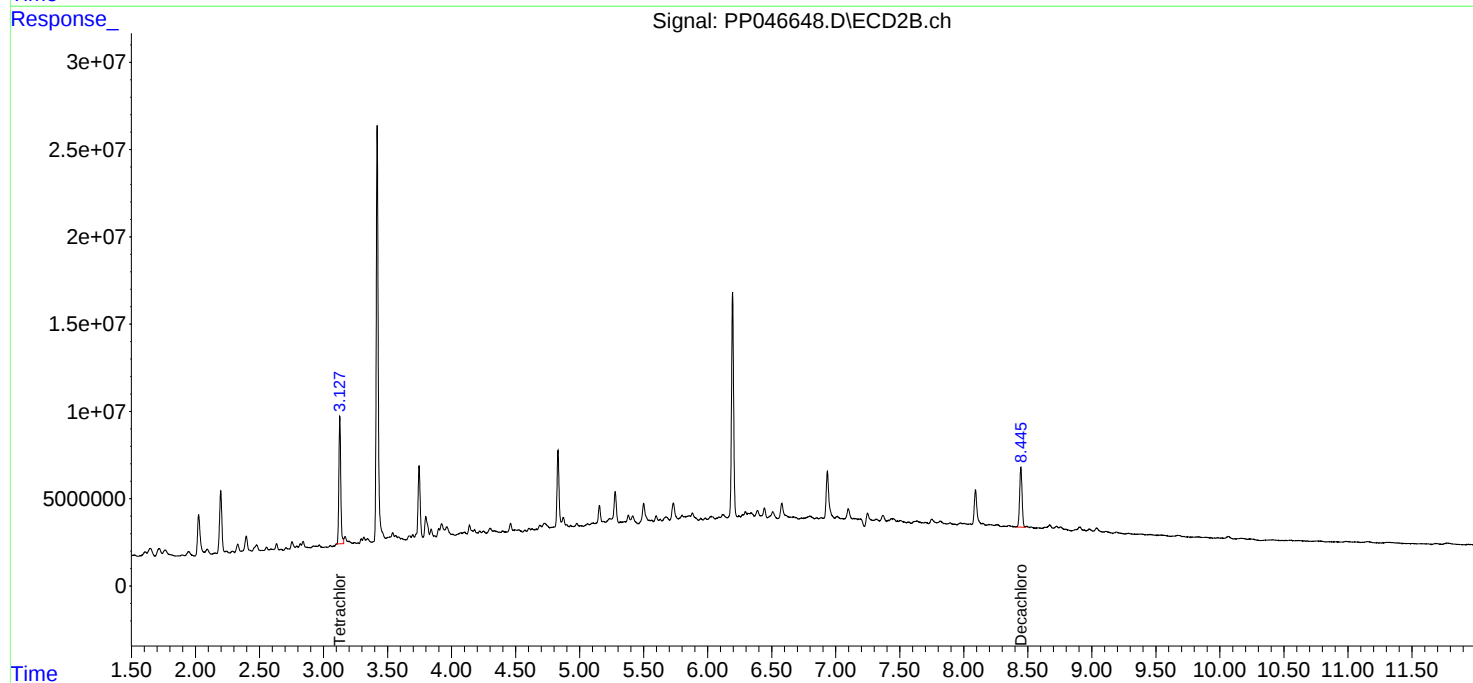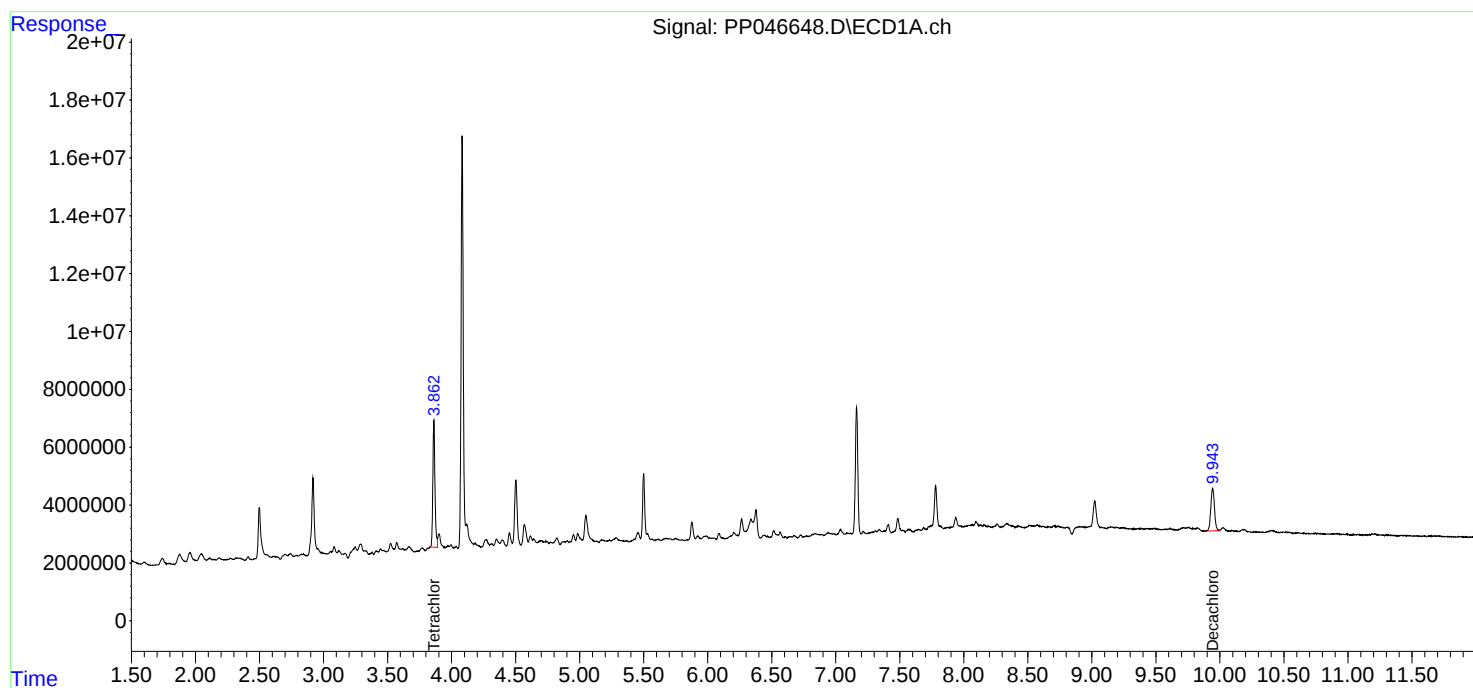


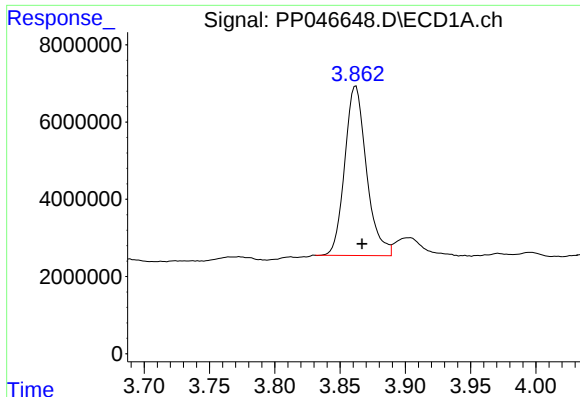

#1 Tetrachloro-m-xylene


R.T.: 3.862 min
Delta R.T.: -0.005 min
Response: 50777425
Conc: 21.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
PUMP-STATION-207ST-TRAIN-FACILITY

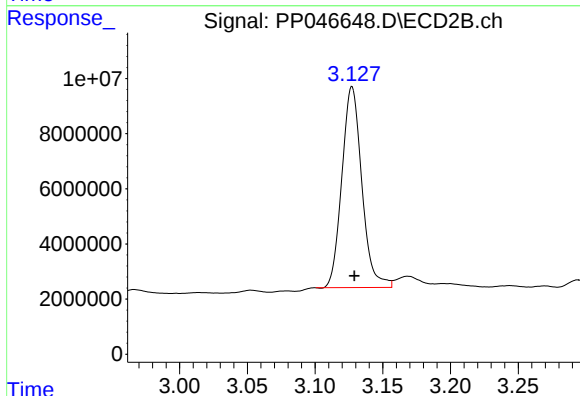


#1 Tetrachloro-m-xylene

R.T.: 3.127 min
Delta R.T.: -0.002 min
Response: 74835941
Conc: 22.81 ng/ml

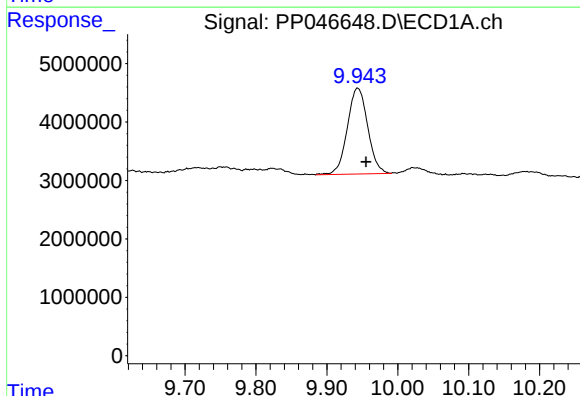

#2 Decachlorobiphenyl

R.T.: 9.944 min
Delta R.T.: -0.012 min
Response: 29323071
Conc: 19.93 ng/ml

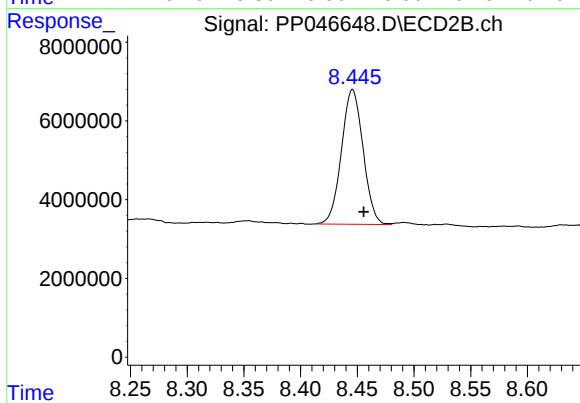

#2 Decachlorobiphenyl

R.T.: 8.446 min
Delta R.T.: -0.010 min
Response: 45375838
Conc: 19.02 ng/ml