

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042522\
 Data File : PP046649.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2022 09:03
 Operator : YP\AJ
 Sample : N2550-02
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DYCKMAN-200ST-A51515T50SB

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/27/2022
 Supervised By :mohammad ahmed 04/27/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 11:39:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 22 19:00:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.862	3.127	46864822	67595516	19.414m	20.606
2) SA Decachlor...	9.944	8.447	30156430	46743579	20.494	19.596

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042522\
Data File : PP046649.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2022 09:03
Operator : YP\AJ
Sample : N2550-02
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
DYCKMAN-200ST-A51515T50SB


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/27/2022
Supervised By :mohammad ahmed 04/27/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 11:39:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 22 19:00:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

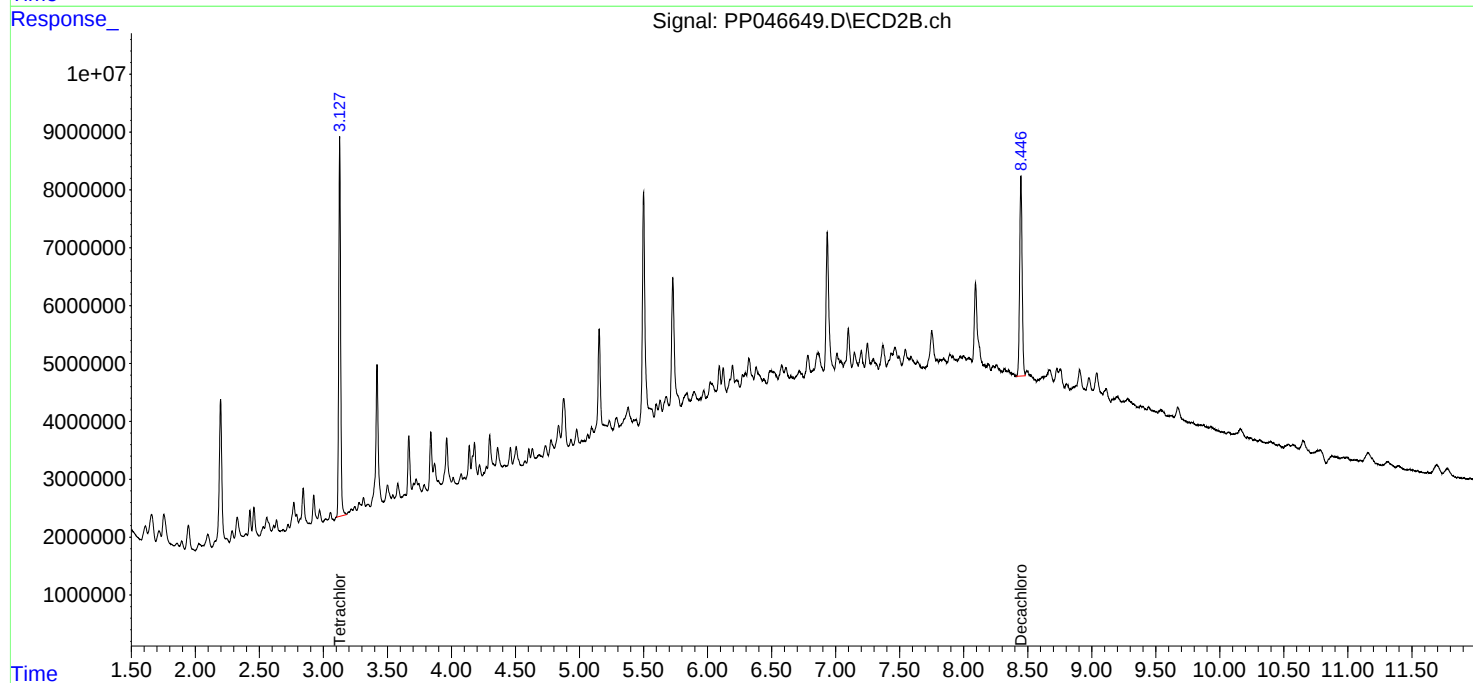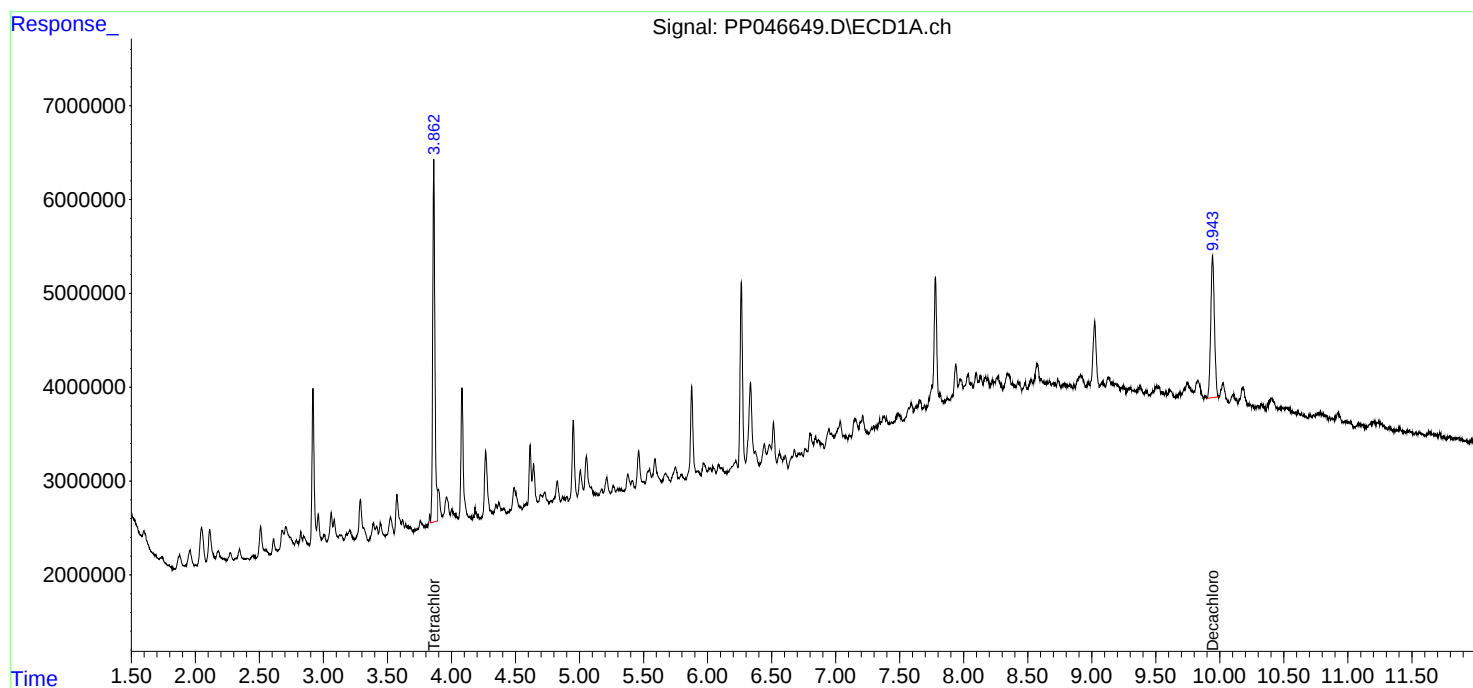

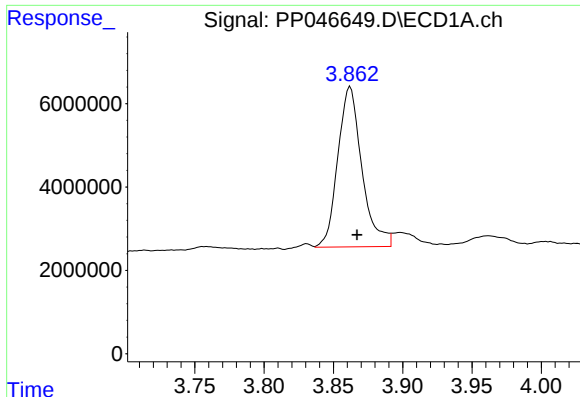


#1 Tetrachloro-m-xylene

R.T.: 3.862 min
Delta R.T.: -0.005 min
Response: 46864822
Conc: 19.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
DYCKMAN-200ST-A51515T50SB


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/27/2022
Supervised By :mohammad ahmed 04/27/2022

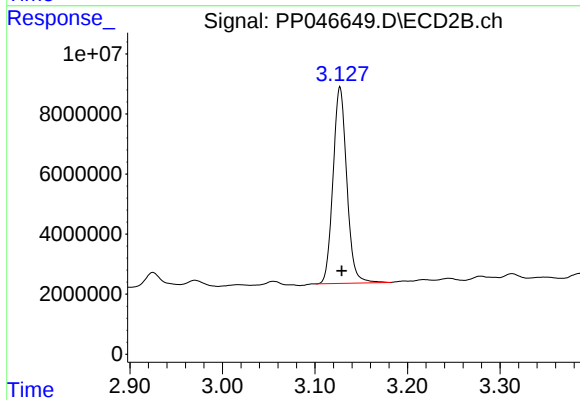


#1 Tetrachloro-m-xylene

R.T.: 3.127 min
Delta R.T.: -0.002 min
Response: 67595516
Conc: 20.61 ng/ml

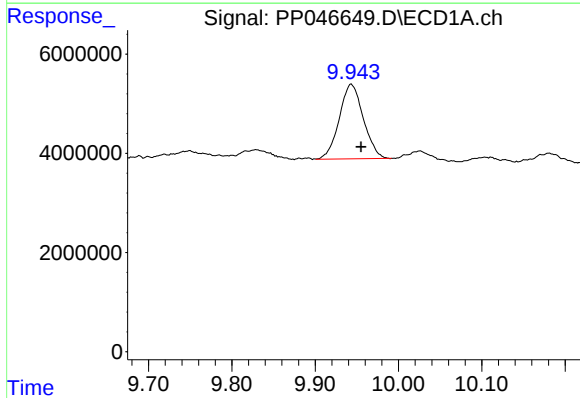

#2 Decachlorobiphenyl

R.T.: 9.944 min
Delta R.T.: -0.012 min
Response: 30156430
Conc: 20.49 ng/ml

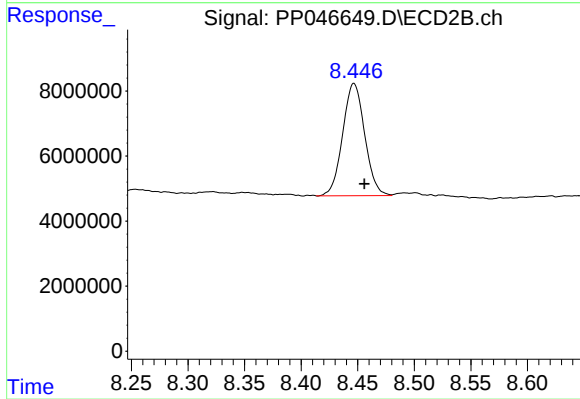

#2 Decachlorobiphenyl

R.T.: 8.447 min
Delta R.T.: -0.009 min
Response: 46743579
Conc: 19.60 ng/ml