

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042523\
 Data File : PP057201.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Apr 2023 13:41
 Operator : YP\AJ
 Sample : 02477-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MID-H4(ELEV-22)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 21:37:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 20 16:59:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.403	3.631	41943819	32938815	18.962	19.498
2) SA Decachlor...	10.218	8.686	28352738	29661355	17.668	16.580

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042523\
Data File : PP057201.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Apr 2023 13:41
Operator : YP\AJ
Sample : 02477-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MID-H4(ELEV-22)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 21:37:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042023.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 20 16:59:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

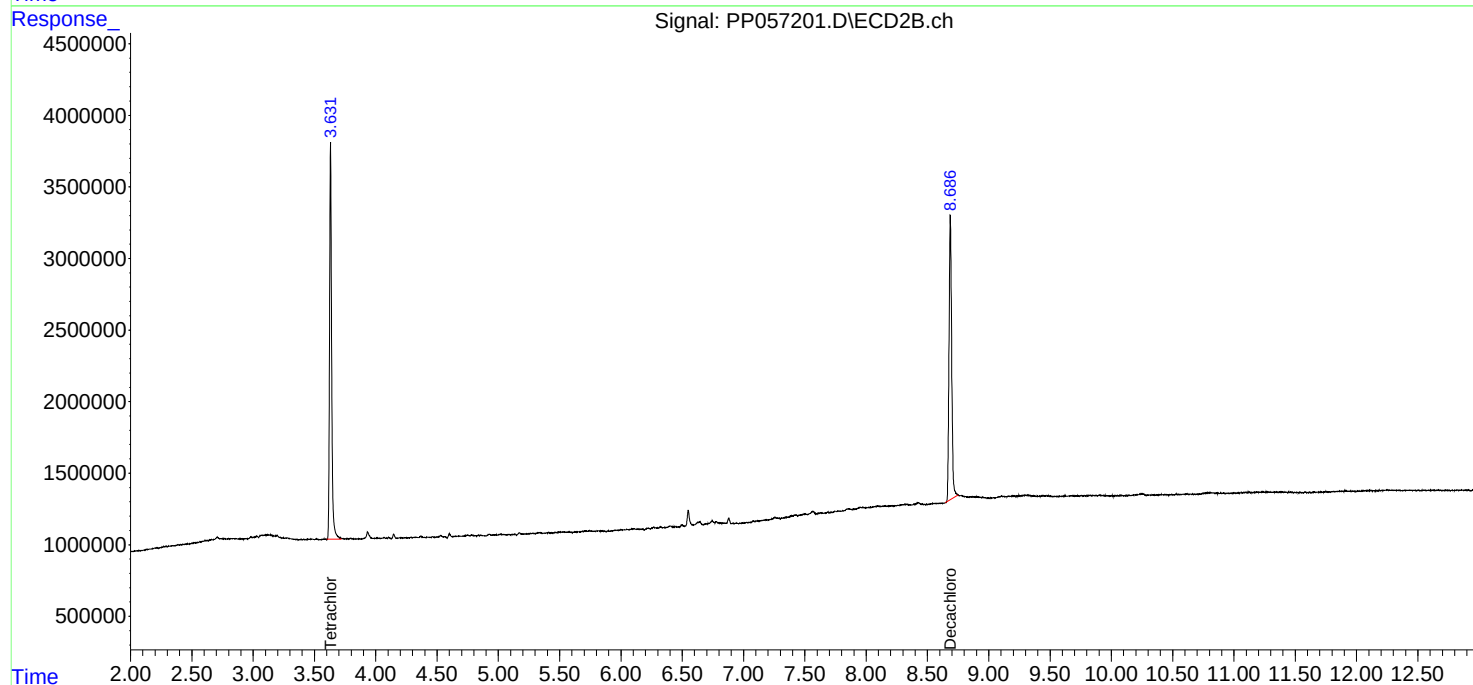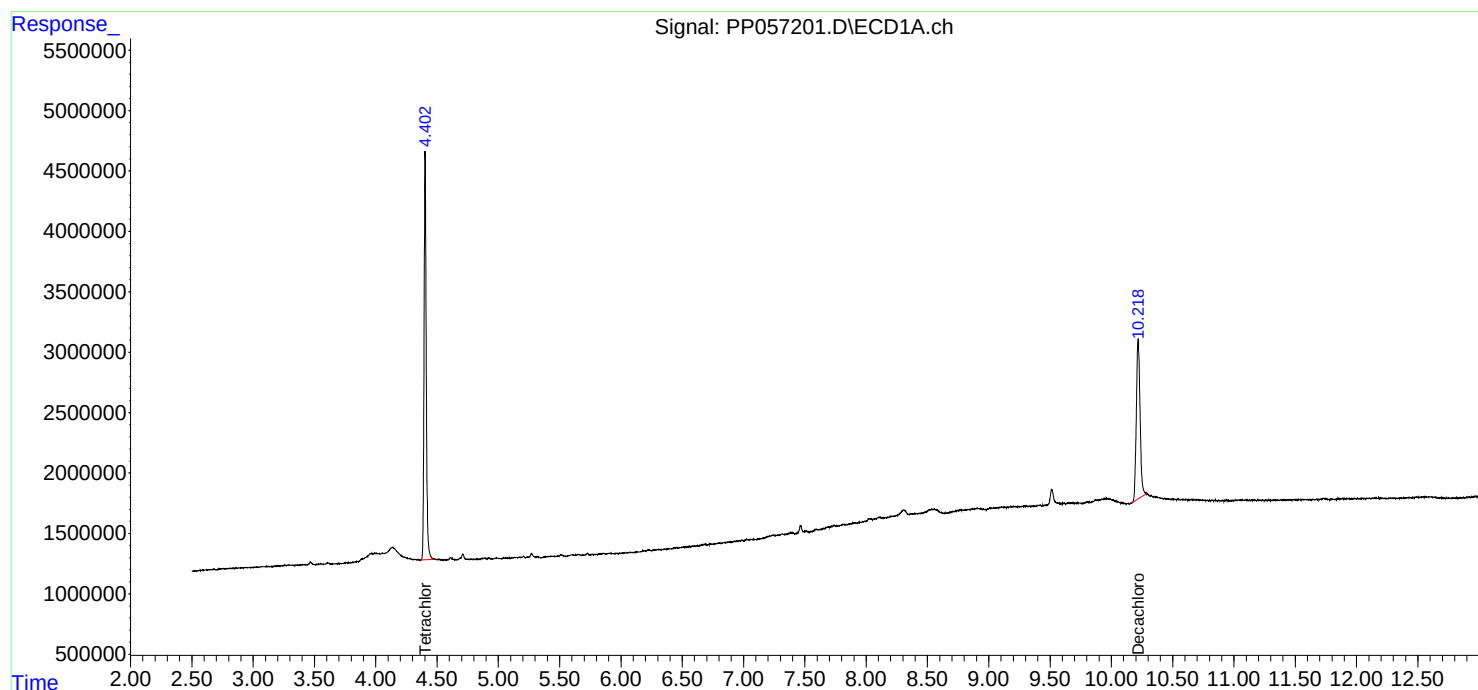


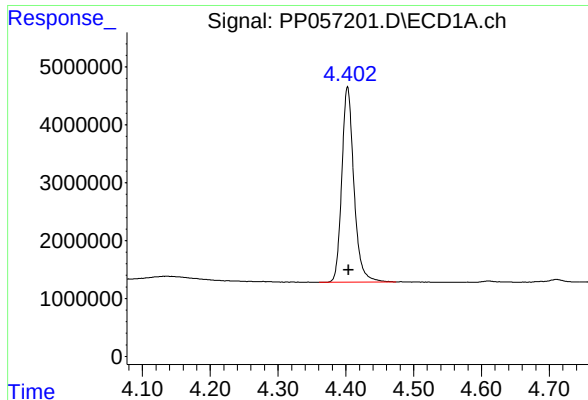

#1 Tetrachloro-m-xylene


R.T.: 4.403 min
Delta R.T.: -0.001 min
Response: 41943819
Conc: 18.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
MID-H4(ELEV-22)

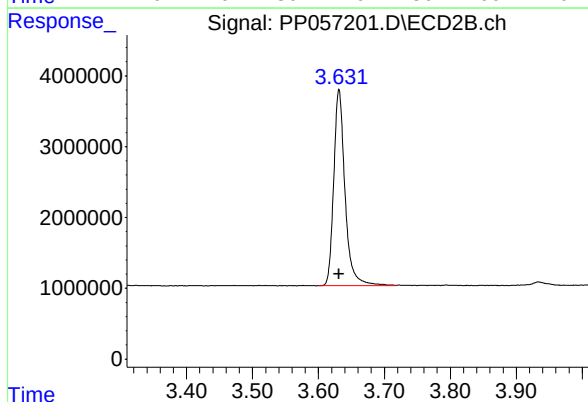


#1 Tetrachloro-m-xylene

R.T.: 3.631 min
Delta R.T.: 0.000 min
Response: 32938815
Conc: 19.50 ng/ml

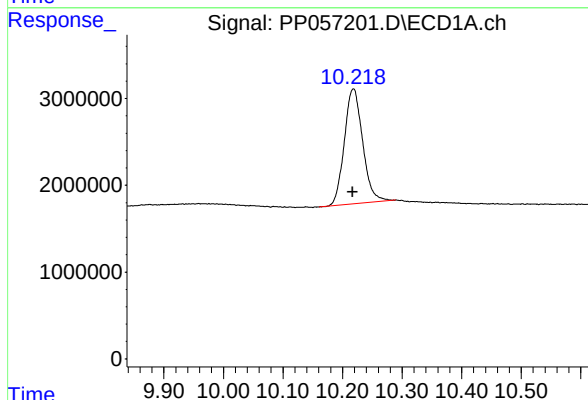

#2 Decachlorobiphenyl

R.T.: 10.218 min
Delta R.T.: 0.001 min
Response: 28352738
Conc: 17.67 ng/ml

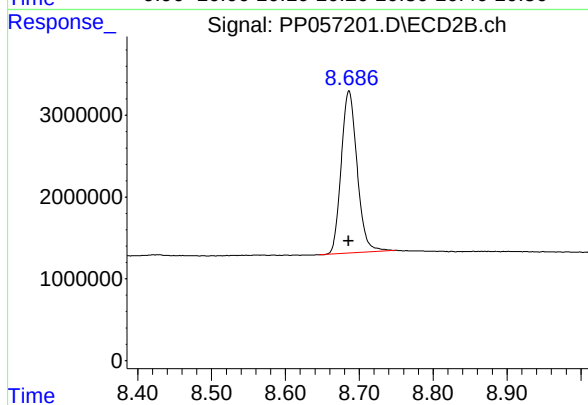

#2 Decachlorobiphenyl

R.T.: 8.686 min
Delta R.T.: 0.000 min
Response: 29661355
Conc: 16.58 ng/ml