

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042525\
 Data File : PP071479.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Apr 2025 17:53
 Operator : YP\AJ
 Sample : Q1868-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HAEFELY-HIPOTRONICS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/28/2025
 Supervised By :mohammad ahmed 05/02/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 23:59:05 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042225.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 23 05:02:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.513	3.813	40312973	26983871	20.333m	19.156
2) SA Decachlor...	10.233	8.847	28584295	16119811	19.740	18.380

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042525\
Data File : PP071479.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Apr 2025 17:53
Operator : YP\AJ
Sample : Q1868-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
HAEFELY-HIPOTRONICS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/28/2025
Supervised By :mohammad ahmed 05/02/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 23:59:05 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042225.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 23 05:02:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

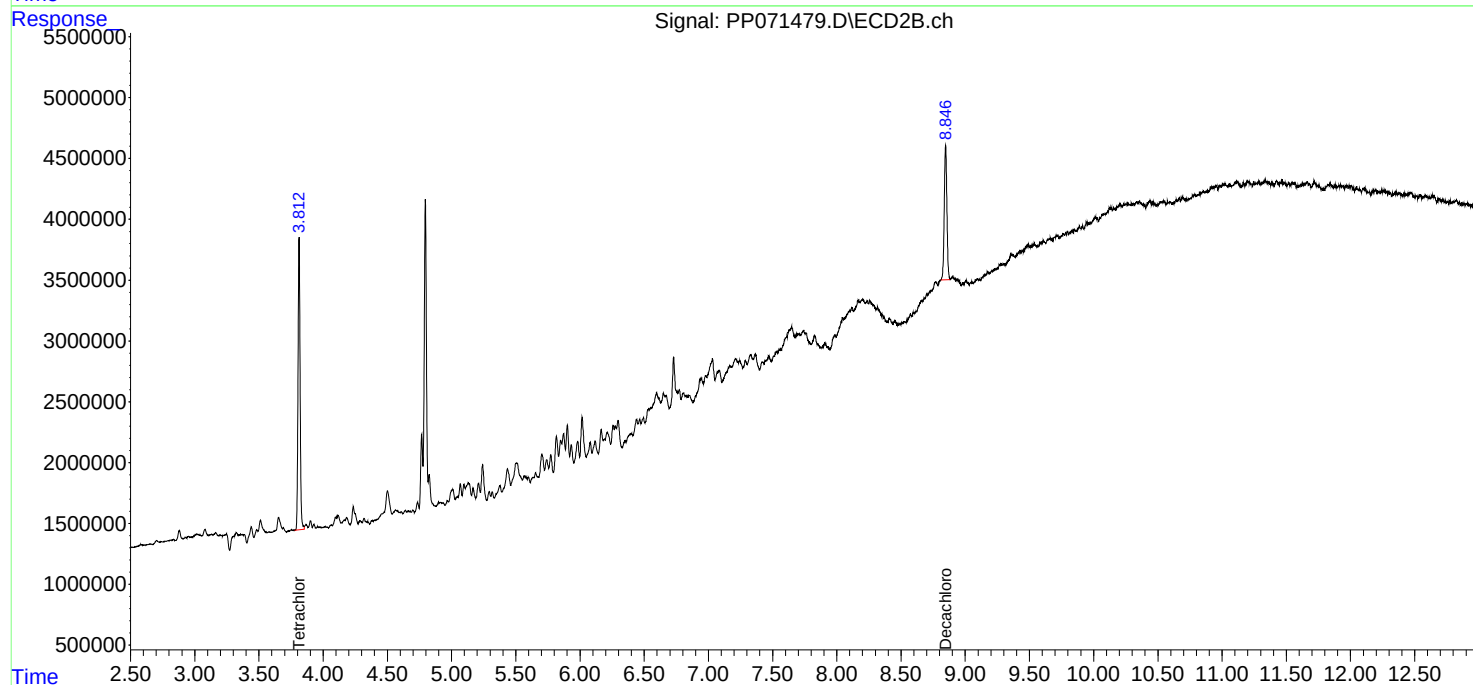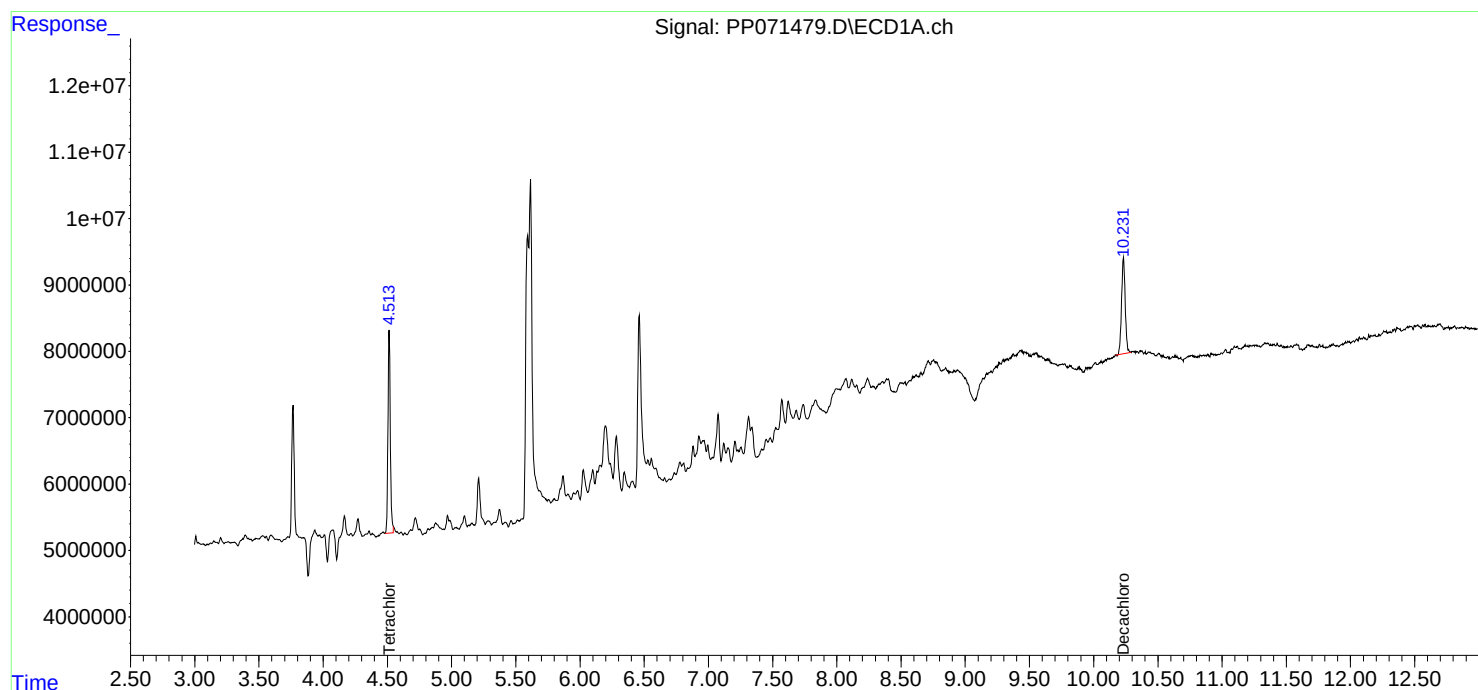

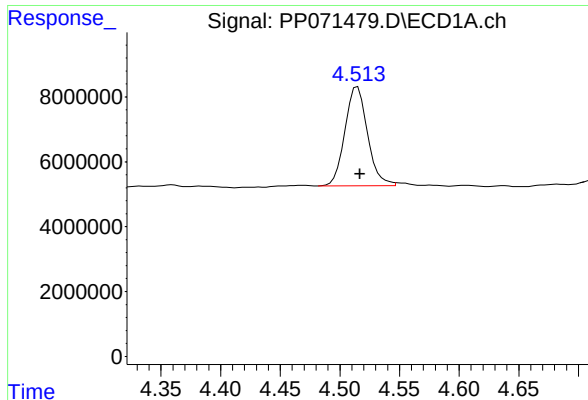


#1 Tetrachloro-m-xylene

R.T.: 4.513 min
Delta R.T.: -0.004 min
Response: 40312973
Conc: 20.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
HAEFELY-HIPOTRONICS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/28/2025
Supervised By :mohammad ahmed 05/02/2025

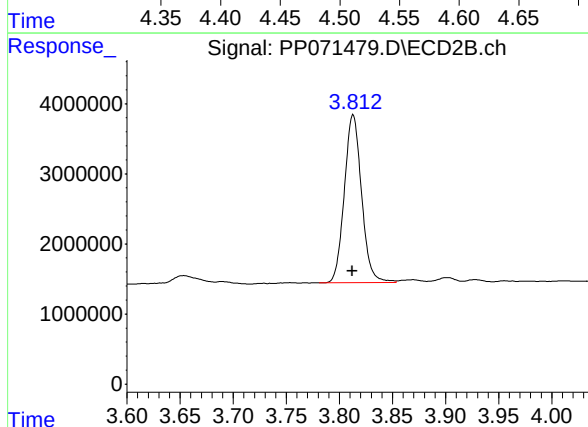


#1 Tetrachloro-m-xylene

R.T.: 3.813 min
Delta R.T.: 0.000 min
Response: 26983871
Conc: 19.16 ng/ml

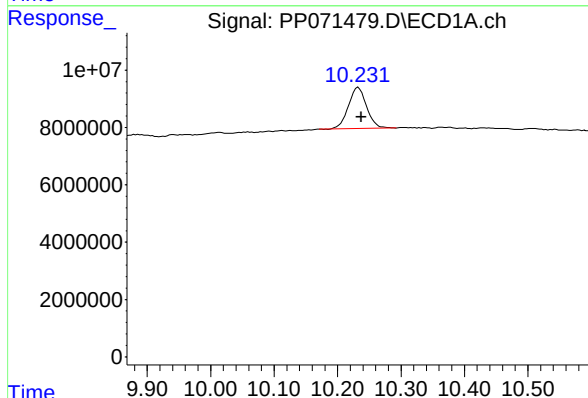

#2 Decachlorobiphenyl

R.T.: 10.233 min
Delta R.T.: -0.005 min
Response: 28584295
Conc: 19.74 ng/ml

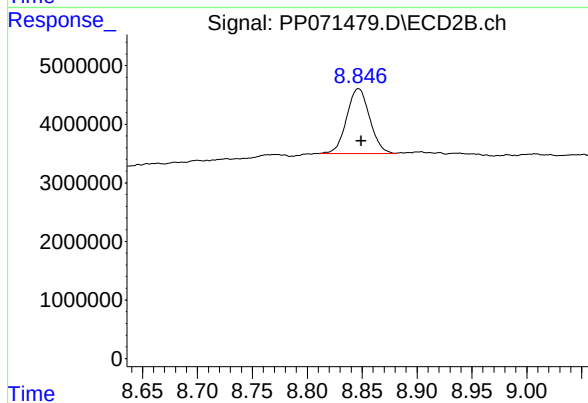

#2 Decachlorobiphenyl

R.T.: 8.847 min
Delta R.T.: -0.002 min
Response: 16119811
Conc: 18.38 ng/ml