

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042619\
 Data File : PP030026.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Apr 2019 14:23
 Operator : EI/SJ
 Sample : MDL-BL-WATER-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-BL-WATER-04

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 15:02:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042519.M
 Quant Title : 8080.M
 QLast Update : Fri Apr 26 10:04:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	12.144	12.215	243.1E6	169.4E6	546.740	423.019
Target Compounds							
3) T	4-Nitroph...	11.763	0.000	1027421	0	2.572	N.D. #
8) T	DICHLORPROP	13.673	0.000	687131	0	1.447	N.D. #
15) T	Picloram	17.802	18.402	1062549	645081	0.300	0.239
16) T	DCPA	18.348	18.236	788252	694012	0.222	0.256



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042619\
Data File : PP030026.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Apr 2019 14:23
Operator : EI/SJ
Sample : MDL-BL-WATER-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-BL-WATER-04

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 15:02:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042519.M
Quant Title : 8080.M
QLast Update : Fri Apr 26 10:04:13 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

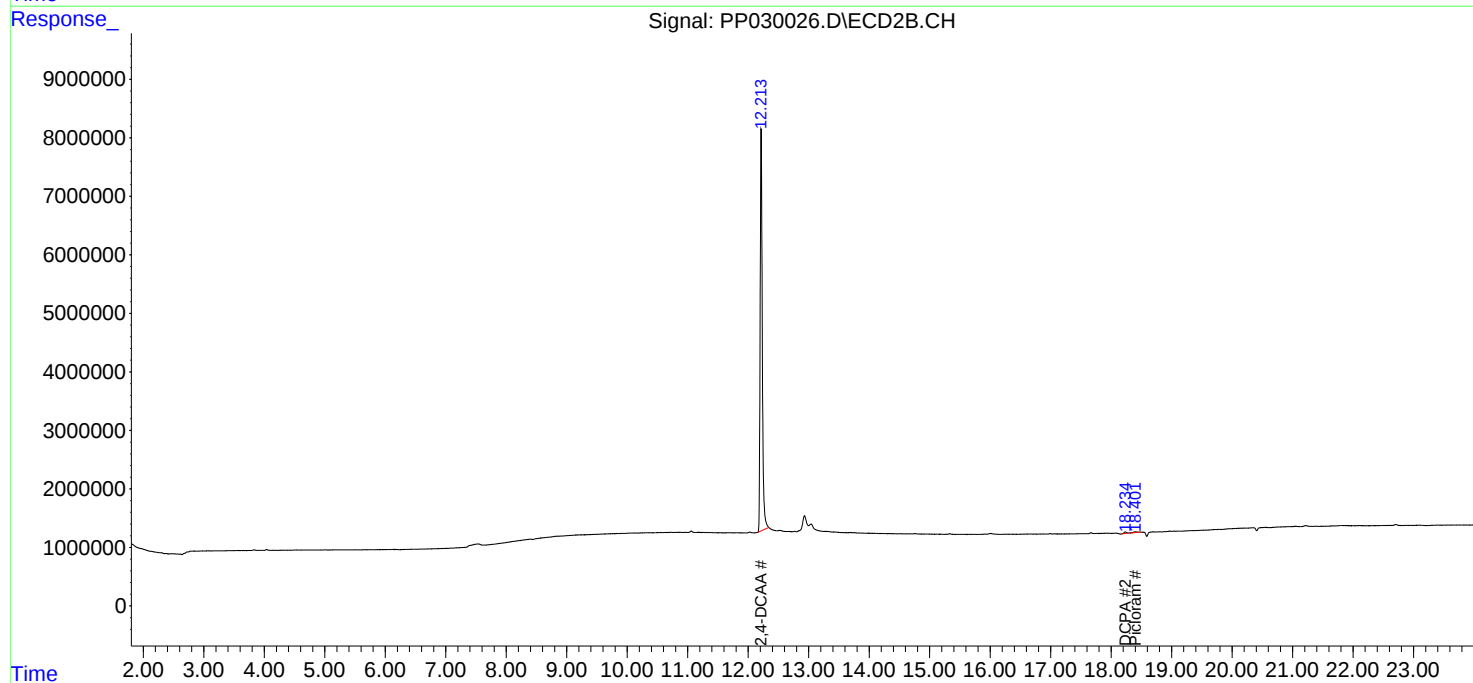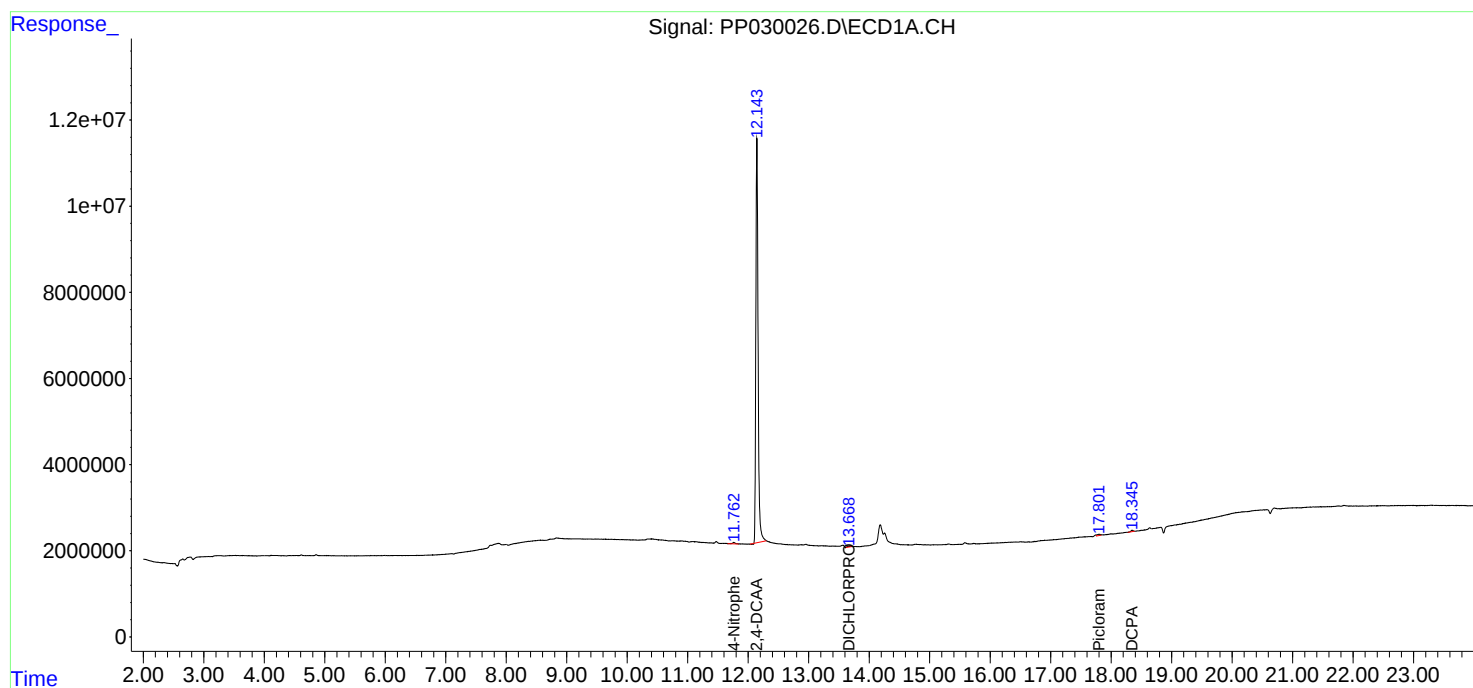


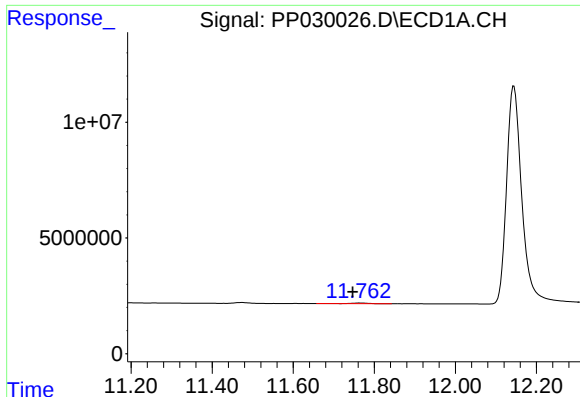

#3 4-Nitrophenol


R.T.: 11.763 min
Delta R.T.: 0.016 min
Response: 1027421
Conc: 2.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-BL-WATER-04

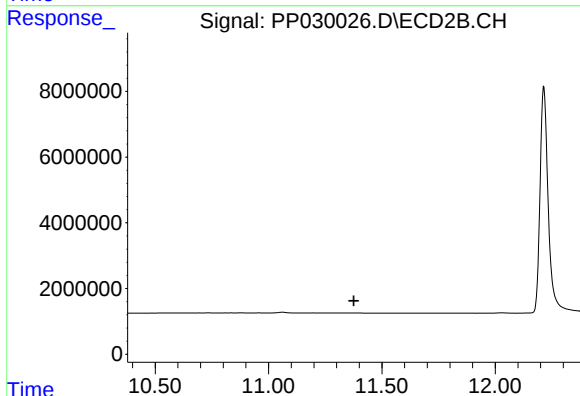


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 11.376 min
Response: 0
Conc: N.D.

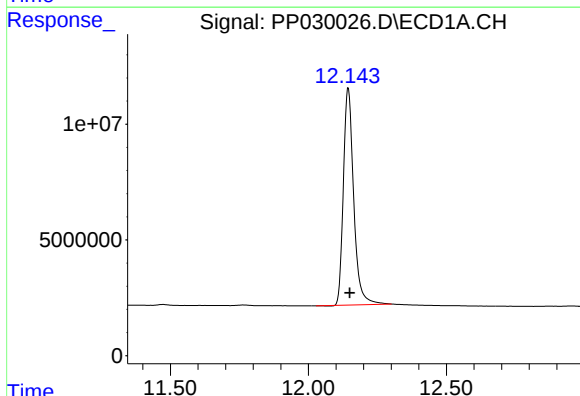


#4 2,4-DCAA

R.T.: 12.144 min
Delta R.T.: -0.005 min
Response: 243132719
Conc: 546.74 ng/ml

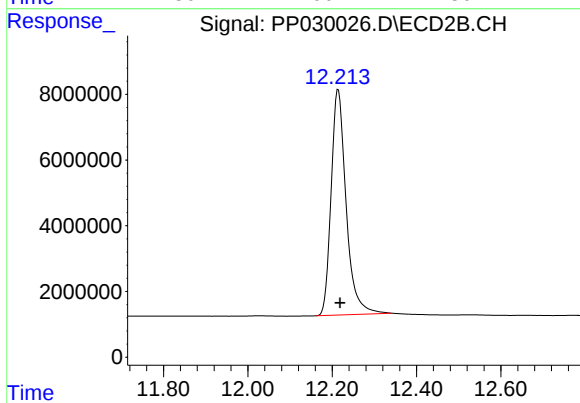

#4 2,4-DCAA


R.T.: 12.215 min
Delta R.T.: -0.004 min
Response: 169350131
Conc: 423.02 ng/ml

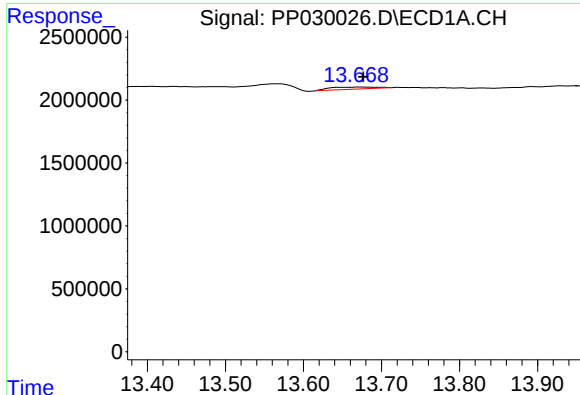

#8 DICHLORPROP


R.T.: 13.673 min
Delta R.T.: -0.004 min
Response: 687131
Conc: 1.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-BL-WATER-04

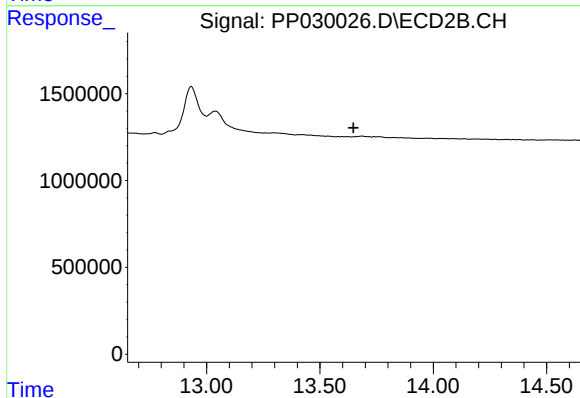


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.649 min
Response: 0
Conc: N.D.

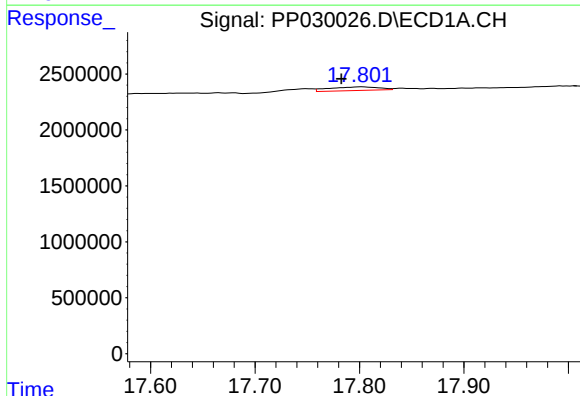


#15 Picloram

R.T.: 17.802 min
Delta R.T.: 0.019 min
Response: 1062549
Conc: 0.30 ng/ml

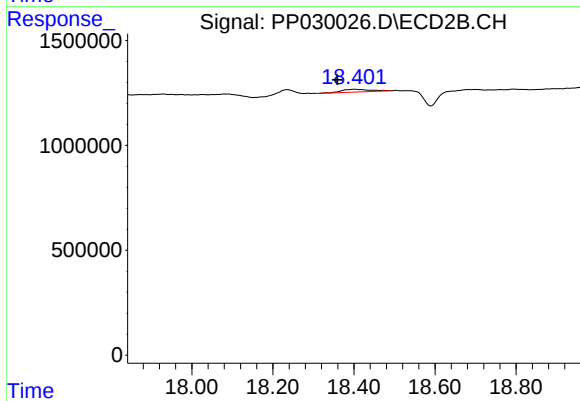

#15 Picloram


R.T.: 18.402 min
Delta R.T.: 0.042 min
Response: 645081
Conc: 0.24 ng/ml

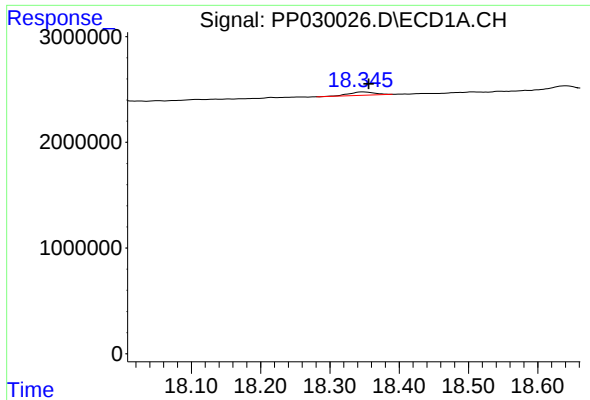

#16 DCPA

R.T.: 18.348 min
Delta R.T.: -0.008 min
Response: 788252
Conc: 0.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-BL-WATER-04

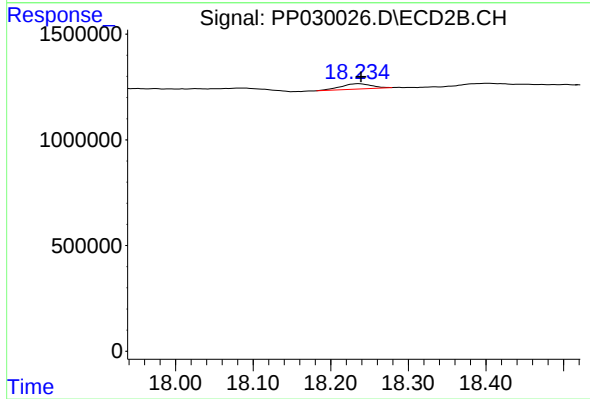

#16 DCPA

R.T.: 18.236 min
Delta R.T.: -0.003 min
Response: 694012
Conc: 0.26 ng/ml