

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042619\
 Data File : PP030027.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Apr 2019 14:51
 Operator : EI/SJ
 Sample : MDL-BL-WATER-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-BL-WATER-05

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 15:28:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042519.M
 Quant Title : 8080.M
 QLast Update : Fri Apr 26 10:04:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	12.141	12.211	282.8E6	199.8E6	635.939	499.009
Target Compounds							
3) T	4-Nitroph...	11.763	0.000	631254	0	1.580	N.D. #
12) T	2,4,5-T	0.000	16.001	0	938819	N.D.	0.451 #
15) T	Picloram	17.793	18.400	2255336	547213	0.636	0.203 #
16) T	DCPA	18.346	18.230	994905	823206	0.280	0.303



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042619\
Data File : PP030027.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Apr 2019 14:51
Operator : EI/SJ
Sample : MDL-BL-WATER-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-BL-WATER-05

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 15:28:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042519.M
Quant Title : 8080.M
QLast Update : Fri Apr 26 10:04:13 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

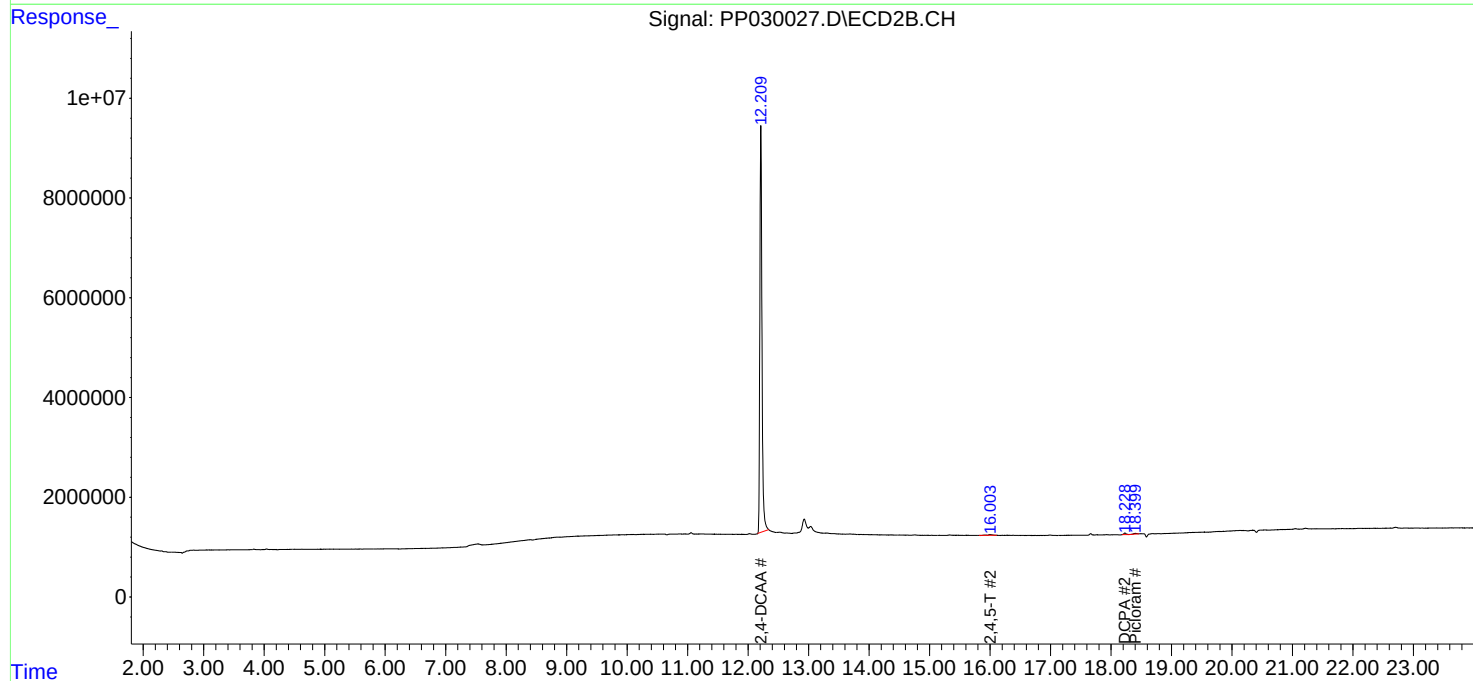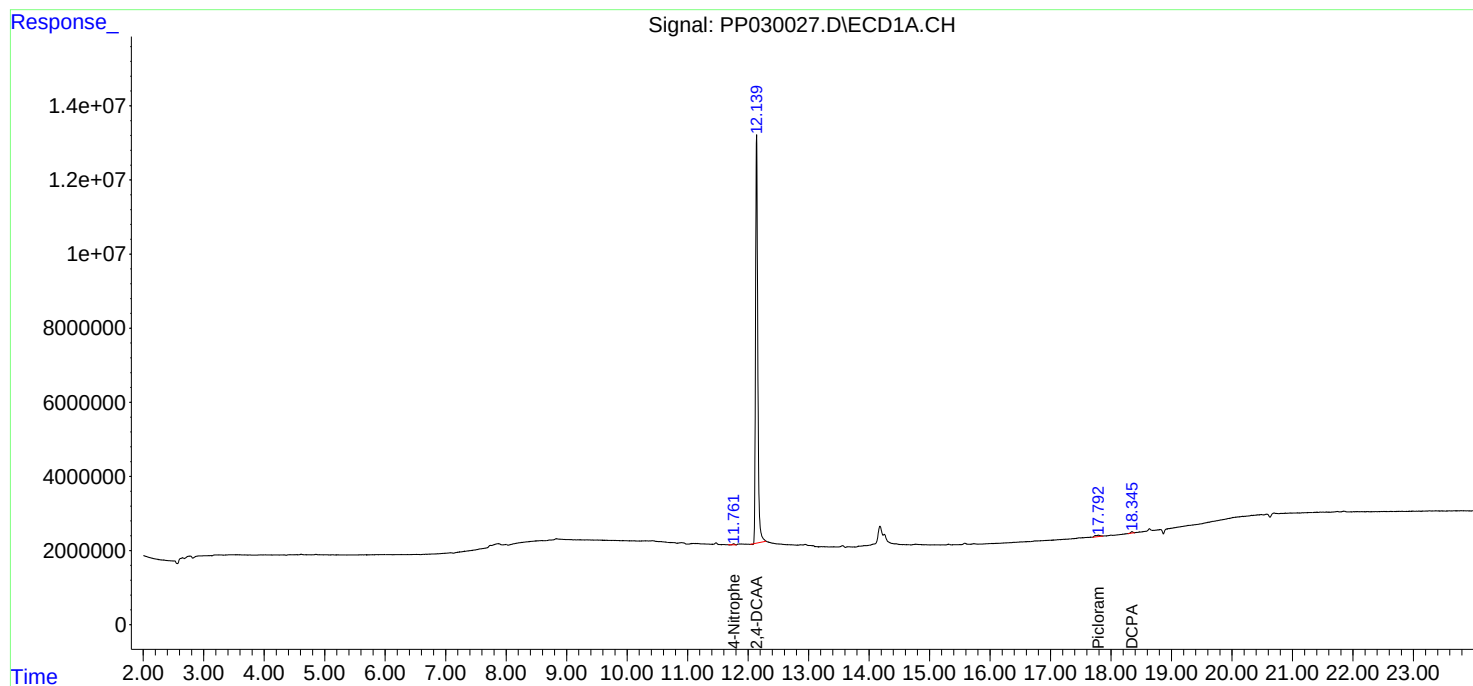


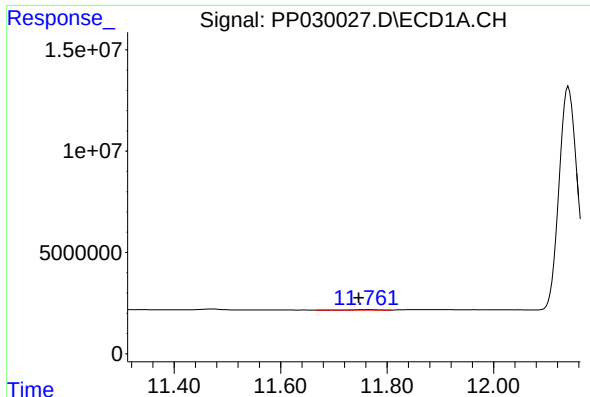

#3 4-Nitrophenol


R.T.: 11.763 min
Delta R.T.: 0.016 min
Response: 631254
Conc: 1.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-BL-WATER-05

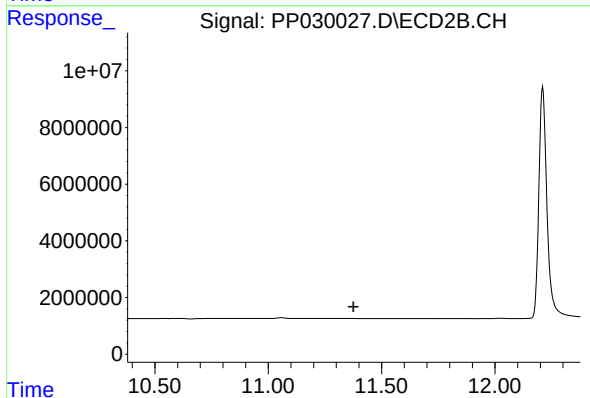


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 11.376 min
Response: 0
Conc: N.D.

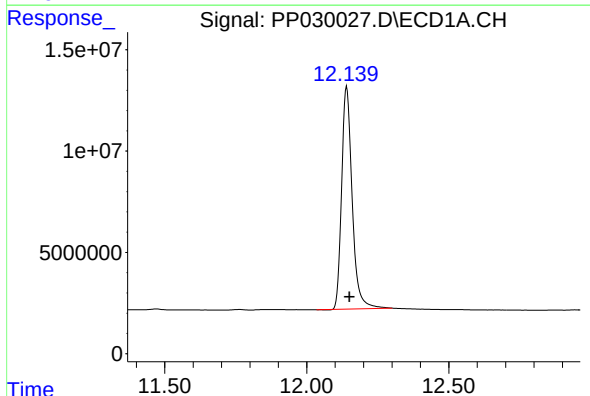


#4 2,4-DCAA

R.T.: 12.141 min
Delta R.T.: -0.009 min
Response: 282798846
Conc: 635.94 ng/ml

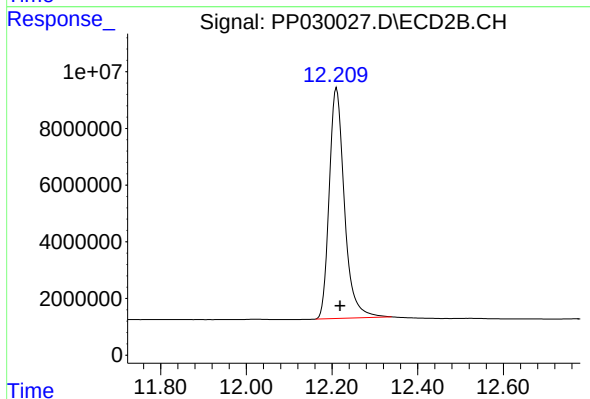

#4 2,4-DCAA


R.T.: 12.211 min
Delta R.T.: -0.008 min
Response: 199771572
Conc: 499.01 ng/ml

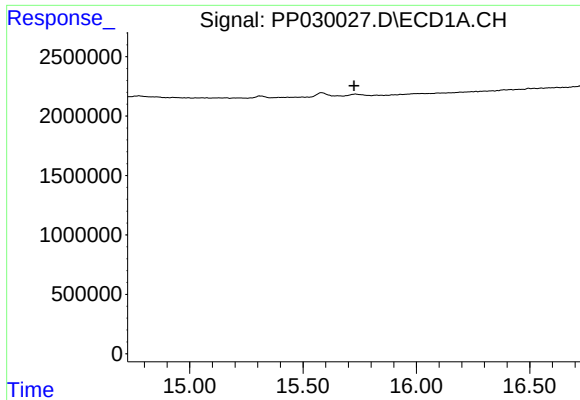

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.725 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-BL-WATER-05

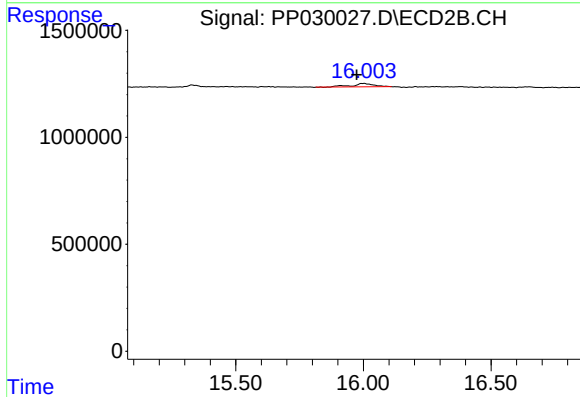


#12 2,4,5-T

R.T.: 16.001 min
Delta R.T.: 0.028 min
Response: 938819
Conc: 0.45 ng/ml

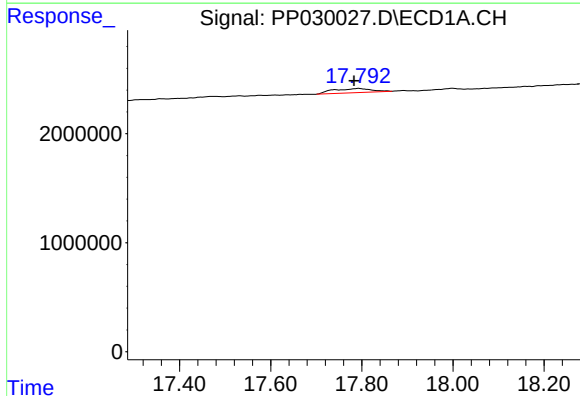


#15 Picloram

R.T.: 17.793 min
Delta R.T.: 0.010 min
Response: 2255336
Conc: 0.64 ng/ml

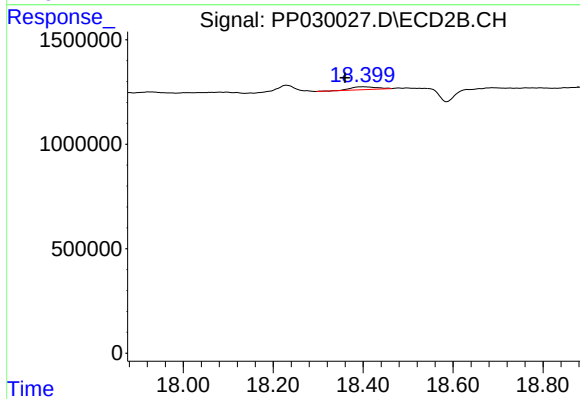

#15 Picloram


R.T.: 18.400 min
Delta R.T.: 0.040 min
Response: 547213
Conc: 0.20 ng/ml

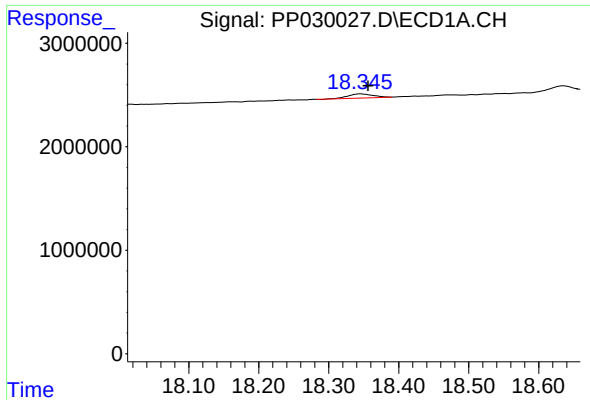

#16 DCPA

R.T.: 18.346 min
Delta R.T.: -0.010 min
Response: 994905
Conc: 0.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-BL-WATER-05

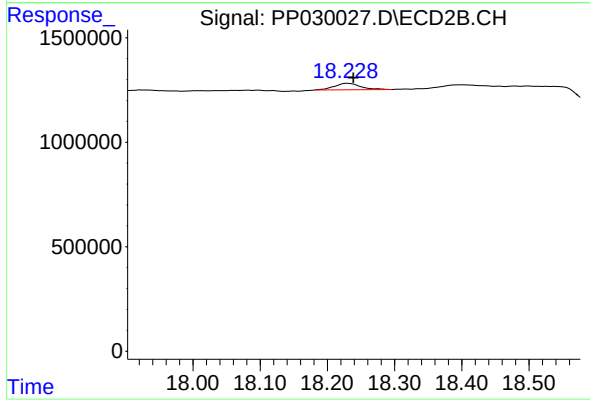

#16 DCPA

R.T.: 18.230 min
Delta R.T.: -0.008 min
Response: 823206
Conc: 0.30 ng/ml