

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042621\
 Data File : PP035288.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Apr 2021 21:29
 Operator : DD\AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248ICC050

Manual Integrations
 APPROVED

Ankita
 4/27/2021 11:15:57 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 05:55:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 27 05:51:35 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.838	4.242	419694	273871	5.324	5.426
2) SA Decachlor...	10.738	9.522	355291	137311	5.121	5.287
Target Compounds						
21) L5 AR-1248-1	6.150	5.493	74089	37945	57.875	58.271
22) L5 AR-1248-2	6.440	5.749	117580	63535	59.058m	55.700
23) L5 AR-1248-3	6.656	5.795	134731	63802	56.112	53.766
24) L5 AR-1248-4	7.084	5.979	117613	70968	51.425	52.232
25) L5 AR-1248-5	7.124	6.403	119619	57944	49.437	45.979m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042621\
Data File : PP035288.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Apr 2021 21:29
Operator : DD\AJ
Sample : AR1248ICC050
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Ankita
4/27/2021 11:15:57 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 05:55:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042621.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 27 05:51:35 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

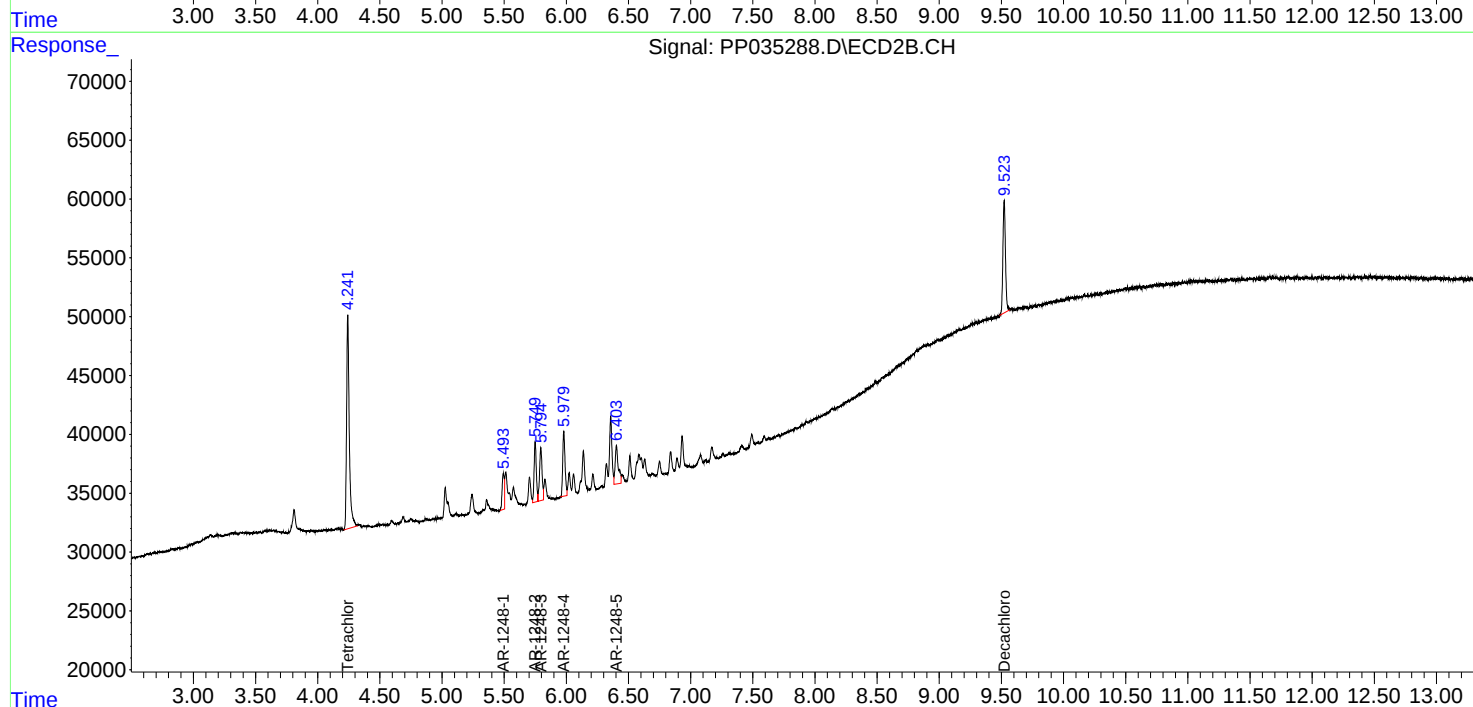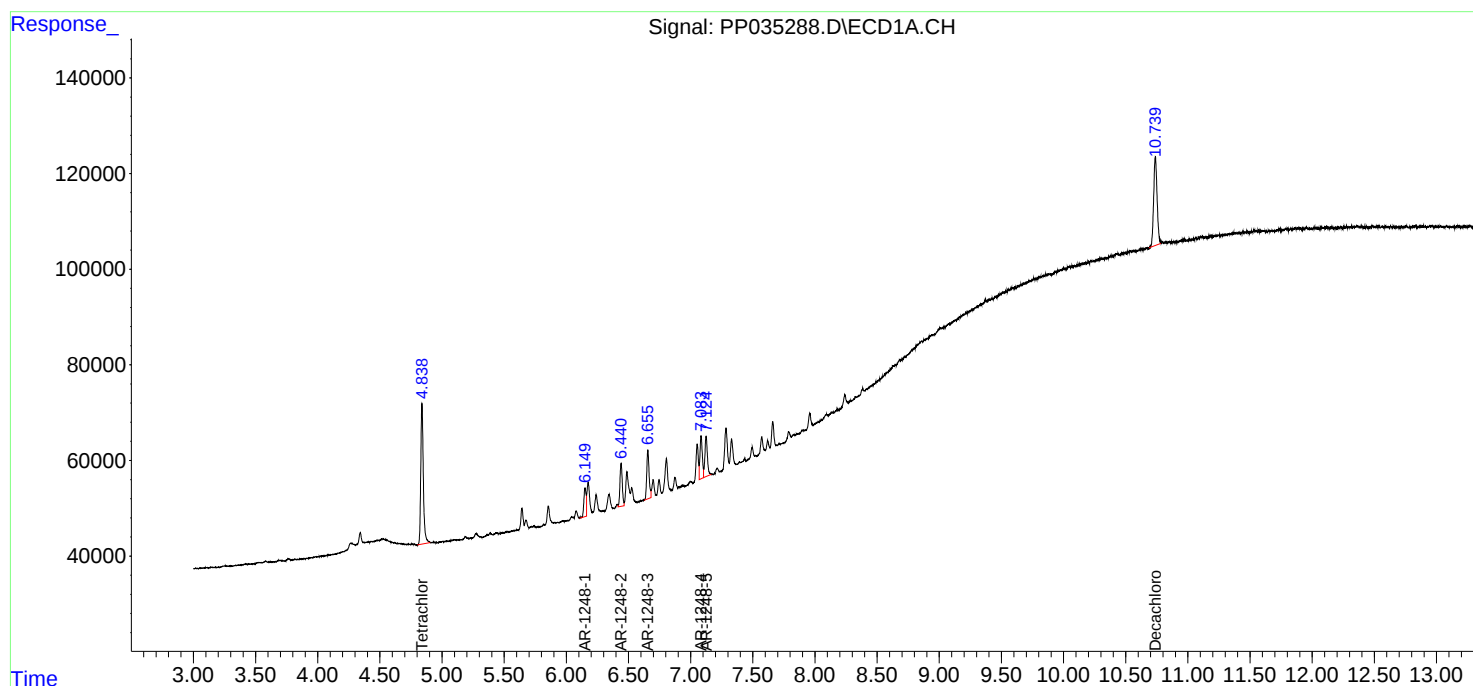

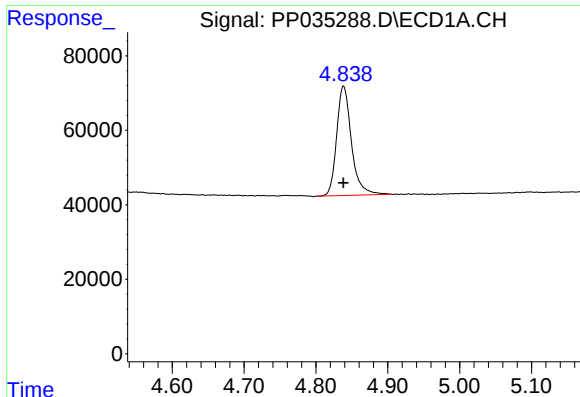


#1 Tetrachloro-m-xylene

R.T.: 4.838 min
Delta R.T.: 0.000 min
Response: 419694
Conc: 5.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Ankita
4/27/2021 11:15:57 AM

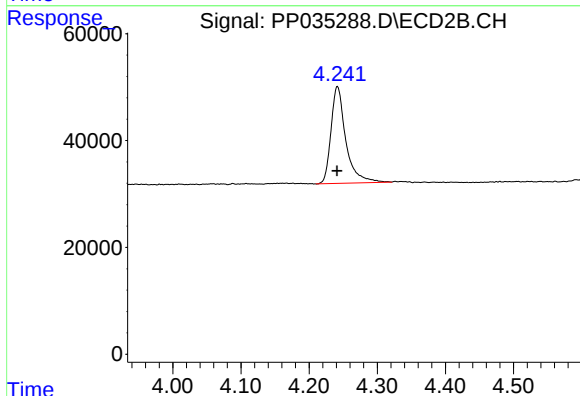


#1 Tetrachloro-m-xylene

R.T.: 4.242 min
Delta R.T.: 0.000 min
Response: 273871
Conc: 5.43 ng/ml

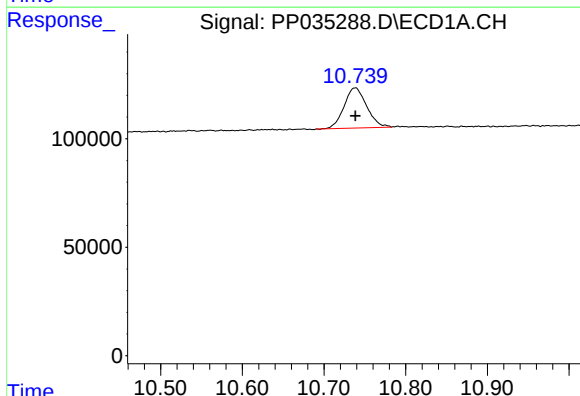


#2 Decachlorobiphenyl

R.T.: 10.738 min
Delta R.T.: 0.000 min
Response: 355291
Conc: 5.12 ng/ml

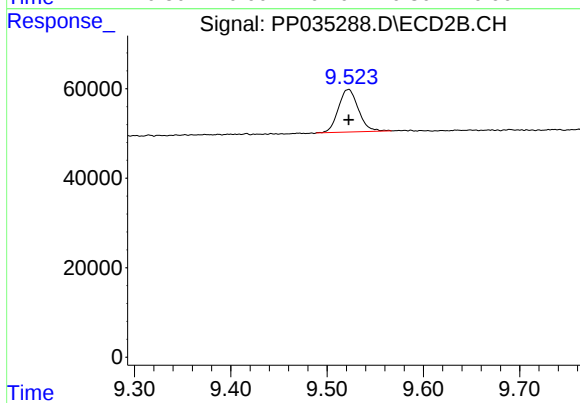

#2 Decachlorobiphenyl

R.T.: 9.522 min
Delta R.T.: 0.000 min
Response: 137311
Conc: 5.29 ng/ml

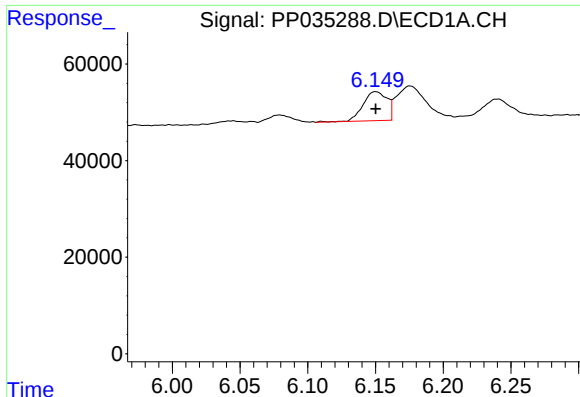


#21 AR-1248-1

R.T.: 6.150 min
Delta R.T.: 0.000 min
Response: 74089
Conc: 57.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Ankita
4/27/2021 11:15:57 AM

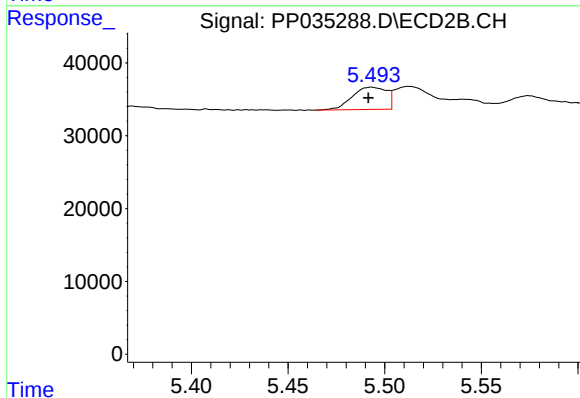


#21 AR-1248-1

R.T.: 5.493 min
Delta R.T.: 0.002 min
Response: 37945
Conc: 58.27 ng/ml

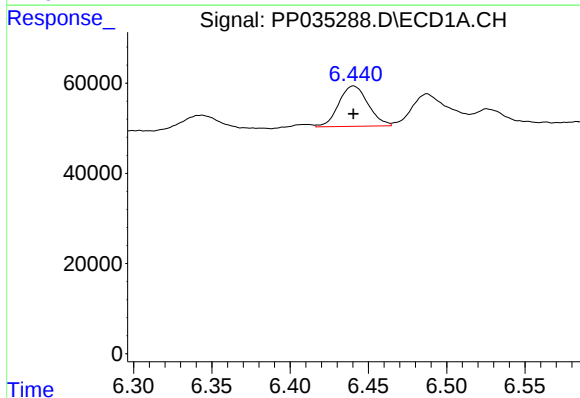


#22 AR-1248-2

R.T.: 6.440 min
Delta R.T.: 0.000 min
Response: 117580
Conc: 59.06 ng/ml m

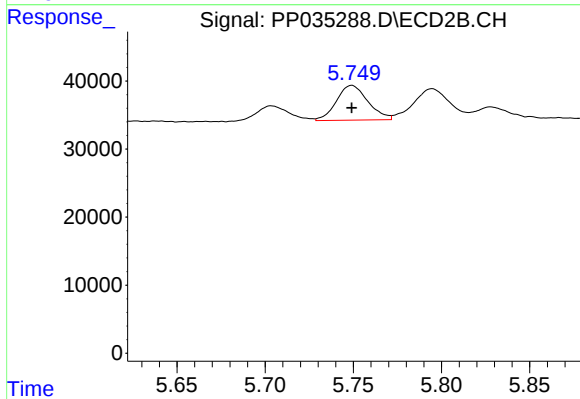

#22 AR-1248-2

R.T.: 5.749 min
Delta R.T.: 0.000 min
Response: 63535
Conc: 55.70 ng/ml

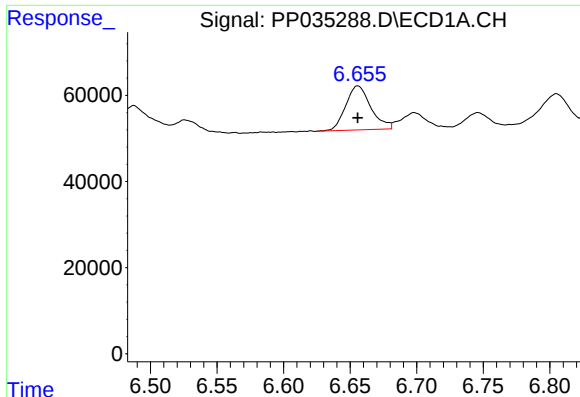


#23 AR-1248-3

R.T.: 6.656 min
Delta R.T.: 0.000 min
Response: 134731
Conc: 56.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Ankita
4/27/2021 11:15:57 AM

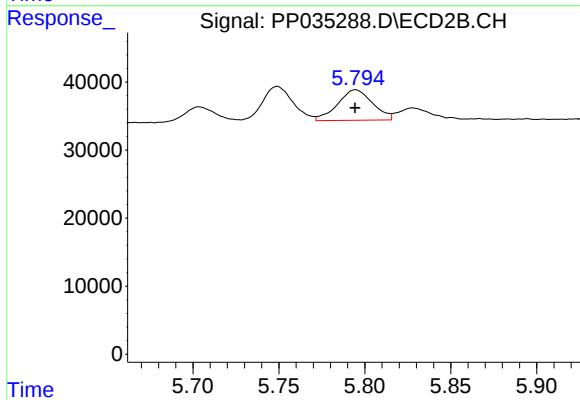


#23 AR-1248-3

R.T.: 5.795 min
Delta R.T.: 0.000 min
Response: 63802
Conc: 53.77 ng/ml

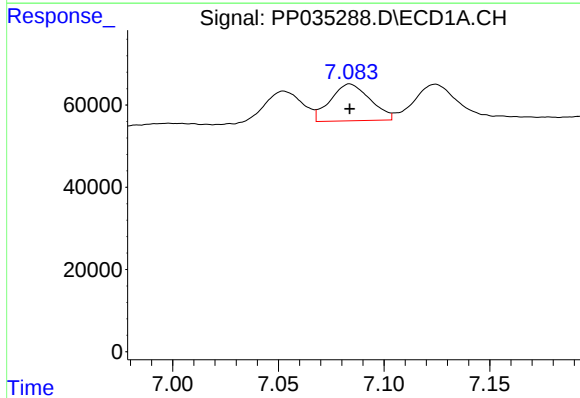


#24 AR-1248-4

R.T.: 7.084 min
Delta R.T.: 0.000 min
Response: 117613
Conc: 51.43 ng/ml

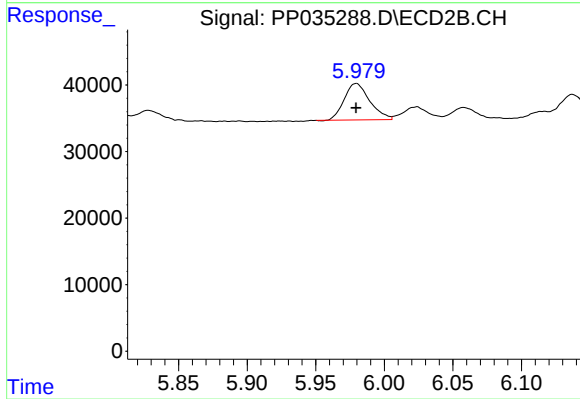

#24 AR-1248-4

R.T.: 5.979 min
Delta R.T.: 0.000 min
Response: 70968
Conc: 52.23 ng/ml

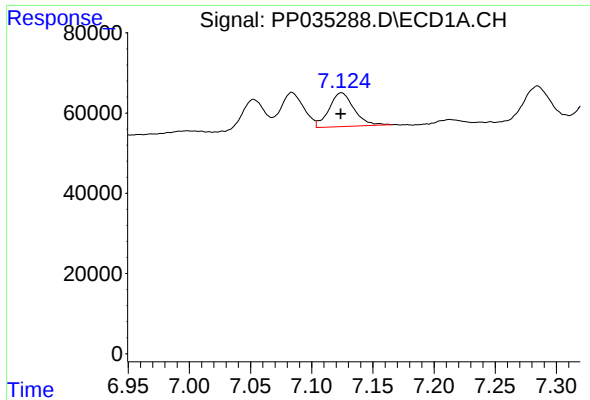


#25 AR-1248-5

R.T.: 7.124 min
Delta R.T.: 0.000 min
Response: 119619
Conc: 49.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050

Manual Integrations
APPROVED

Ankita
4/27/2021 11:15:57 AM

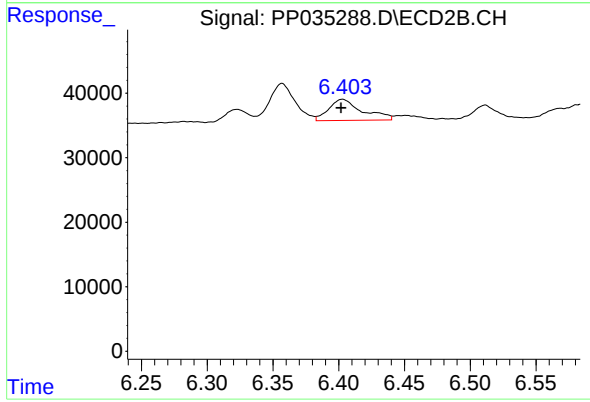

#25 AR-1248-5

R.T.: 6.403 min
Delta R.T.: 0.001 min
Response: 57944
Conc: 45.98 ng/ml m