

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042621\
 Data File : PP035293.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Apr 2021 22:54
 Operator : DD\AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Ankita
 4/27/2021 11:15:59 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 06:11:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 27 06:10:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.838	4.240	414379	271112	5.352	5.459
2) SA Decachlor...	10.739	9.521	350599	144879	5.079	5.579
Target Compounds						
26) L6 AR-1254-1	7.050	6.353	150844	99536	56.349	53.869m
27) L6 AR-1254-2	7.279	6.511	229260	89990	56.389	54.649
28) L6 AR-1254-3	7.660	6.931	210580	110168	49.445	46.116
29) L6 AR-1254-4	7.956	7.169	154870	55867	58.577m	51.369m
30) L6 AR-1254-5	8.381	7.591	164818	100600	47.895m	47.657

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042621\
Data File : PP035293.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Apr 2021 22:54
Operator : DD\AJ
Sample : AR1254ICC050
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
4/27/2021 11:15:59 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 06:11:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042621.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 27 06:10:21 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

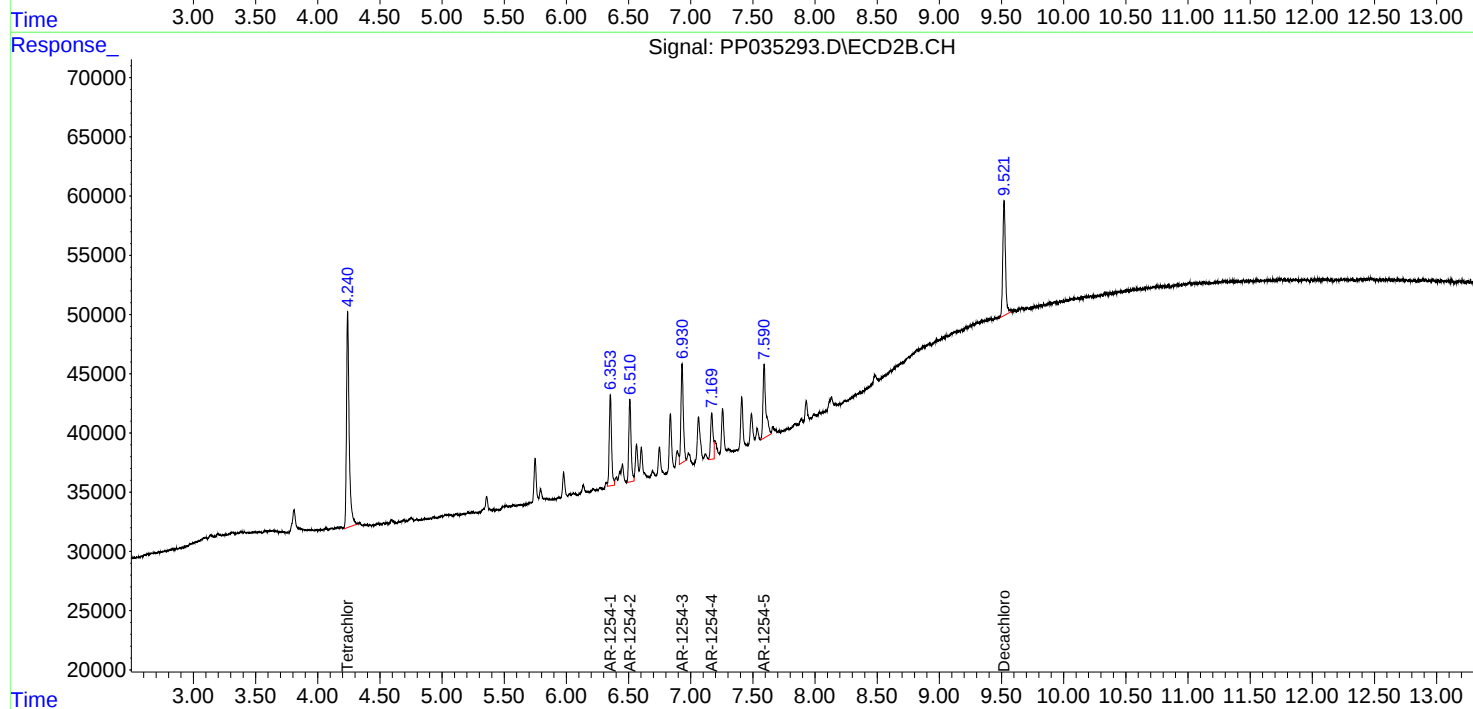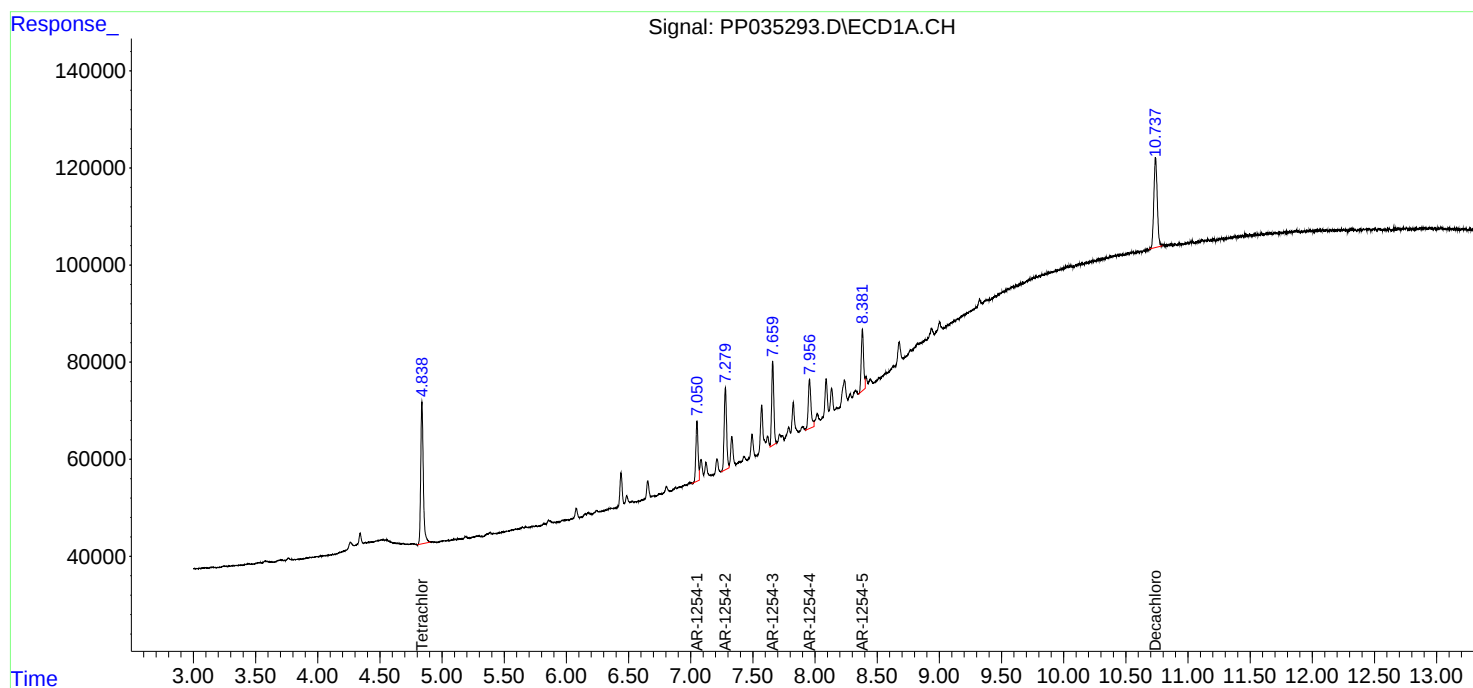

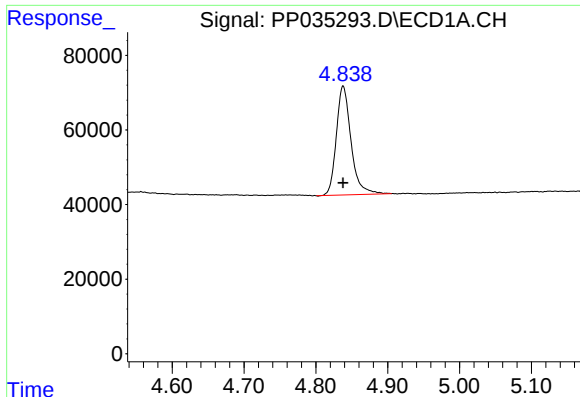


#1 Tetrachloro-m-xylene

R.T.: 4.838 min
Delta R.T.: 0.000 min
Response: 414379
Conc: 5.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
4/27/2021 11:15:59 AM

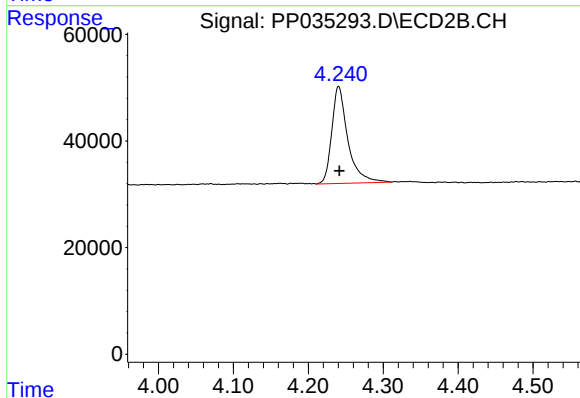


#1 Tetrachloro-m-xylene

R.T.: 4.240 min
Delta R.T.: 0.000 min
Response: 271112
Conc: 5.46 ng/ml

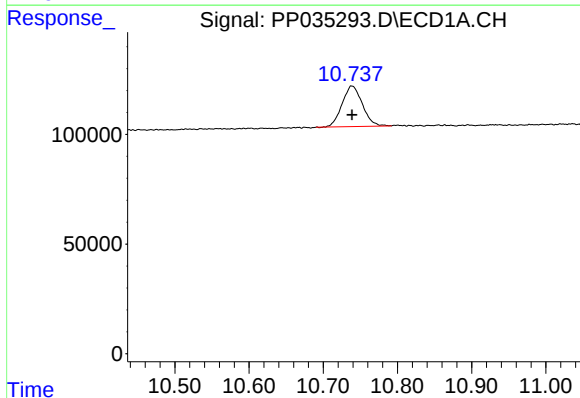


#2 Decachlorobiphenyl

R.T.: 10.739 min
Delta R.T.: 0.000 min
Response: 350599
Conc: 5.08 ng/ml

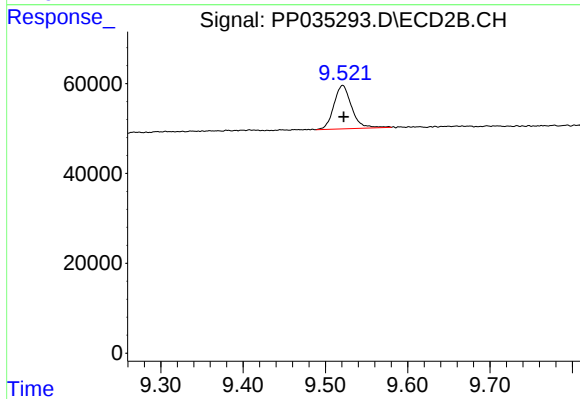

#2 Decachlorobiphenyl

R.T.: 9.521 min
Delta R.T.: -0.001 min
Response: 144879
Conc: 5.58 ng/ml

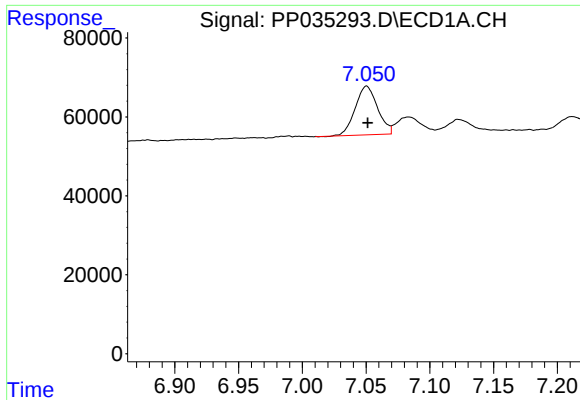


#26 AR-1254-1

R.T.: 7.050 min
Delta R.T.: 0.000 min
Response: 150844
Conc: 56.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
4/27/2021 11:15:59 AM

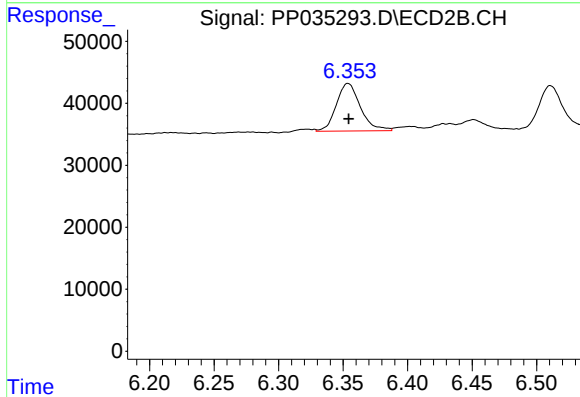


#26 AR-1254-1

R.T.: 6.353 min
Delta R.T.: -0.001 min
Response: 99536
Conc: 53.87 ng/ml m

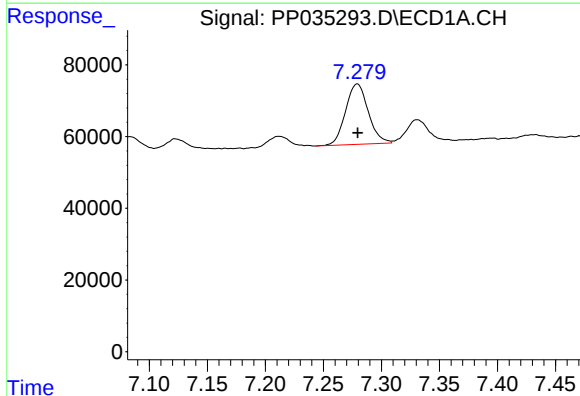


#27 AR-1254-2

R.T.: 7.279 min
Delta R.T.: 0.000 min
Response: 229260
Conc: 56.39 ng/ml

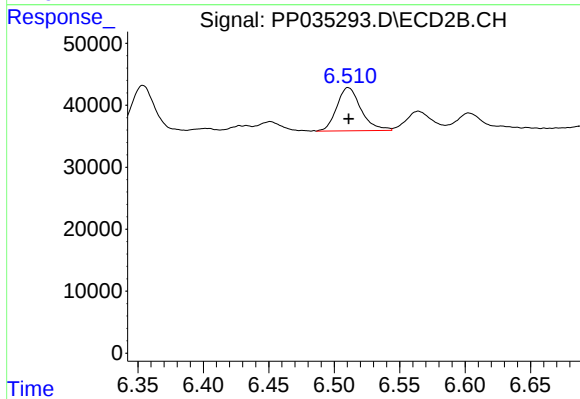

#27 AR-1254-2

R.T.: 6.511 min
Delta R.T.: 0.000 min
Response: 89990
Conc: 54.65 ng/ml

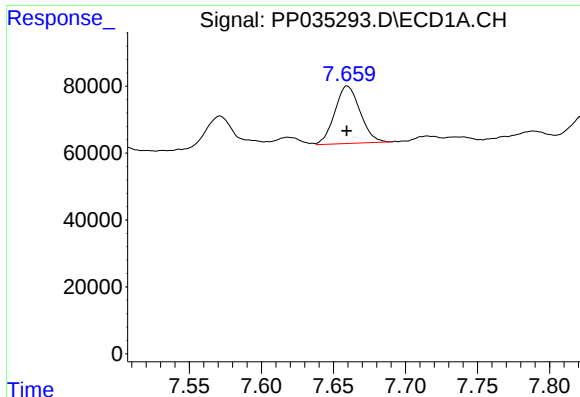


#28 AR-1254-3

R.T.: 7.660 min
Delta R.T.: 0.000 min
Response: 210580
Conc: 49.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
4/27/2021 11:15:59 AM

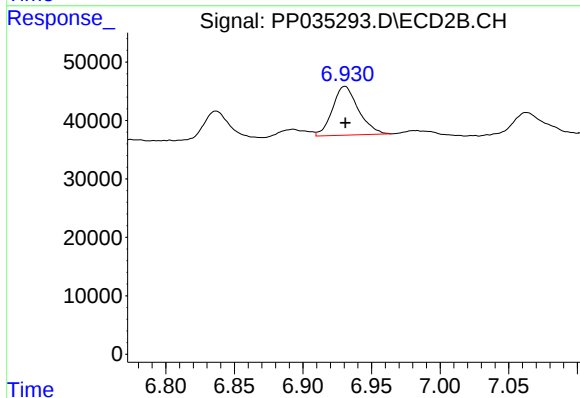


#28 AR-1254-3

R.T.: 6.931 min
Delta R.T.: 0.000 min
Response: 110168
Conc: 46.12 ng/ml

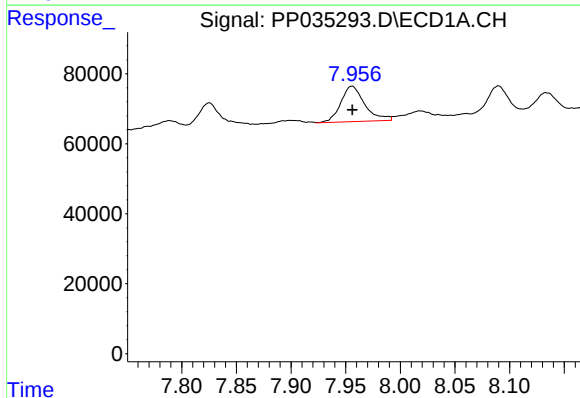


#29 AR-1254-4

R.T.: 7.956 min
Delta R.T.: 0.000 min
Response: 154870
Conc: 58.58 ng/ml m

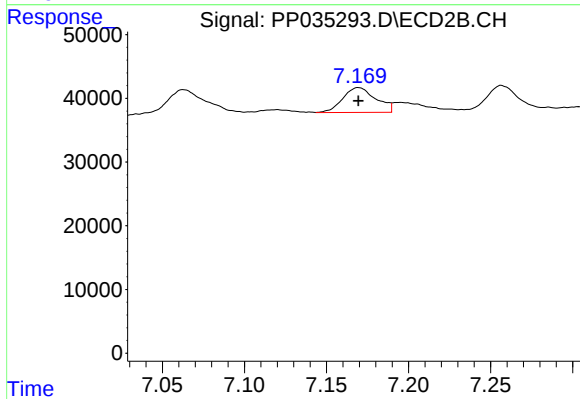

#29 AR-1254-4

R.T.: 7.169 min
Delta R.T.: 0.000 min
Response: 55867
Conc: 51.37 ng/ml m

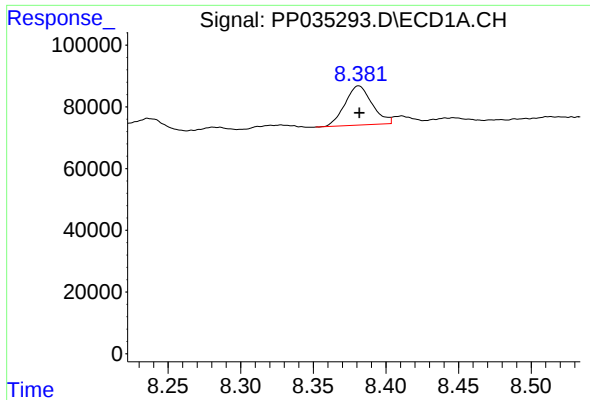


#30 AR-1254-5

R.T.: 8.381 min
Delta R.T.: -0.001 min
Response: 164818
Conc: 47.89 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Ankita
4/27/2021 11:15:59 AM

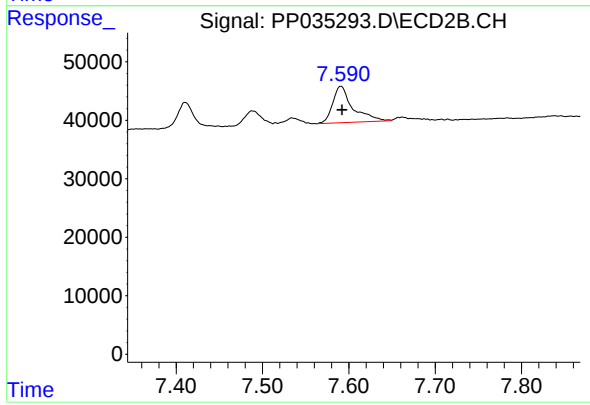

#30 AR-1254-5

R.T.: 7.591 min
Delta R.T.: -0.001 min
Response: 100600
Conc: 47.66 ng/ml