

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042621\
 Data File : PP035303.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Apr 2021 1:42
 Operator : DD\AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1268ICC050

Manual Integrations
 APPROVED

Ankita
 4/27/2021 11:16:03 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 07:23:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 27 07:22:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.837	4.241	425214	267719	5.418	5.361
2)	SA Decachlor...	10.738	9.520	646699	243647	5.435	5.535
Target Compounds							
41)	L9 AR-1268-1	9.297	8.415	501100	235254	52.772m	56.640m
42)	L9 AR-1268-2	9.391	8.481	459410	211180	48.212	52.219
43)	L9 AR-1268-3	9.605	8.684	432002	197447	51.938m	56.186m
44)	L9 AR-1268-4	10.028	8.976	149125	60852	52.158	52.132
45)	L9 AR-1268-5	10.421	9.268	1228605	482903	49.022m	50.089

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042621\
Data File : PP035303.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Apr 2021 1:42
Operator : DD\AJ
Sample : AR1268ICC050
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Ankita
4/27/2021 11:16:03 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 07:23:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042621.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 27 07:22:10 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

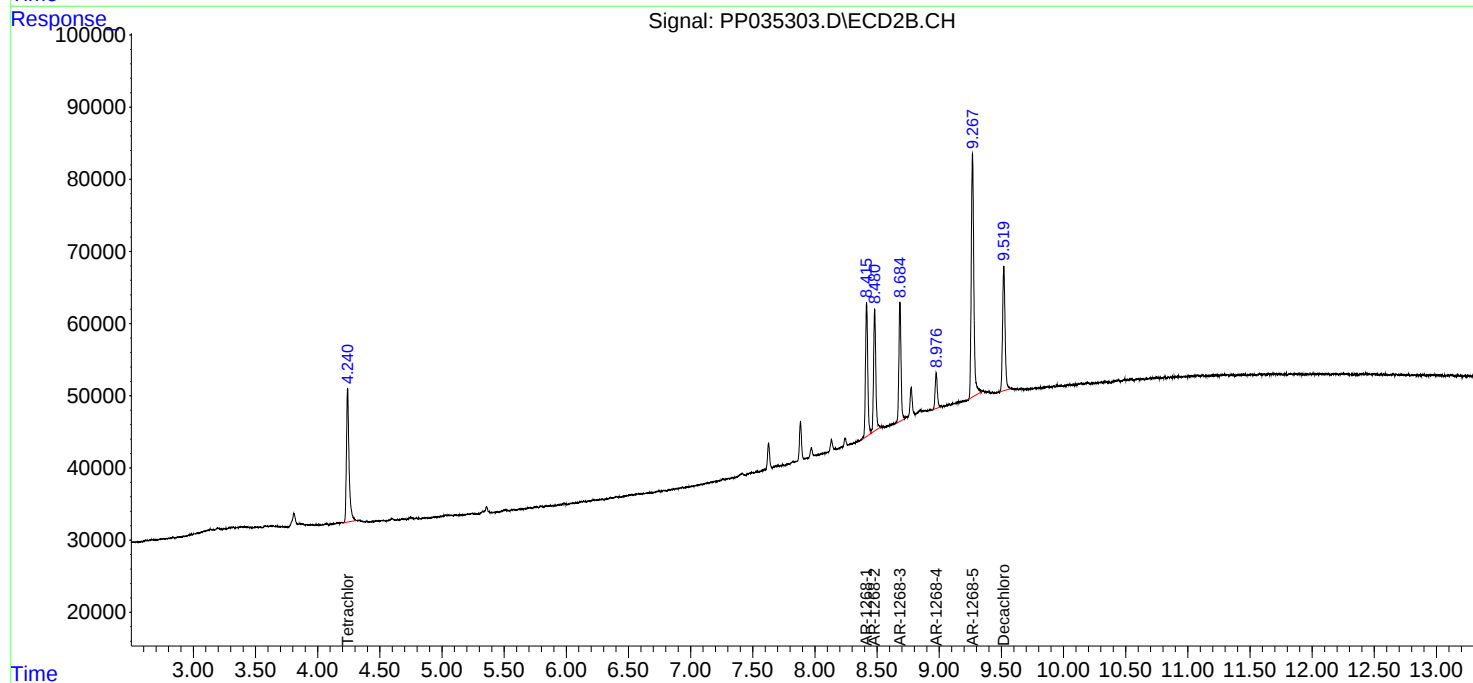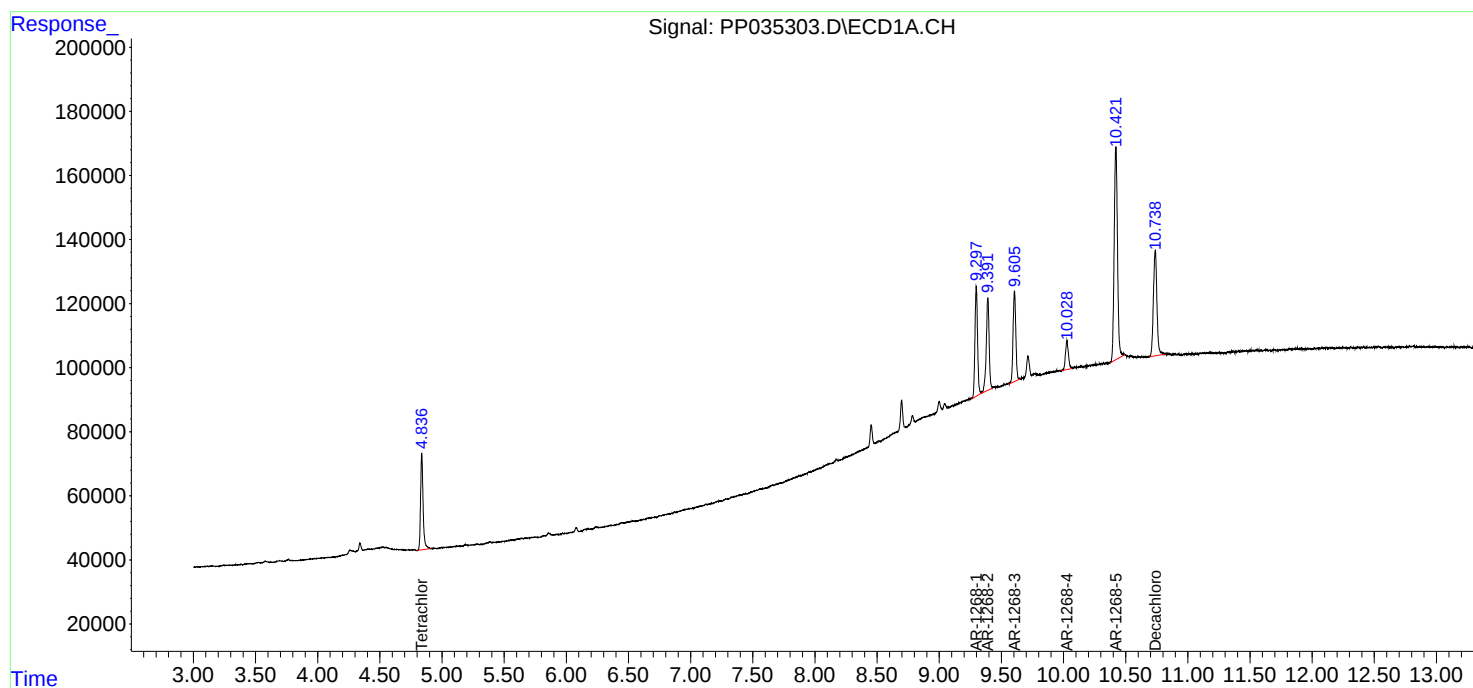

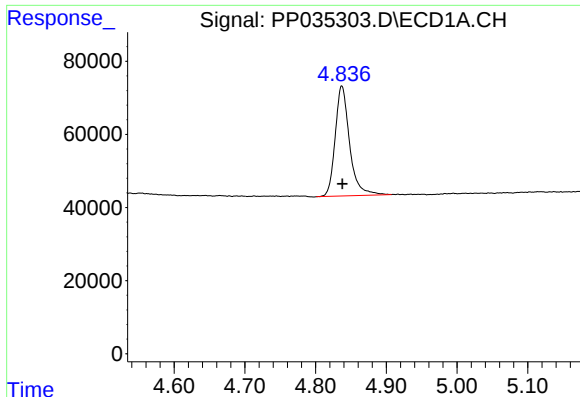


#1 Tetrachloro-m-xylene

R.T.: 4.837 min
Delta R.T.: -0.001 min
Response: 425214
Conc: 5.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Ankita
4/27/2021 11:16:03 AM

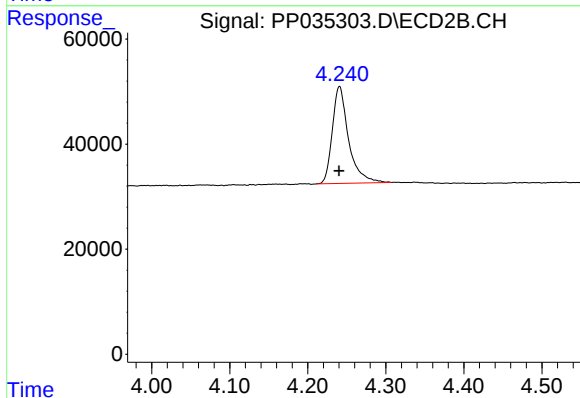


#1 Tetrachloro-m-xylene

R.T.: 4.241 min
Delta R.T.: 0.000 min
Response: 267719
Conc: 5.36 ng/ml

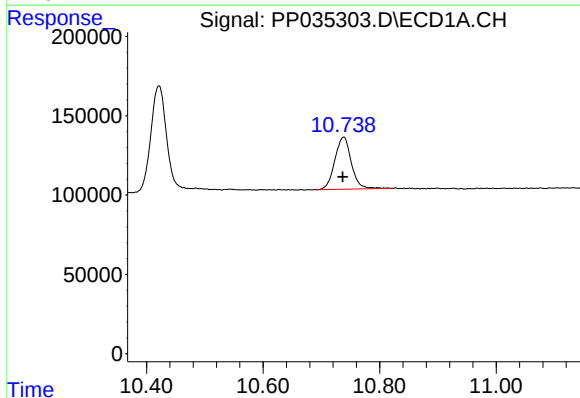


#2 Decachlorobiphenyl

R.T.: 10.738 min
Delta R.T.: 0.002 min
Response: 646699
Conc: 5.43 ng/ml

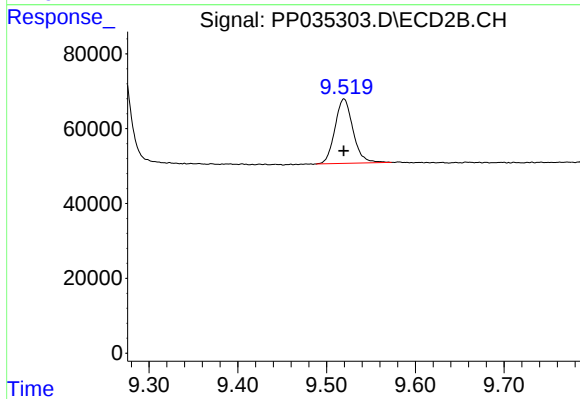

#2 Decachlorobiphenyl

R.T.: 9.520 min
Delta R.T.: 0.000 min
Response: 243647
Conc: 5.53 ng/ml

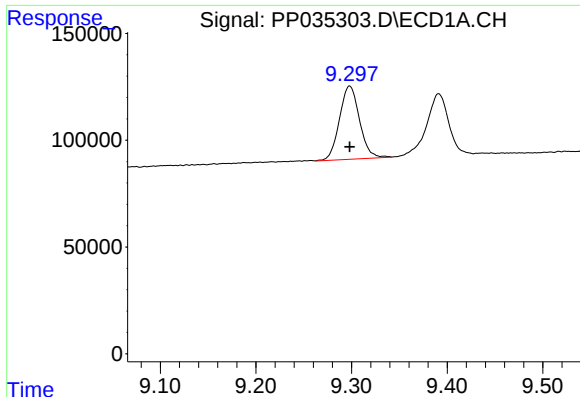


#41 AR-1268-1

R.T.: 9.297 min
Delta R.T.: 0.000 min
Response: 501100
Conc: 52.77 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Ankita
4/27/2021 11:16:03 AM

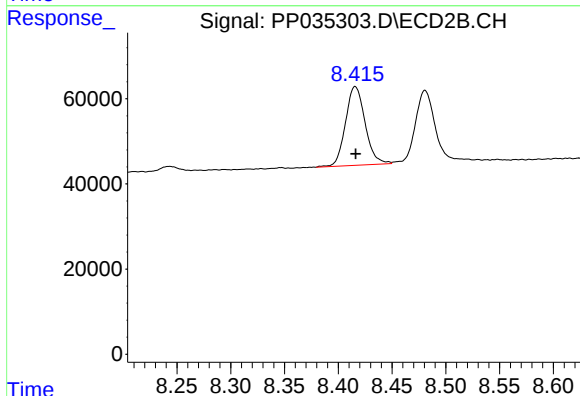


#41 AR-1268-1

R.T.: 8.415 min
Delta R.T.: 0.000 min
Response: 235254
Conc: 56.64 ng/ml m

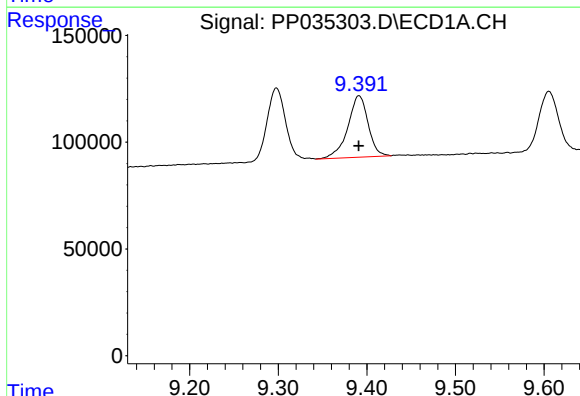


#42 AR-1268-2

R.T.: 9.391 min
Delta R.T.: 0.000 min
Response: 459410
Conc: 48.21 ng/ml

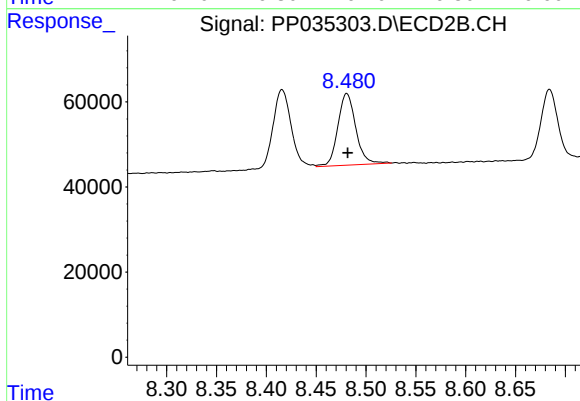

#42 AR-1268-2

R.T.: 8.481 min
Delta R.T.: 0.000 min
Response: 211180
Conc: 52.22 ng/ml

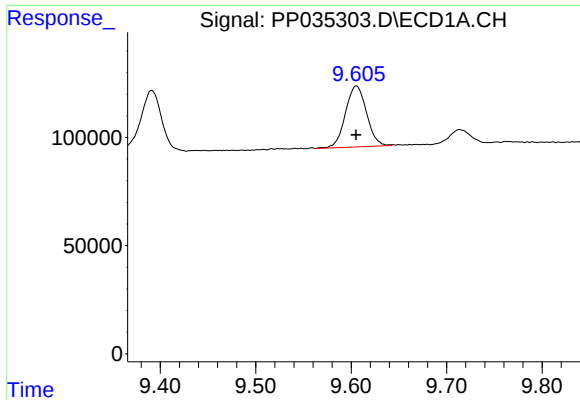


#43 AR-1268-3

R.T.: 9.605 min
Delta R.T.: 0.000 min
Response: 432002
Conc: 51.94 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Ankita
4/27/2021 11:16:03 AM

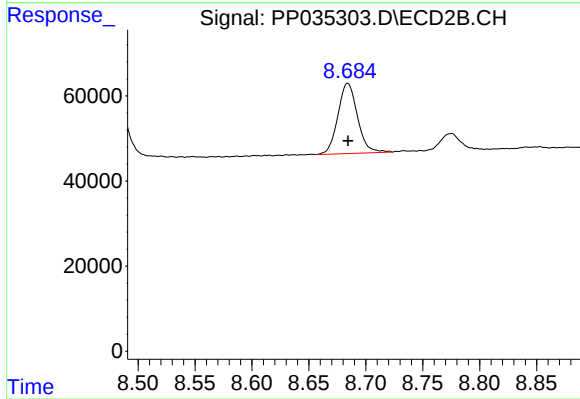


#43 AR-1268-3

R.T.: 8.684 min
Delta R.T.: 0.000 min
Response: 197447
Conc: 56.19 ng/ml m

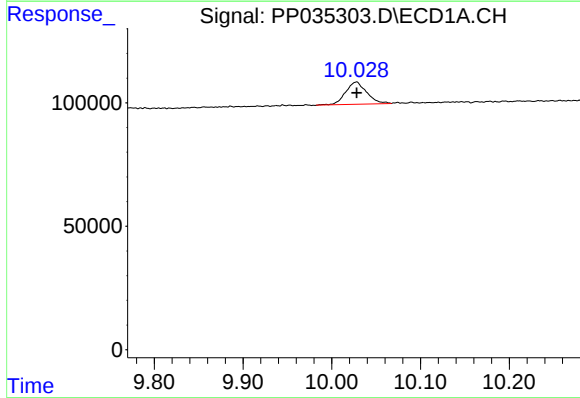


#44 AR-1268-4

R.T.: 10.028 min
Delta R.T.: 0.000 min
Response: 149125
Conc: 52.16 ng/ml

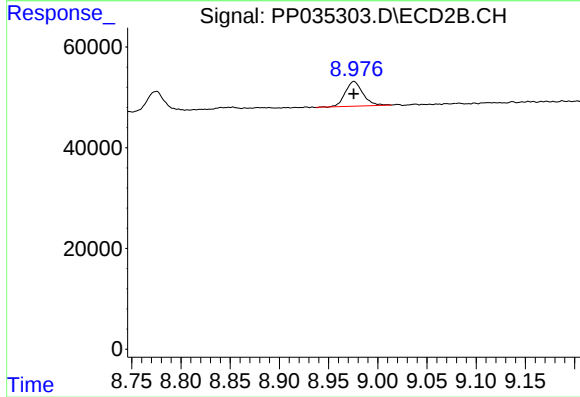

#44 AR-1268-4

R.T.: 8.976 min
Delta R.T.: 0.000 min
Response: 60852
Conc: 52.13 ng/ml

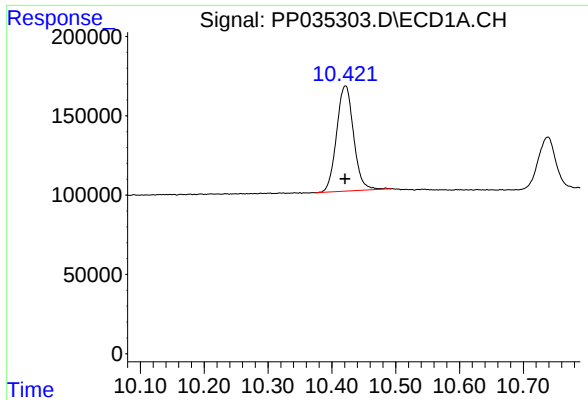


#45 AR-1268-5

R.T.: 10.421 min
Delta R.T.: 0.000 min
Response: 1228605
Conc: 49.02 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050

Manual Integrations
APPROVED

Ankita
4/27/2021 11:16:03 AM

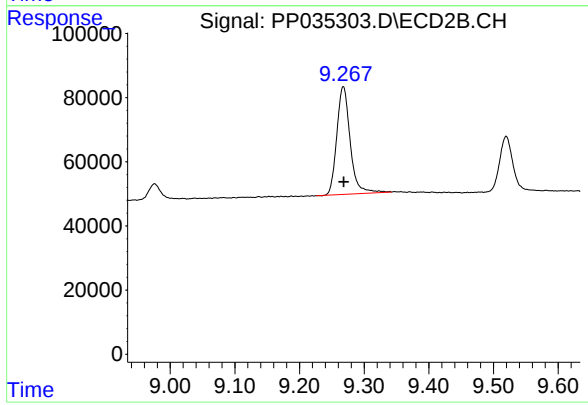

#45 AR-1268-5

R.T.: 9.268 min
Delta R.T.: 0.000 min
Response: 482903
Conc: 50.09 ng/ml