

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042622\
 Data File : PP046686.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2022 03:35
 Operator : YP\AJ
 Sample : N2551-03
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 20220377-096-21-03-ELUTRIATE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/27/2022
 Supervised By :mohammad ahmed 04/27/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 05:16:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 22 19:00:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.864	2.639f	41797896	36854694	17.315	11.235m#
2) SA Decachlor...	9.945	6.945f	15447570	28617695	10.498	11.997m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042622\
Data File : PP046686.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2022 03:35
Operator : YP\AJ
Sample : N2551-03
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
20220377-096-21-03-ELUTRIATE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/27/2022
Supervised By :mohammad ahmed 04/27/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 05:16:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 22 19:00:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

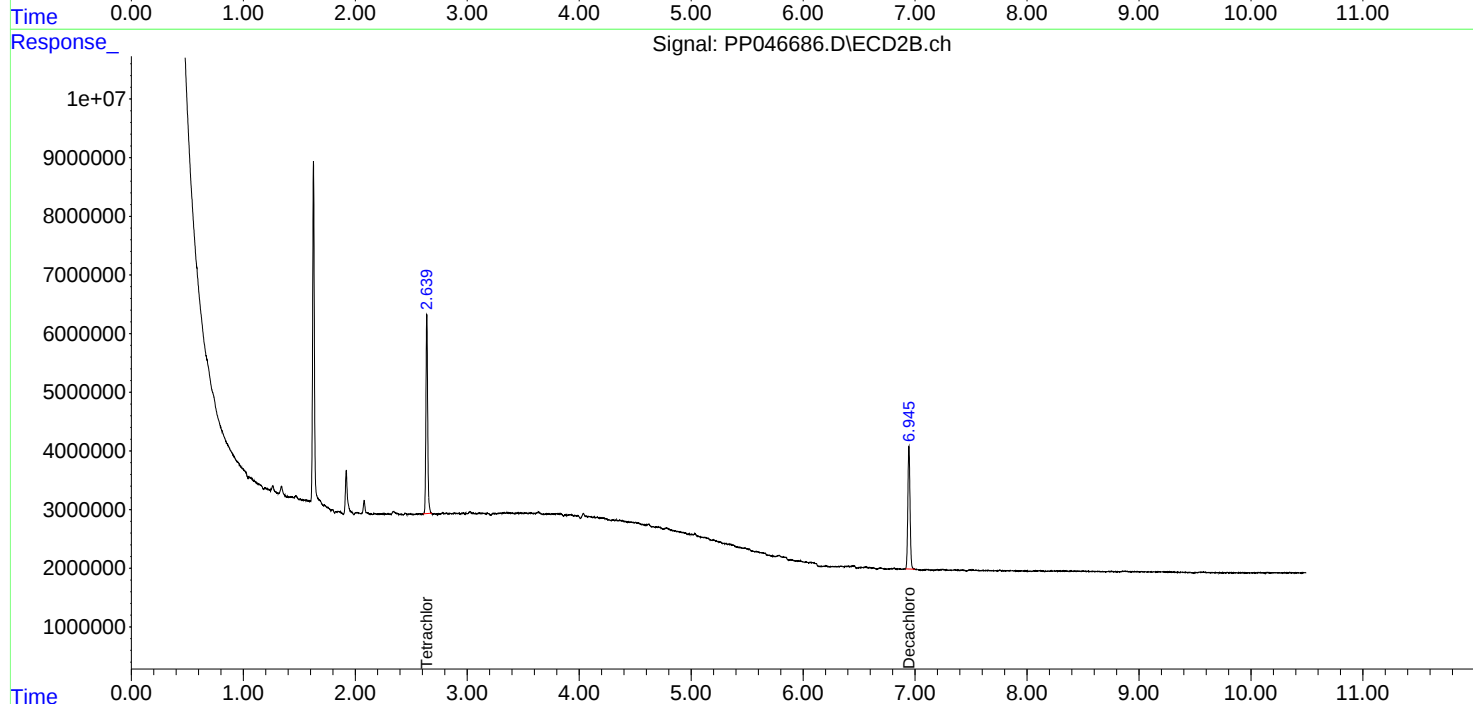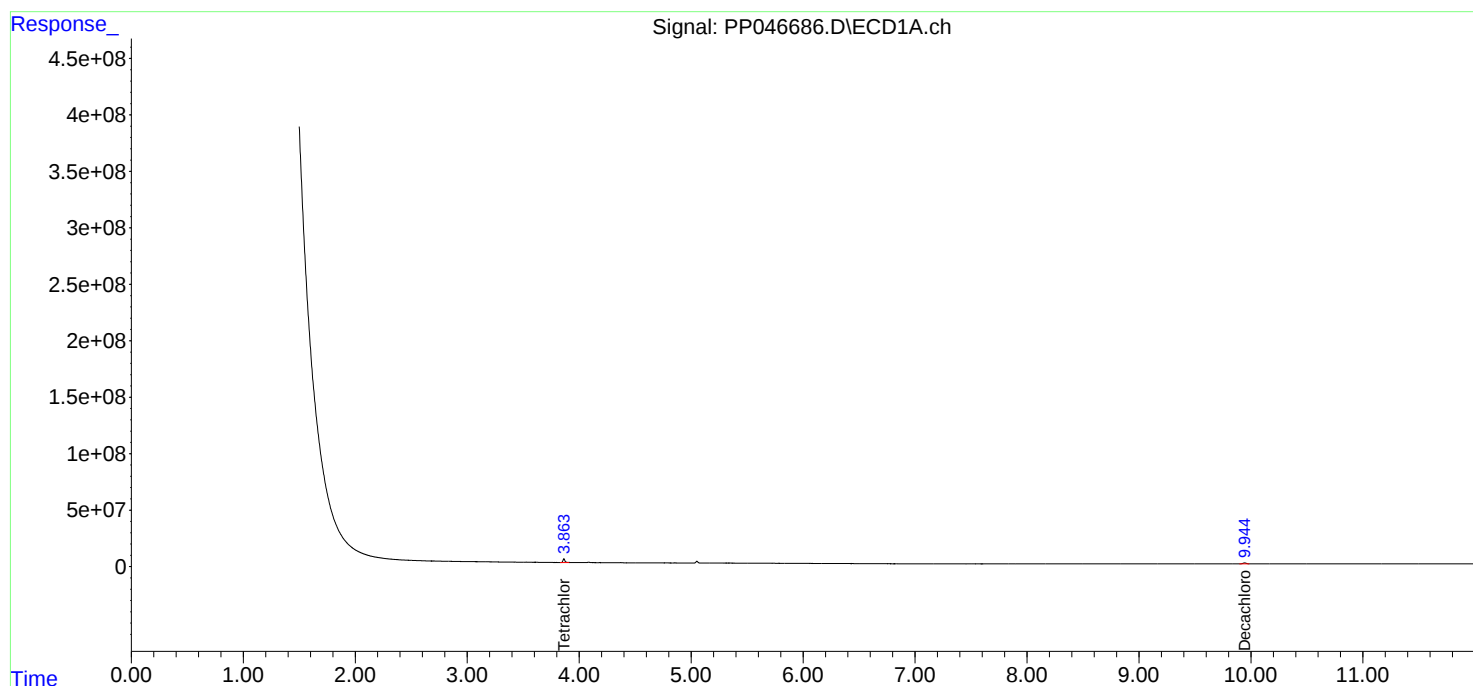

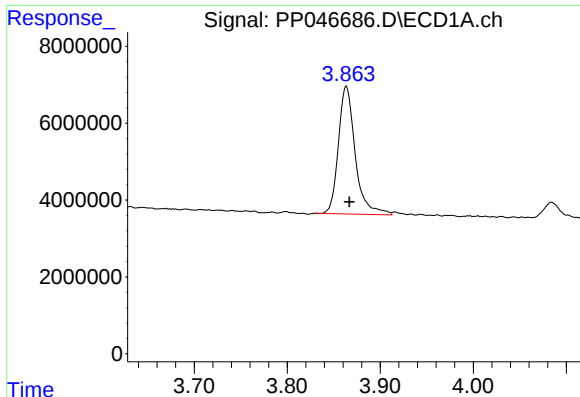


#1 Tetrachloro-m-xylene

R.T.: 3.864 min
Delta R.T.: -0.003 min
Response: 41797896
Conc: 17.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
20220377-096-21-03-ELUTRIATE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/27/2022
Supervised By :mohammad ahmed 04/27/2022

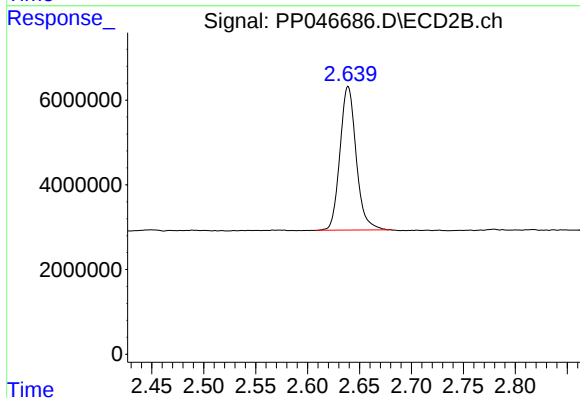


#1 Tetrachloro-m-xylene

R.T.: 2.639 min
Delta R.T.: -0.490 min
Response: 36854694
Conc: 11.23 ng/ml m

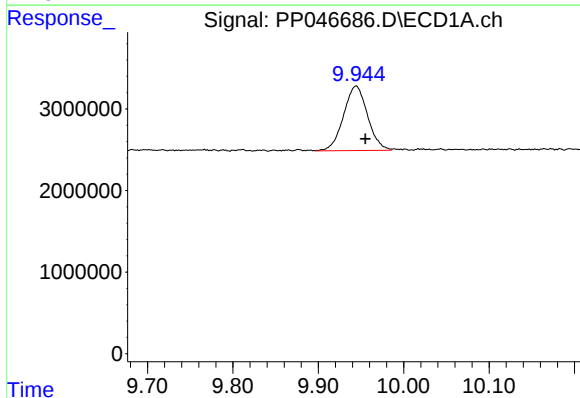

#2 Decachlorobiphenyl

R.T.: 9.945 min
Delta R.T.: -0.011 min
Response: 15447570
Conc: 10.50 ng/ml

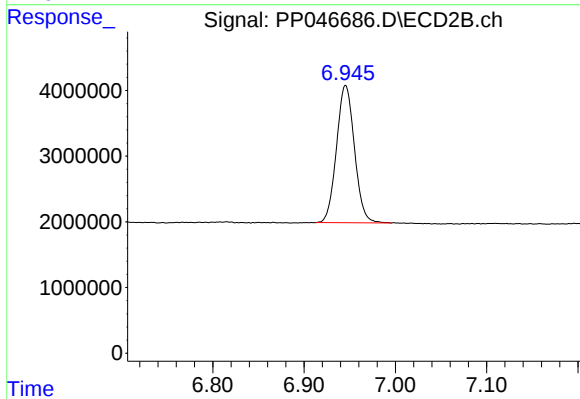

#2 Decachlorobiphenyl

R.T.: 6.945 min
Delta R.T.: -1.511 min
Response: 28617695
Conc: 12.00 ng/ml m