

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042719\
 Data File : PP030030.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Apr 2019 23:44
 Operator : EI/SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 03:18:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042519.M
 Quant Title : 8080.M
 QLast Update : Fri Apr 26 10:04:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

5) T	DICAMBA	12.456	0.000	504491	0	0.247	N.D.	#
15) T	Picloram	17.798	18.391	1620917	794597	0.457	0.295	#
16) T	DCPA	18.361	18.237	992464	667512	0.279	0.246	



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042719\
Data File : PP030030.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Apr 2019 23:44
Operator : EI/SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 03:18:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042519.M
Quant Title : 8080.M
QLast Update : Fri Apr 26 10:04:13 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

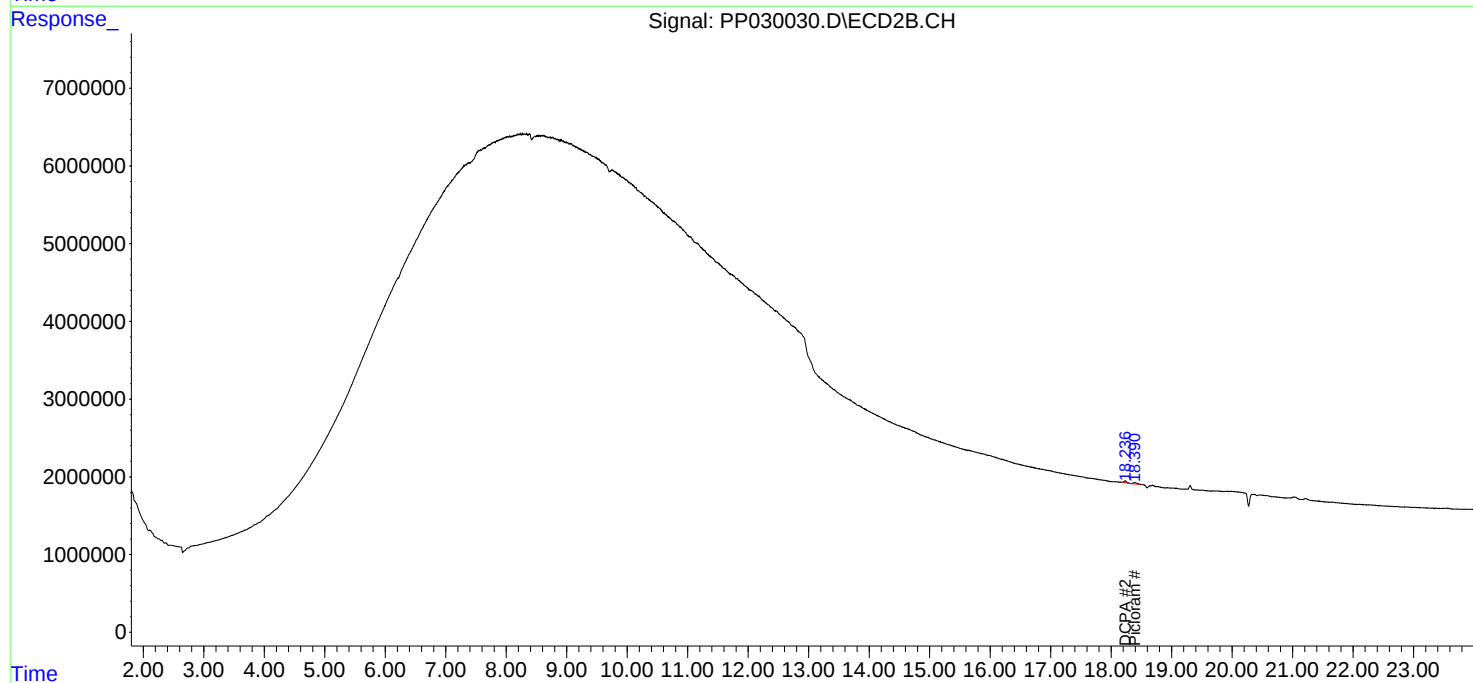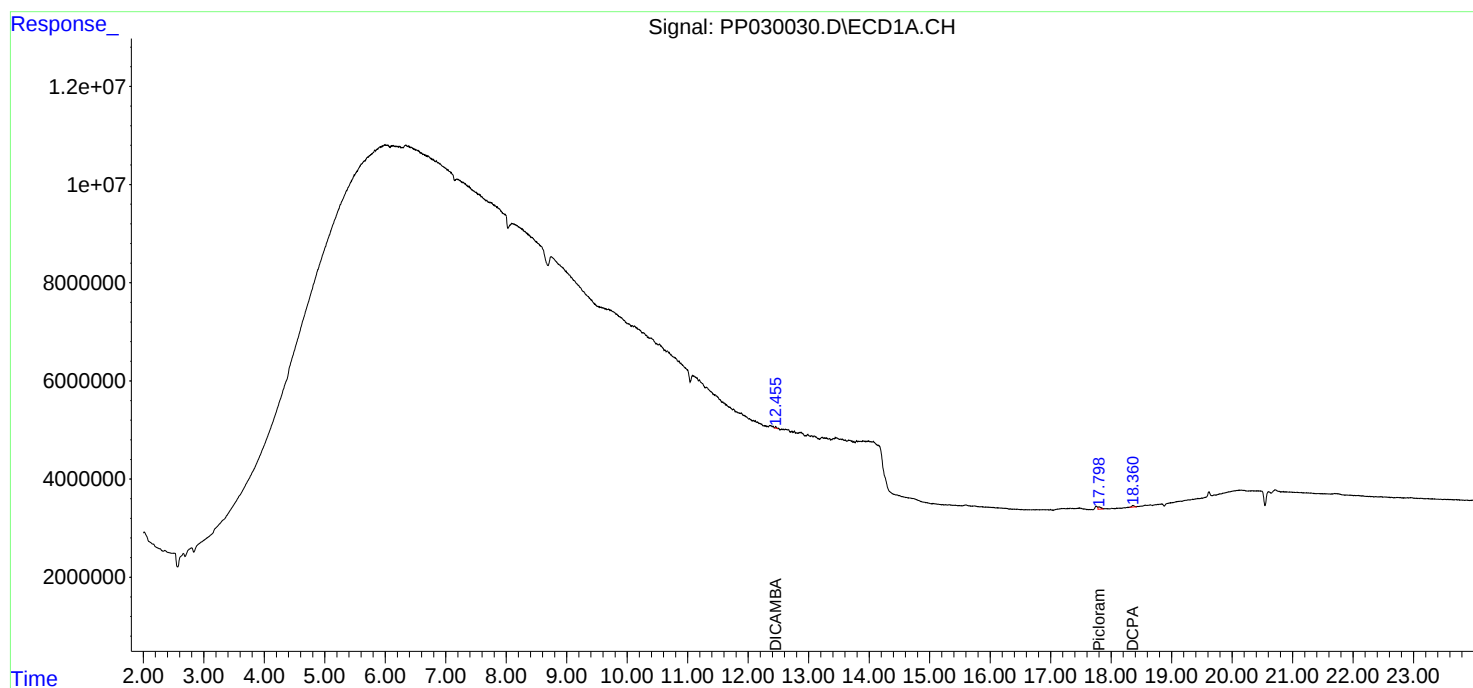


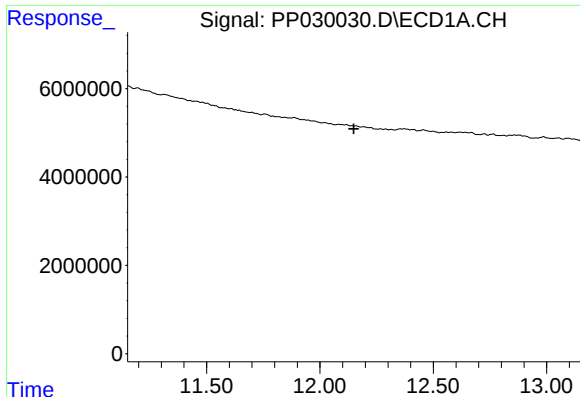

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 12.149 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

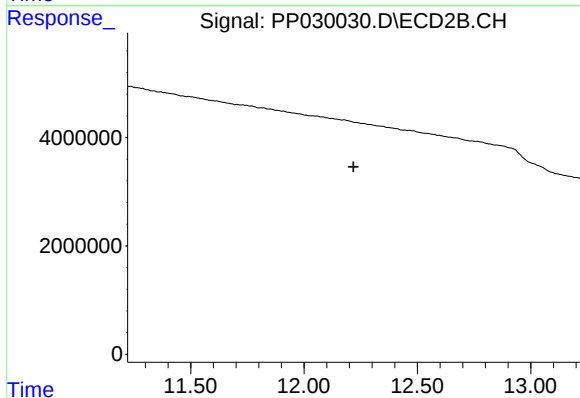


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 12.219 min
Response: 0
Conc: N.D.

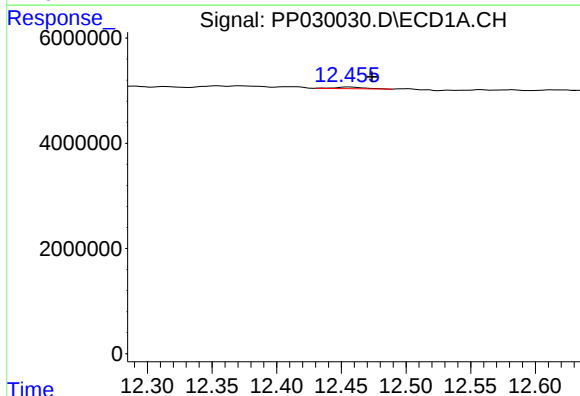


#5 DICAMBA

R.T.: 12.456 min
Delta R.T.: -0.018 min
Response: 504491
Conc: 0.25 ng/ml

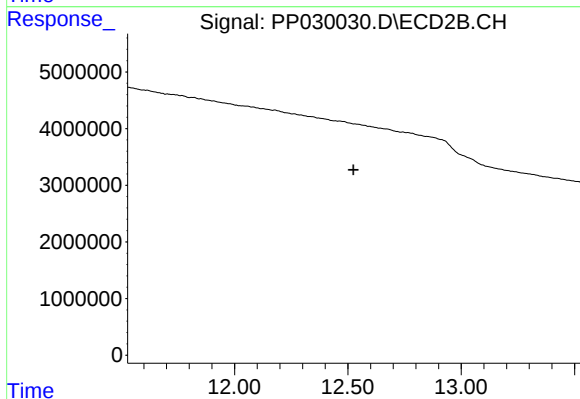

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 12.525 min
Response: 0
Conc: N.D.

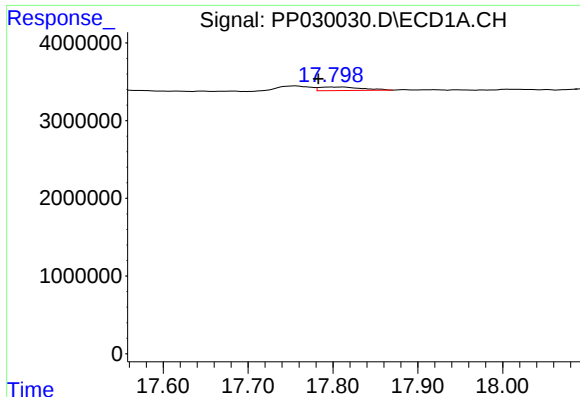

#15 Picloram


R.T.: 17.798 min
Delta R.T.: 0.016 min
Response: 1620917
Conc: 0.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

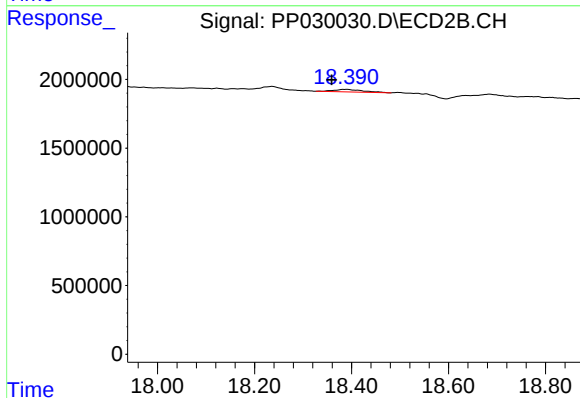


#15 Picloram

R.T.: 18.391 min
Delta R.T.: 0.031 min
Response: 794597
Conc: 0.29 ng/ml

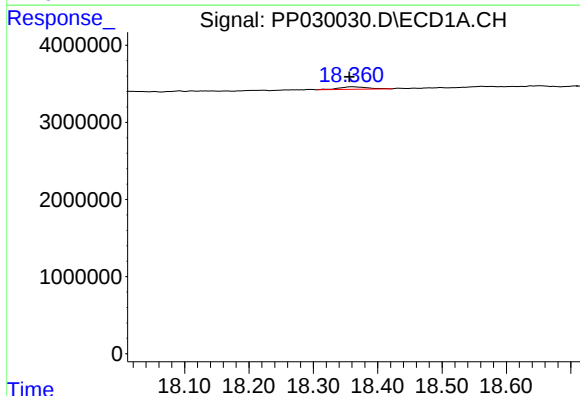

#16 DCPA

R.T.: 18.361 min
Delta R.T.: 0.005 min
Response: 992464
Conc: 0.28 ng/ml

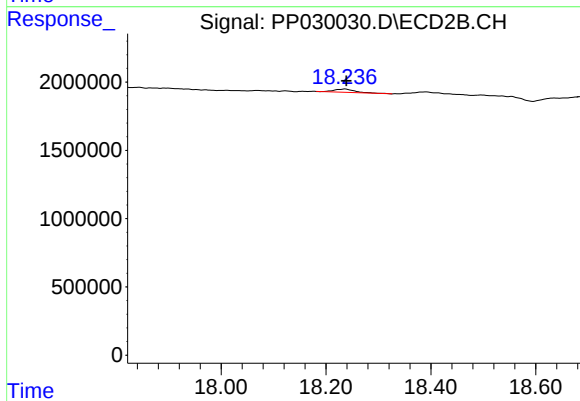

#16 DCPA

R.T.: 18.237 min
Delta R.T.: -0.002 min
Response: 667512
Conc: 0.25 ng/ml