

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042719\
 Data File : PP030040.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Apr 2019 5:08
 Operator : EI/SJ
 Sample : MDL-BL-WATER-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-BL-WATER-07

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 06:42:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042519.M
 Quant Title : 8080.M
 QLast Update : Fri Apr 26 10:04:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	12.144	12.215	201.3E6	133.0E6	452.681	332.338 #
Target Compounds							
16) T	DCPA	18.348	18.235	921050	727401	0.259	0.268



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042719\
Data File : PP030040.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Apr 2019 5:08
Operator : EI/SJ
Sample : MDL-BL-WATER-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-BL-WATER-07

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 06:42:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042519.M
Quant Title : 8080.M
QLast Update : Fri Apr 26 10:04:13 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

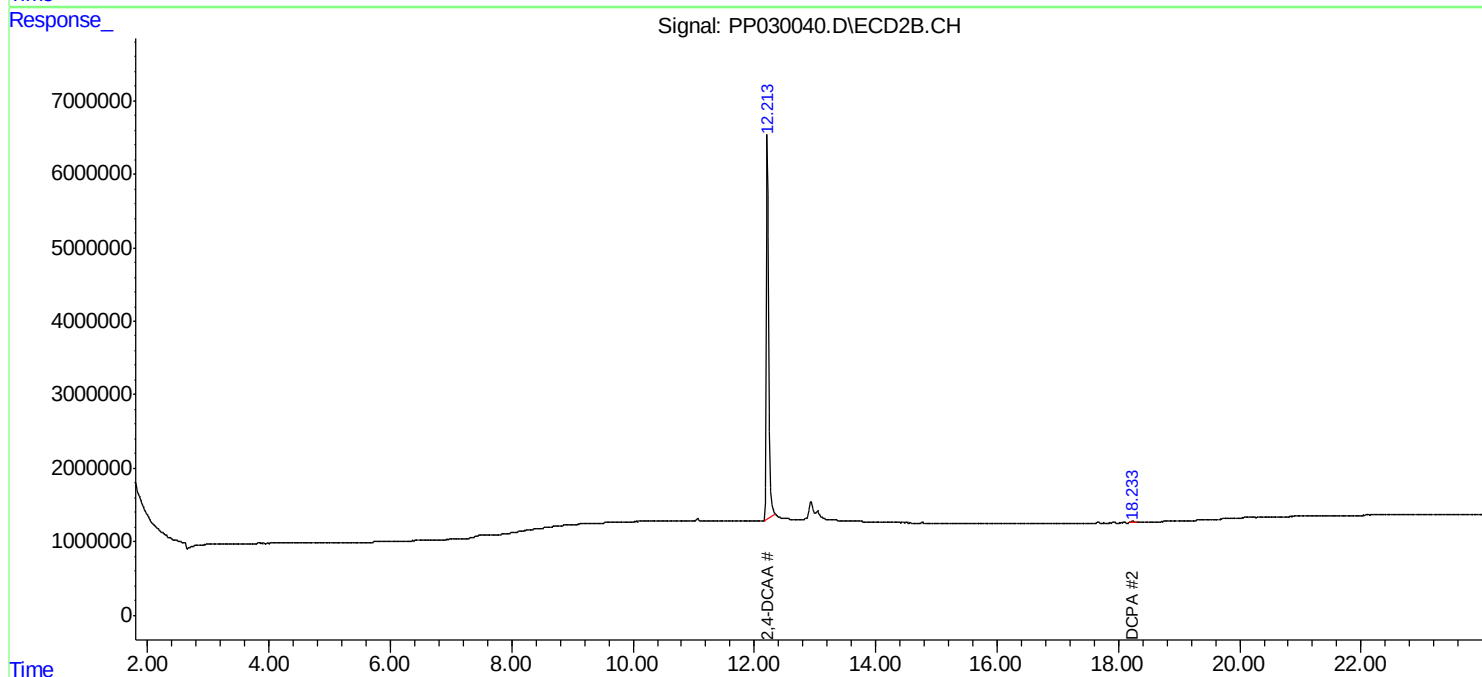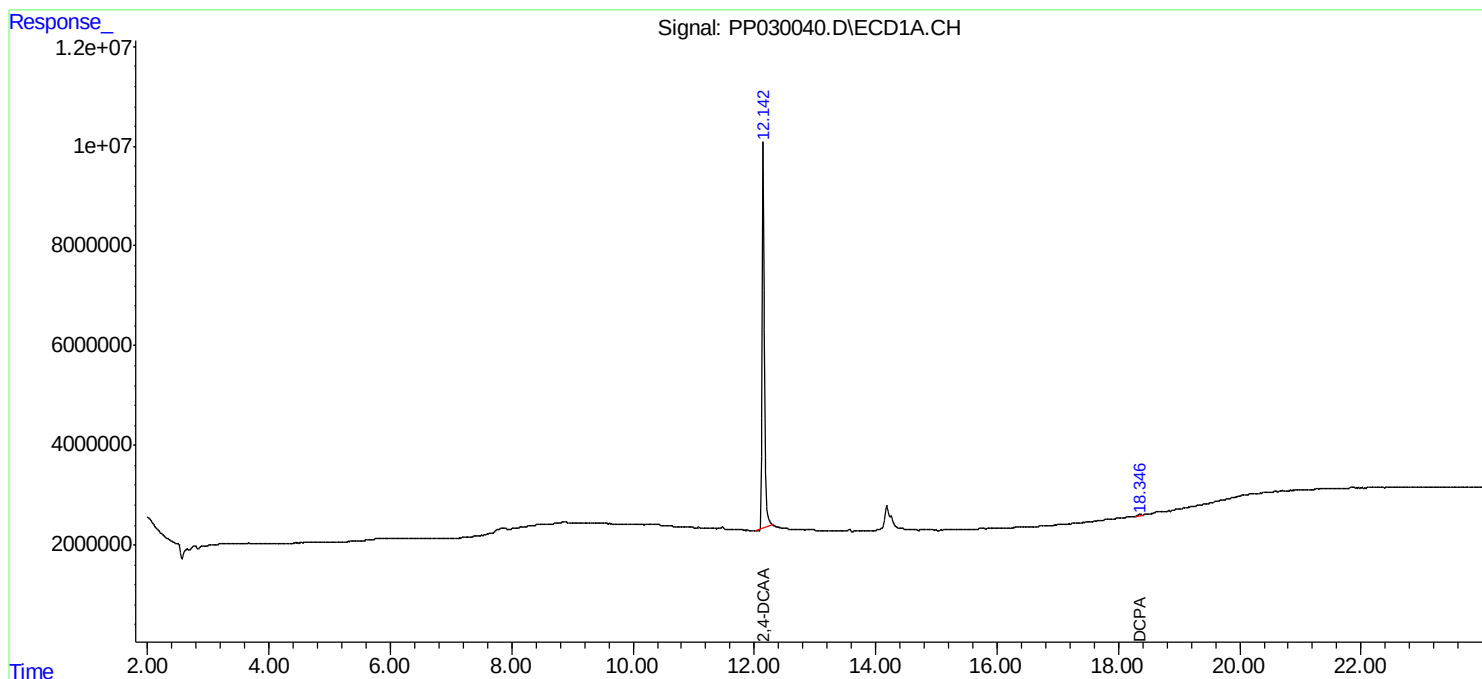


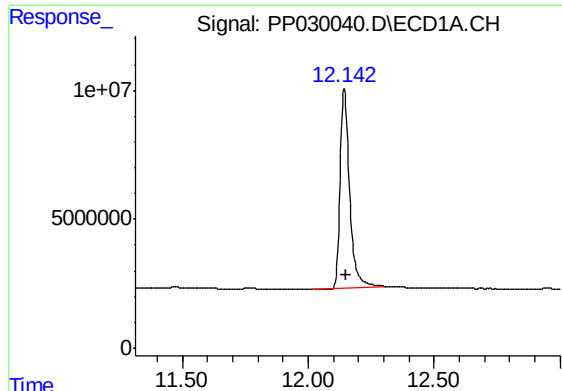

#4 2,4-DCAA


R.T.: 12.144 min
Delta R.T.: -0.005 min
Response: 201305003
Conc: 452.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-BL-WATER-07

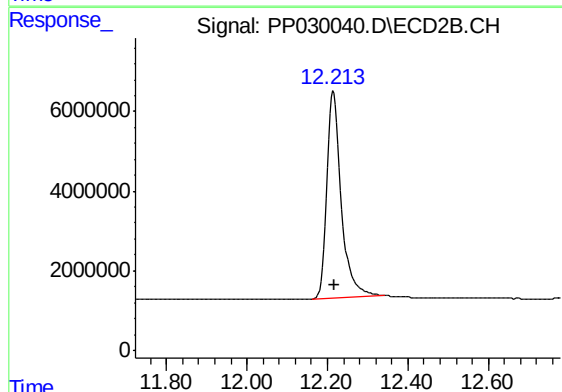


#4 2,4-DCAA

R.T.: 12.215 min
Delta R.T.: -0.004 min
Response: 133046928
Conc: 332.34 ng/ml

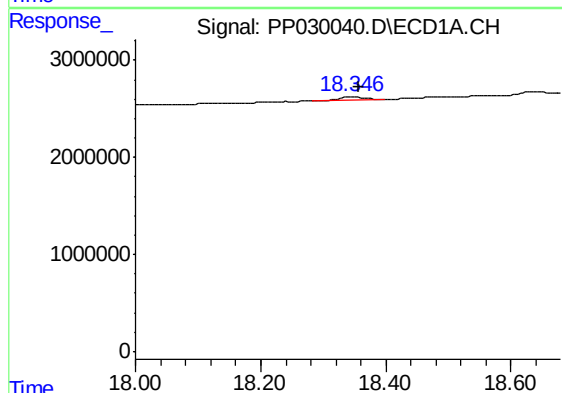

#16 DCPA

R.T.: 18.348 min
Delta R.T.: -0.008 min
Response: 921050
Conc: 0.26 ng/ml

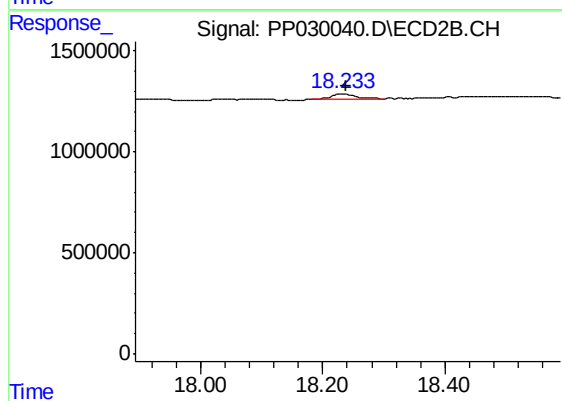

#16 DCPA

R.T.: 18.235 min
Delta R.T.: -0.004 min
Response: 727401
Conc: 0.27 ng/ml