

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042721\
 Data File : PP035333.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Apr 2021 16:32
 Operator : DD\AJ
 Sample : M2158-04 20X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 17:33:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 27 07:44:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.836	4.238	93336	57683	1.152	1.105
2) SA Decachlor...	10.735	9.518	73659	34420	1.031	1.247
Target Compounds						
34) L7 AR-1260-4	8.656f	0.000	53594	0	16.052	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042721\
Data File : PP035333.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Apr 2021 16:32
Operator : DD\AJ
Sample : M2158-04 20X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 17:33:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042621.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 27 07:44:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

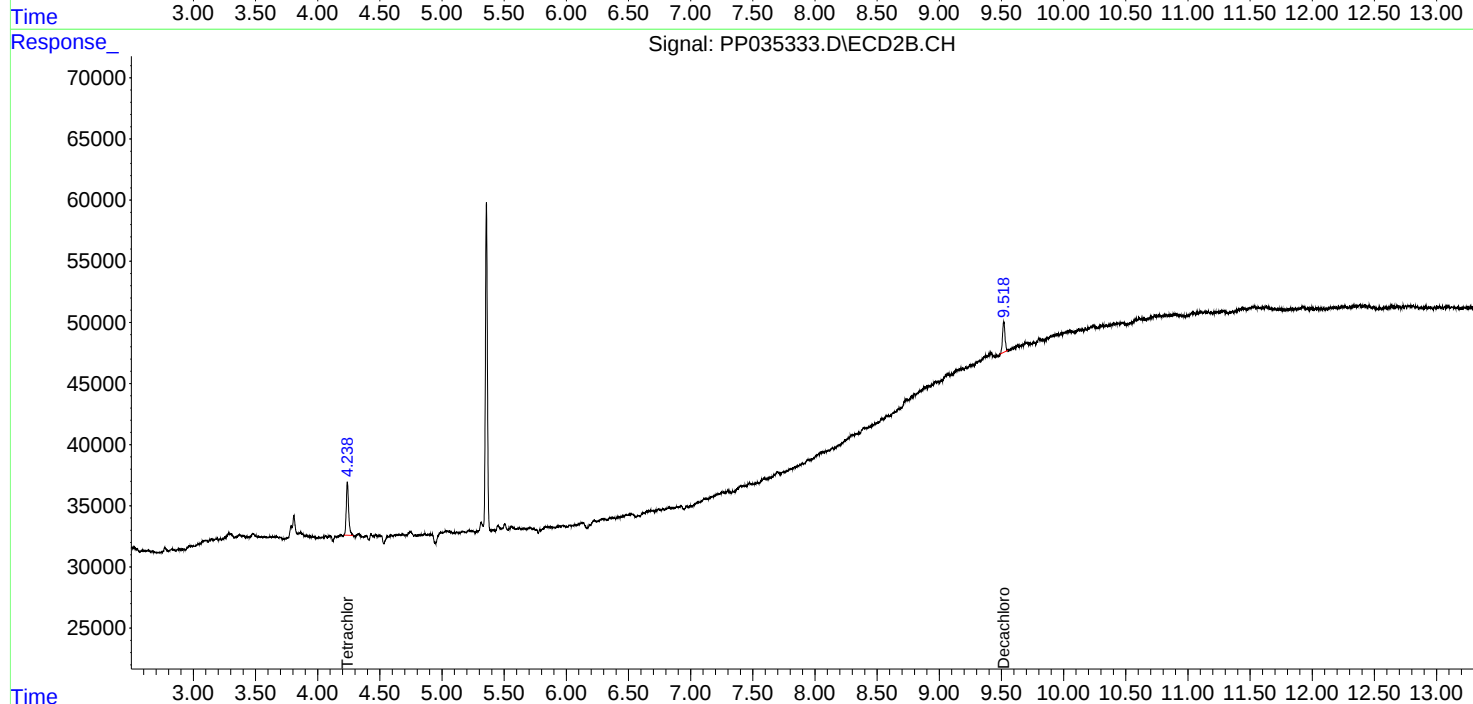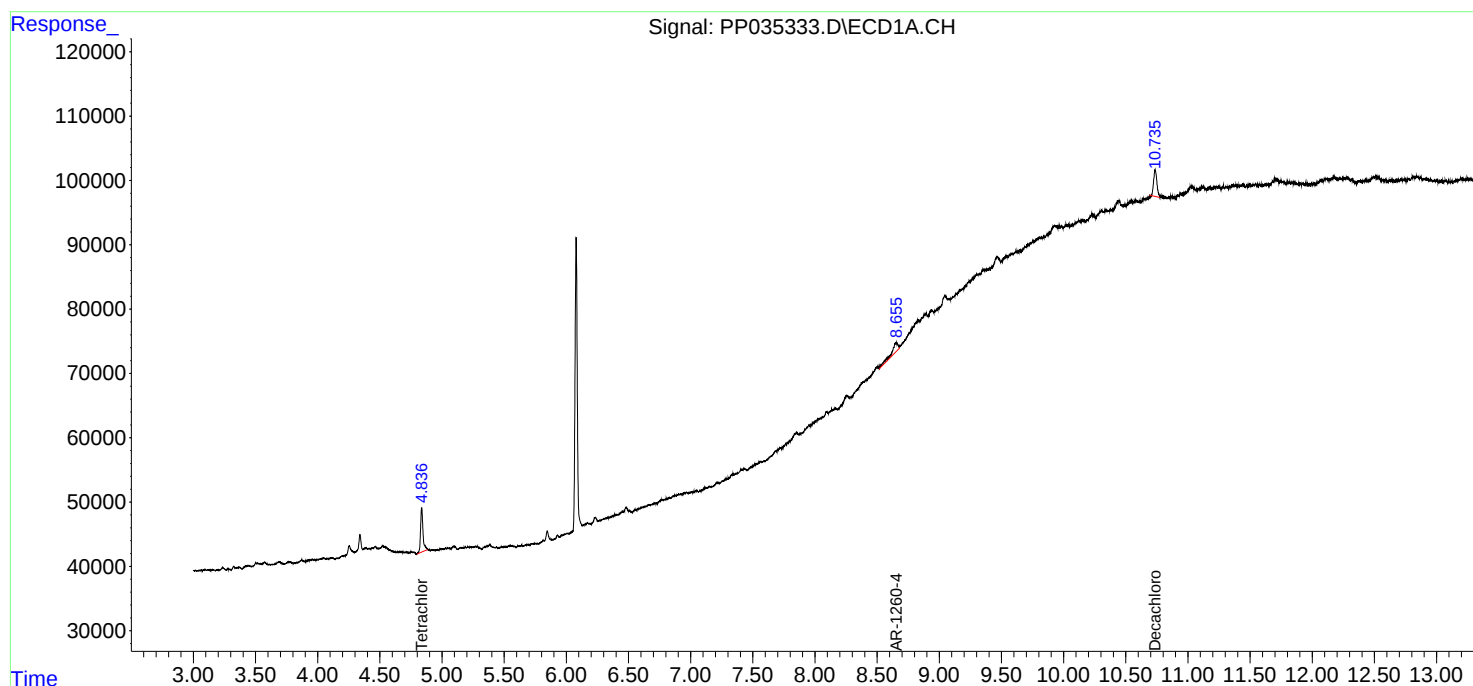


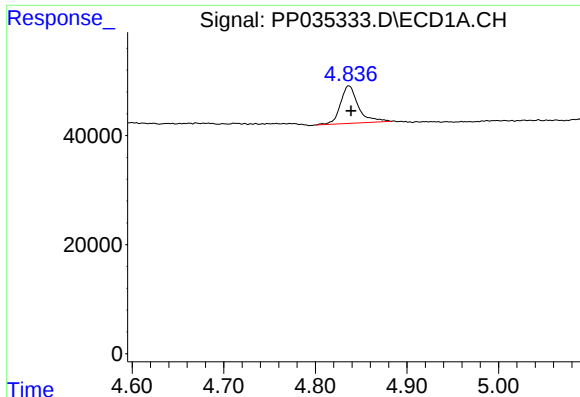

#1 Tetrachloro-m-xylene


R.T.: 4.836 min
Delta R.T.: -0.003 min
Response: 93336
Conc: 1.15 ng/ml

Instrument :
ECD_P
ClientSampleId :

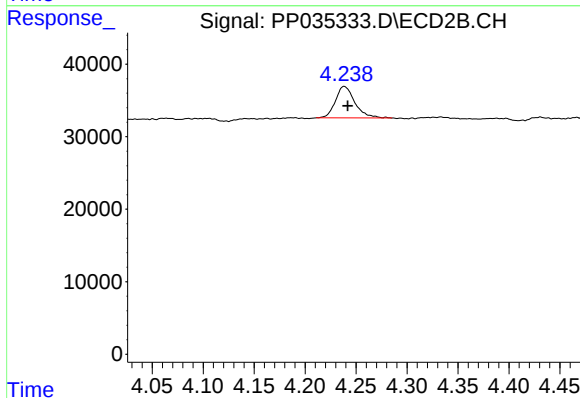


#1 Tetrachloro-m-xylene

R.T.: 4.238 min
Delta R.T.: -0.003 min
Response: 57683
Conc: 1.10 ng/ml

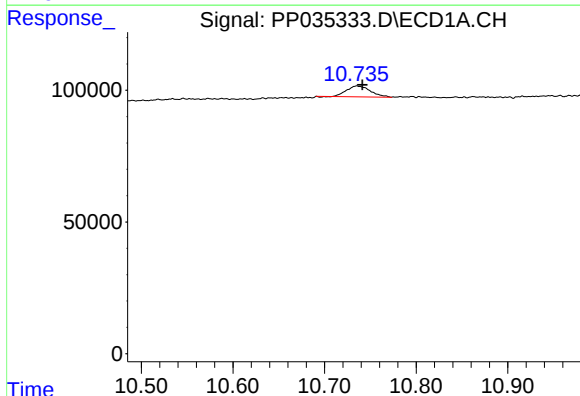


#2 Decachlorobiphenyl

R.T.: 10.735 min
Delta R.T.: -0.006 min
Response: 73659
Conc: 1.03 ng/ml

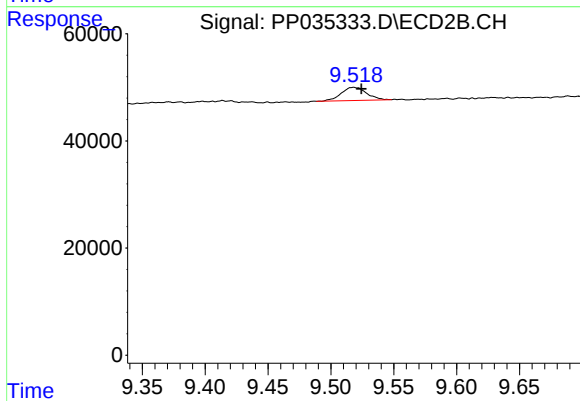

#2 Decachlorobiphenyl


R.T.: 9.518 min
Delta R.T.: -0.006 min
Response: 34420
Conc: 1.25 ng/ml

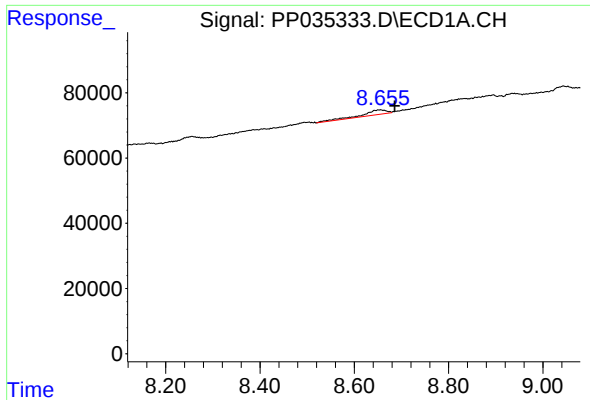

#34 AR-1260-4

R.T.: 8.656 min
Delta R.T.: -0.030 min
Response: 53594
Conc: 16.05 ng/ml

Instrument :
ECD_P
ClientSampleId :

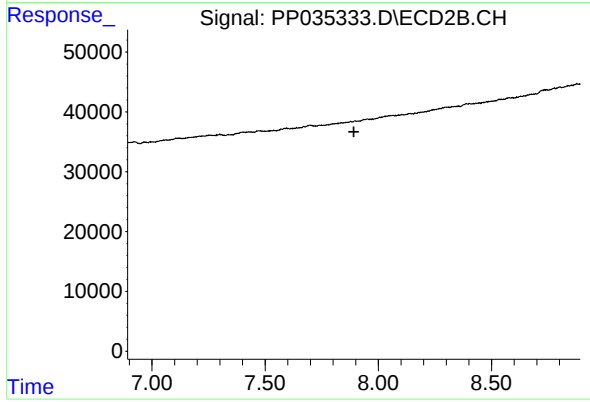

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.892 min
Response: 0
Conc: N.D.