

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042721\
 Data File : PP035332.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Apr 2021 16:15
 Operator : DD\AJ
 Sample : M2158-03 20X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KQA103H-END-1-3

Manual Integrations
 APPROVED

Ankita
 4/28/2021 3:39:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 17:33:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 27 07:44:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.836	4.237	68748	46348	0.849m	0.888
2) SA Decachlor...	10.738	9.519	78281	31360	1.096	1.136

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042721\
Data File : PP035332.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Apr 2021 16:15
Operator : DD\AJ
Sample : M2158-03 20X
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KQA103H-END-1-3


Manual Integrations
APPROVED

Ankita
4/28/2021 3:39:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 17:33:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042621.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 27 07:44:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

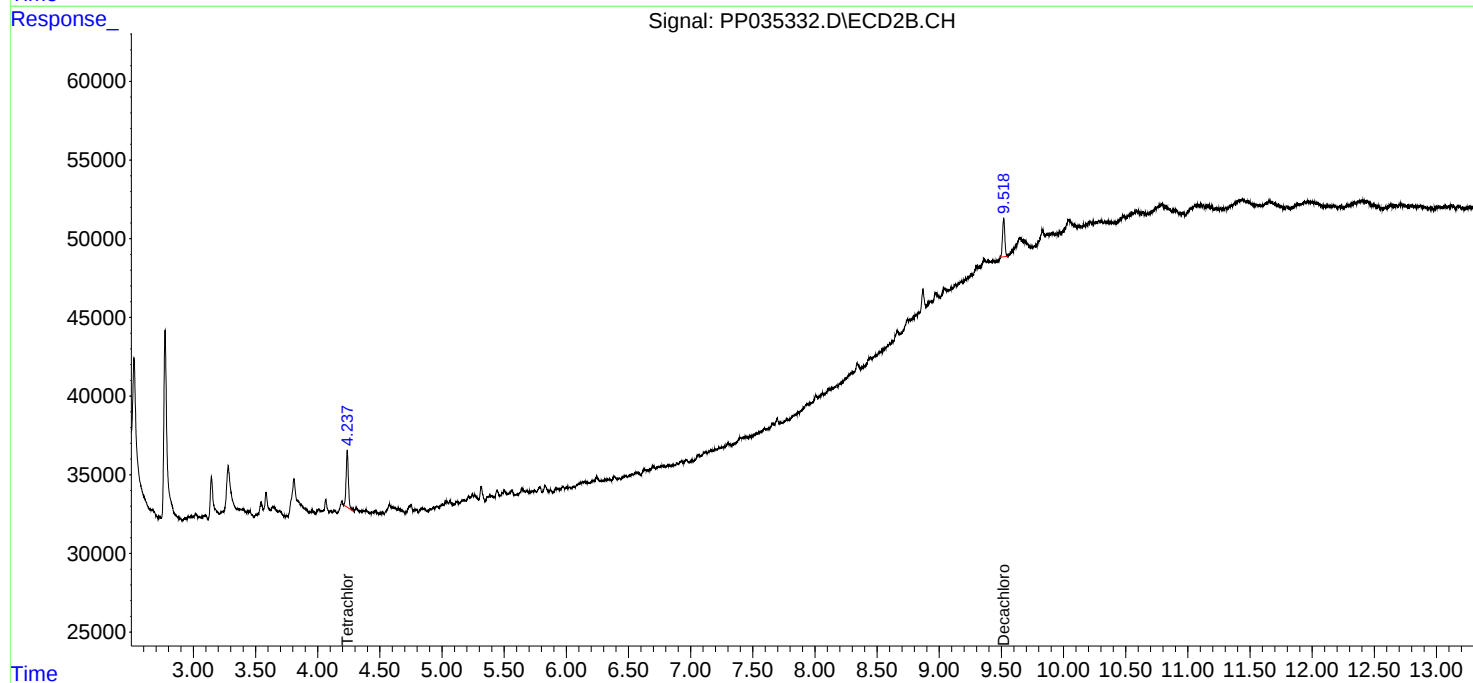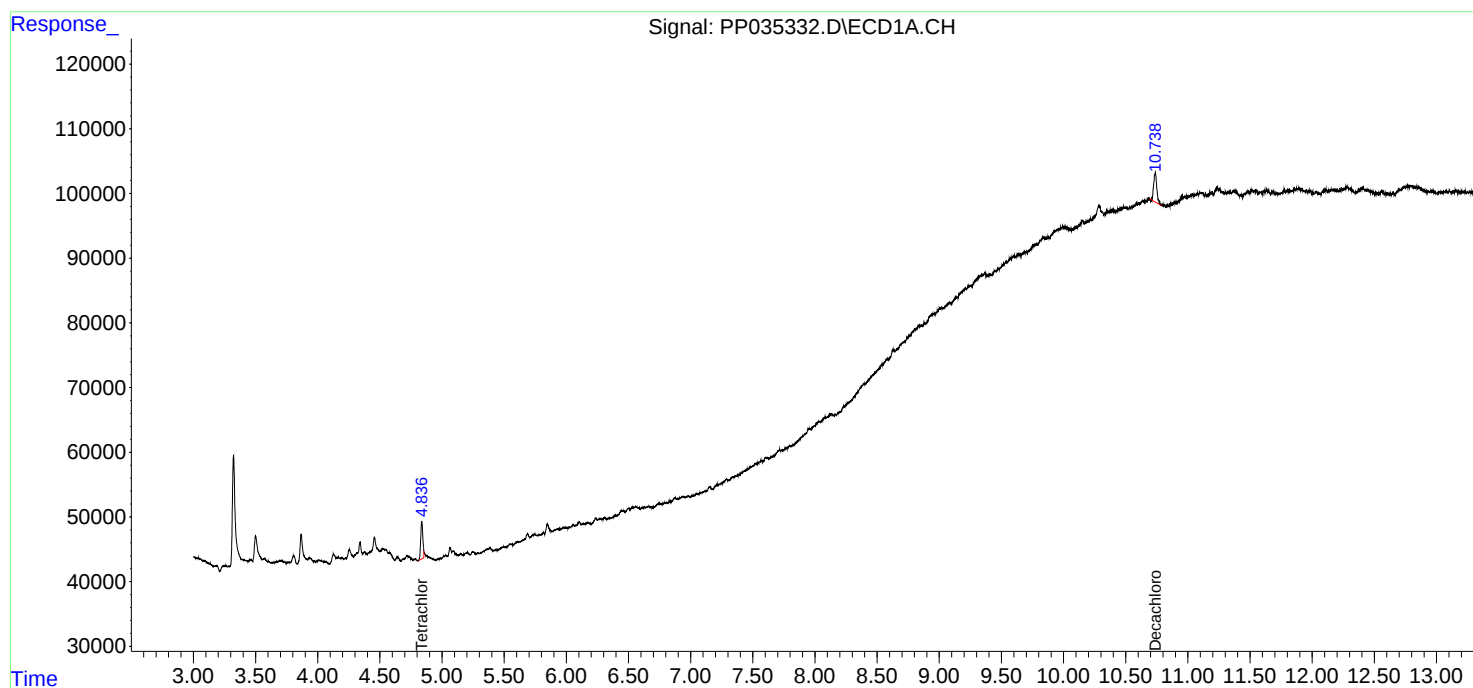

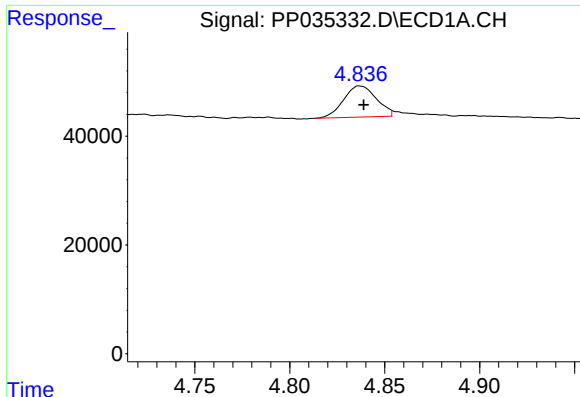


#1 Tetrachloro-m-xylene

R.T.: 4.836 min
Delta R.T.: -0.003 min
Response: 68748
Conc: 0.85 ng/ml m

Instrument :
ECD_P
ClientSampleId :
KQA103H-END-1-3


Manual Integrations
APPROVED

Ankita
4/28/2021 3:39:46 PM

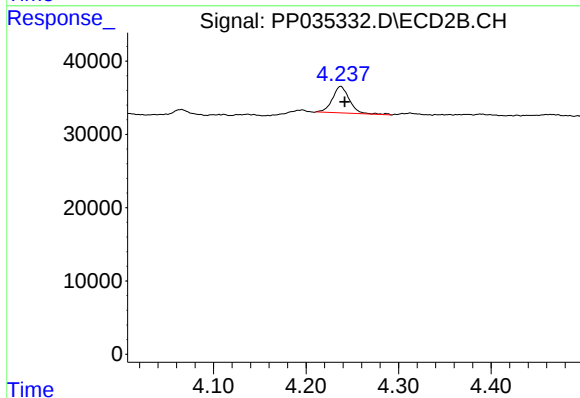


#1 Tetrachloro-m-xylene

R.T.: 4.237 min
Delta R.T.: -0.004 min
Response: 46348
Conc: 0.89 ng/ml

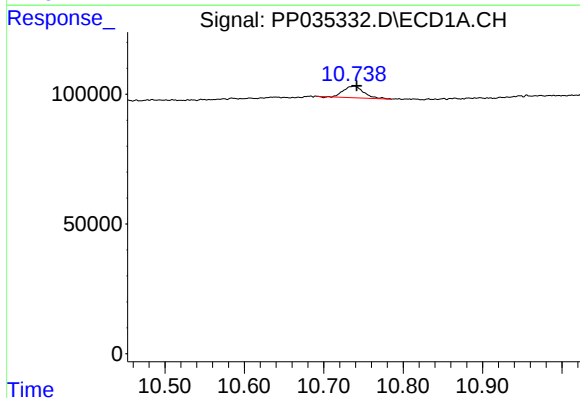

#2 Decachlorobiphenyl

R.T.: 10.738 min
Delta R.T.: -0.003 min
Response: 78281
Conc: 1.10 ng/ml

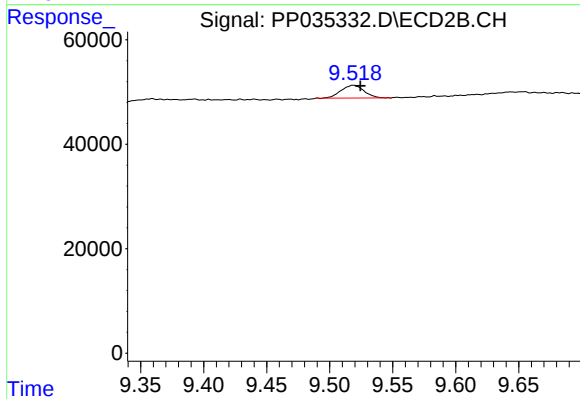

#2 Decachlorobiphenyl

R.T.: 9.519 min
Delta R.T.: -0.006 min
Response: 31360
Conc: 1.14 ng/ml