

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042721\
 Data File : PP035335.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Apr 2021 17:05
 Operator : DD\AJ
 Sample : M2158-06 20X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KQA103H-END-2-3

Manual Integrations
 APPROVED

Ankita
 4/28/2021 3:39:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 17:34:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 27 07:44:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.835	4.238	79245	50047	0.978m	0.958
2) SA Decachlor...	10.734	9.518	77952	28363	1.091	1.027m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042721\
Data File : PP035335.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Apr 2021 17:05
Operator : DD\AJ
Sample : M2158-06 20X
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KQA103H-END-2-3


Manual Integrations
APPROVED

Ankita
4/28/2021 3:39:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 17:34:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042621.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 27 07:44:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

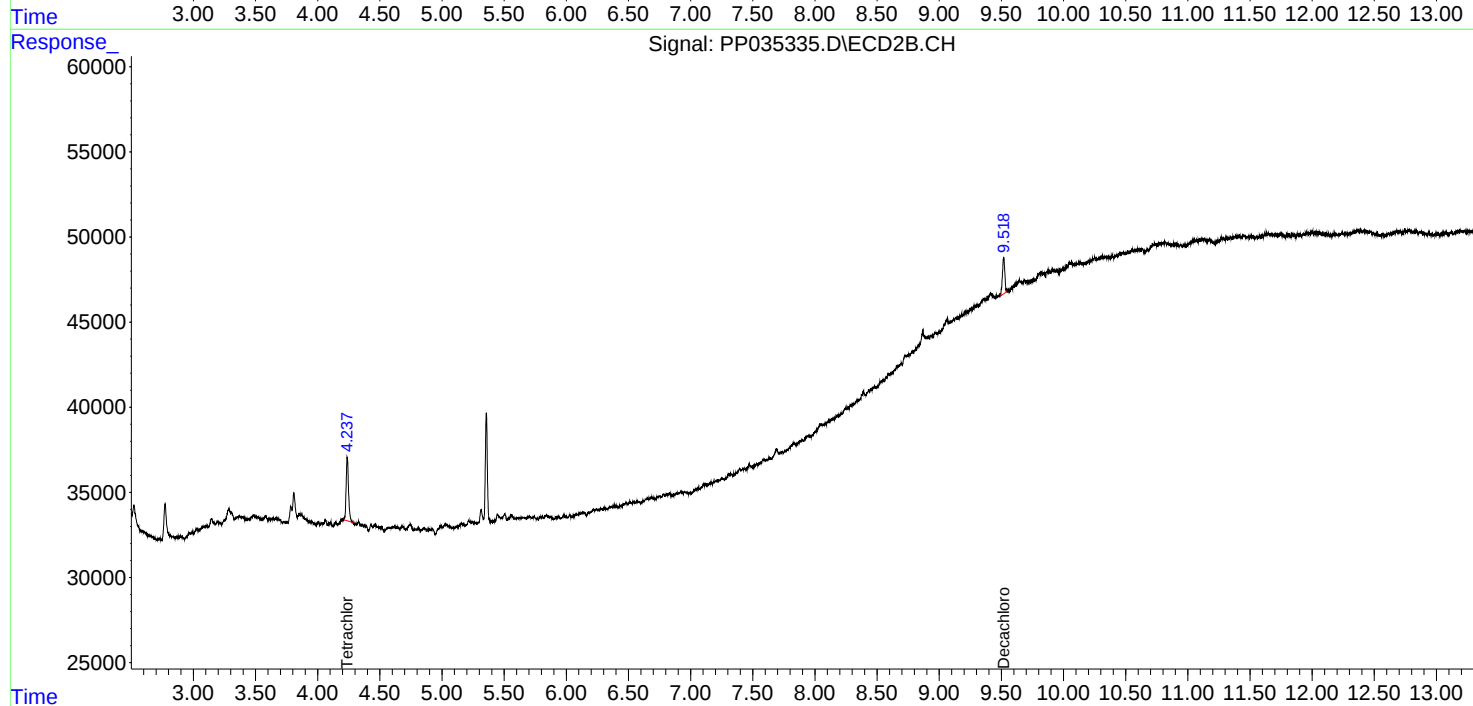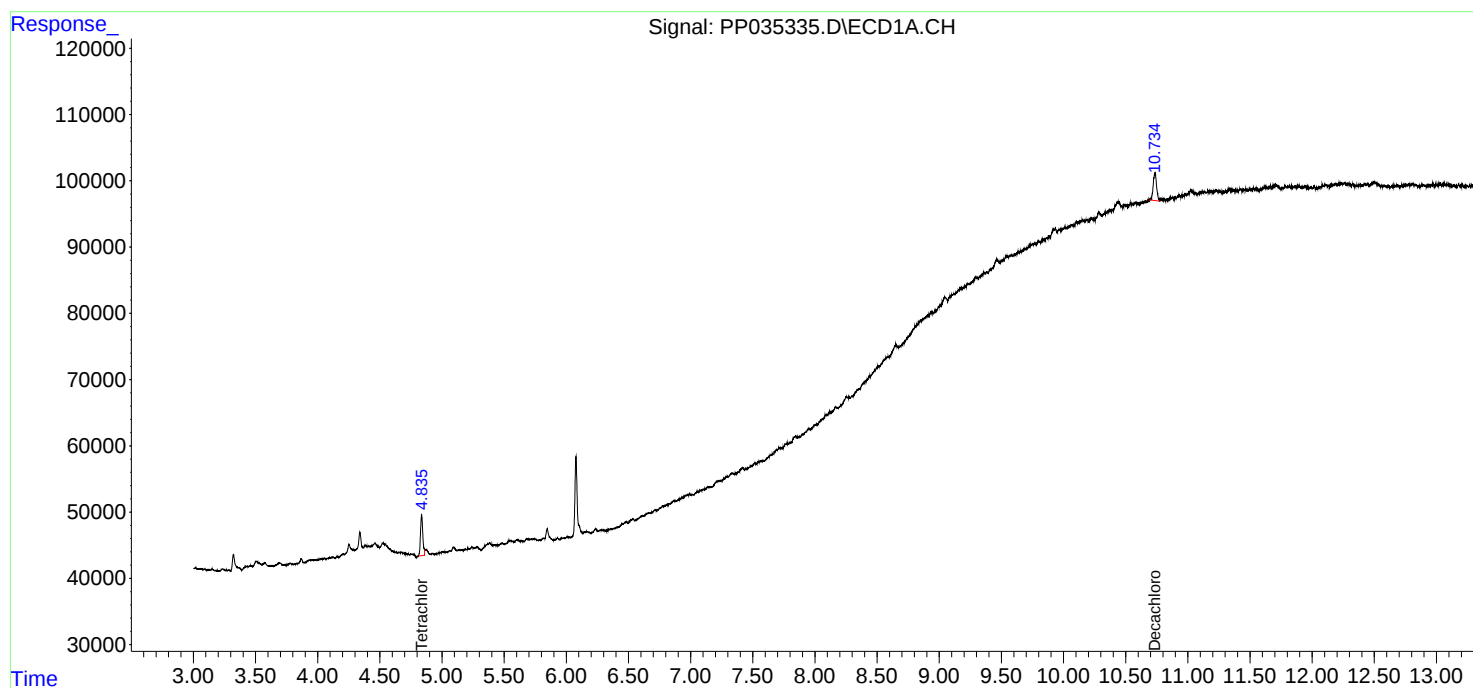

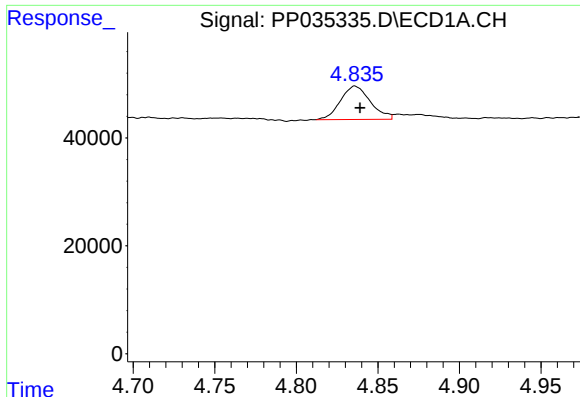


#1 Tetrachloro-m-xylene

R.T.: 4.835 min
Delta R.T.: -0.004 min
Response: 79245
Conc: 0.98 ng/ml m

Instrument :
ECD_P
ClientSampleId :
KQA103H-END-2-3


Manual Integrations
APPROVED

Ankita
4/28/2021 3:39:52 PM

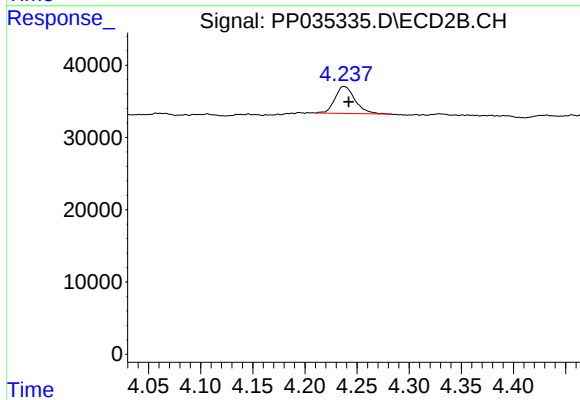


#1 Tetrachloro-m-xylene

R.T.: 4.238 min
Delta R.T.: -0.004 min
Response: 50047
Conc: 0.96 ng/ml

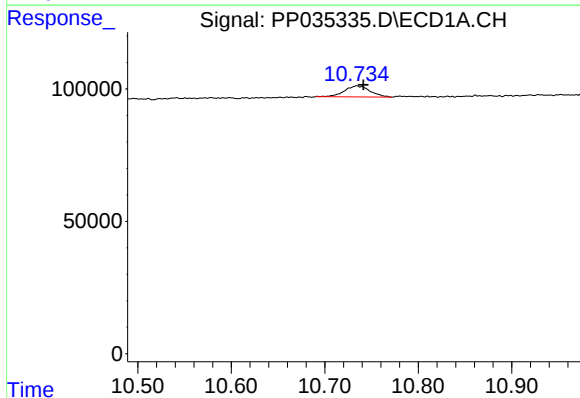

#2 Decachlorobiphenyl

R.T.: 10.734 min
Delta R.T.: -0.007 min
Response: 77952
Conc: 1.09 ng/ml

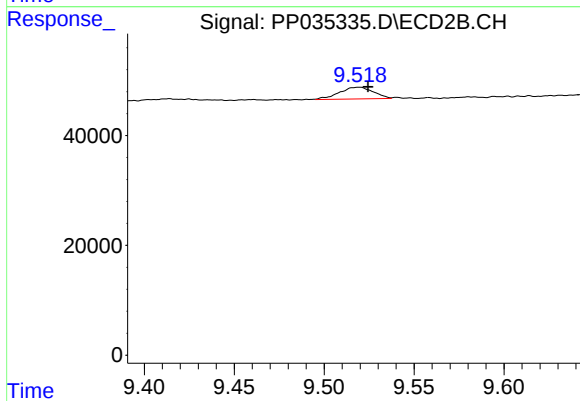

#2 Decachlorobiphenyl

R.T.: 9.518 min
Delta R.T.: -0.006 min
Response: 28363
Conc: 1.03 ng/ml m