

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042722\
 Data File : PP046733.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2022 23:45
 Operator : YP\AJ
 Sample : N2563-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 STORM-WATER-042622

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/28/2022
 Supervised By :mohammad ahmed 04/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 28 04:10:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 22 19:00:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.862	3.124	66791965	53390051	27.669	16.276m#
2) SA Decachlor...	9.938	8.443	25626162	41578088	17.415	17.431

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042722\
Data File : PP046733.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2022 23:45
Operator : YP\AJ
Sample : N2563-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
STORM-WATER-042622


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/28/2022
Supervised By :mohammad ahmed 04/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 28 04:10:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 22 19:00:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

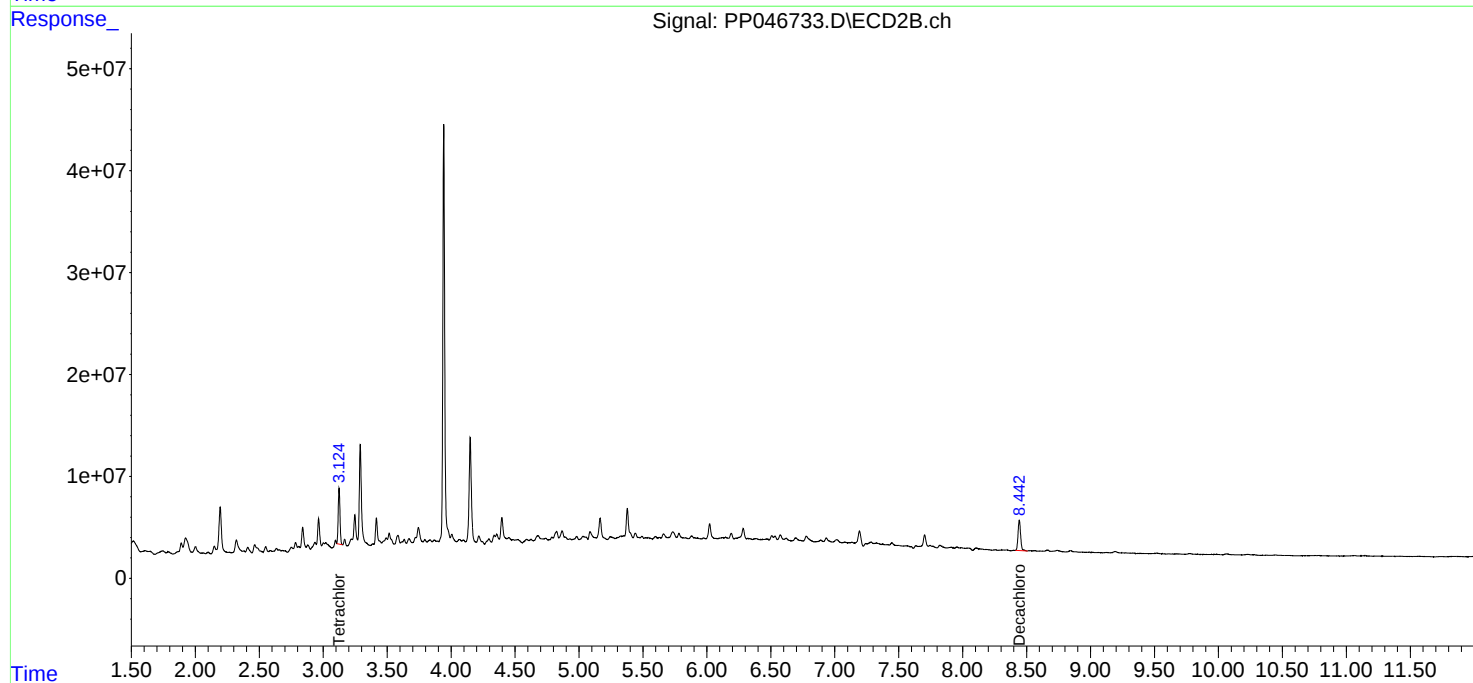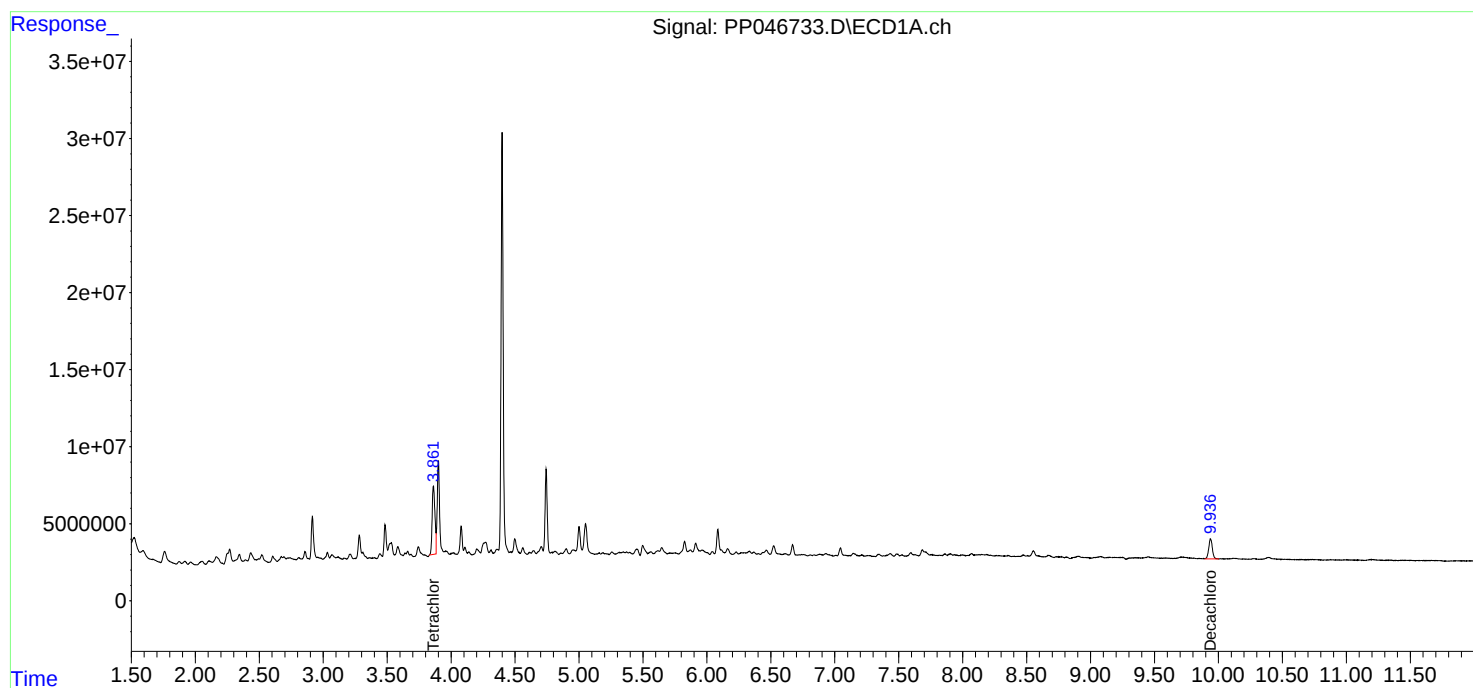

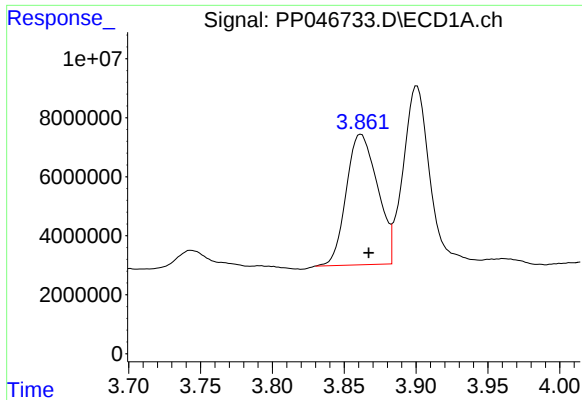


#1 Tetrachloro-m-xylene

R.T.: 3.862 min
Delta R.T.: -0.005 min
Response: 66791965
Conc: 27.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
STORM-WATER-042622


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/28/2022
Supervised By :mohammad ahmed 04/28/2022

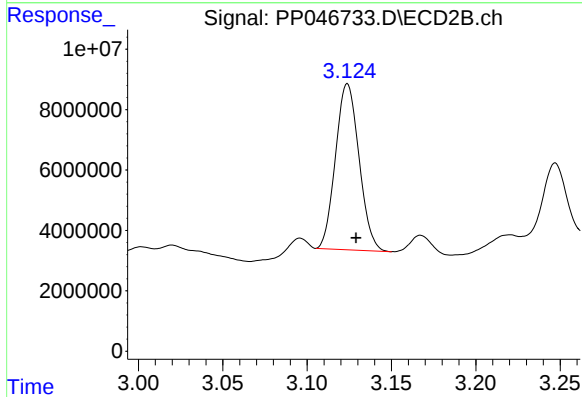


#1 Tetrachloro-m-xylene

R.T.: 3.124 min
Delta R.T.: -0.006 min
Response: 53390051
Conc: 16.28 ng/ml m

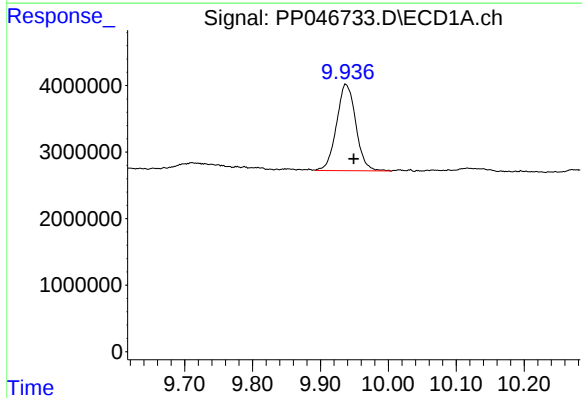

#2 Decachlorobiphenyl

R.T.: 9.938 min
Delta R.T.: -0.011 min
Response: 25626162
Conc: 17.41 ng/ml

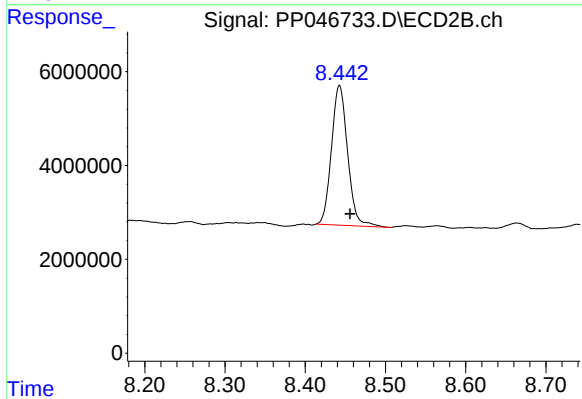

#2 Decachlorobiphenyl

R.T.: 8.443 min
Delta R.T.: -0.013 min
Response: 41578088
Conc: 17.43 ng/ml