

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042821\
 Data File : PP035370.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Apr 2021 17:25
 Operator : DD\AJ
 Sample : M2196-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WALL-D-4075-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 28 17:44:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 27 07:44:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.838	4.238	1624994	1038503	20.061	19.888
2) SA Decachlor...	10.737	9.516	1560077	580207	21.841	21.014

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042821\
Data File : PP035370.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Apr 2021 17:25
Operator : DD\AJ
Sample : M2196-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
WALL-D-4075-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 28 17:44:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042621.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 27 07:44:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

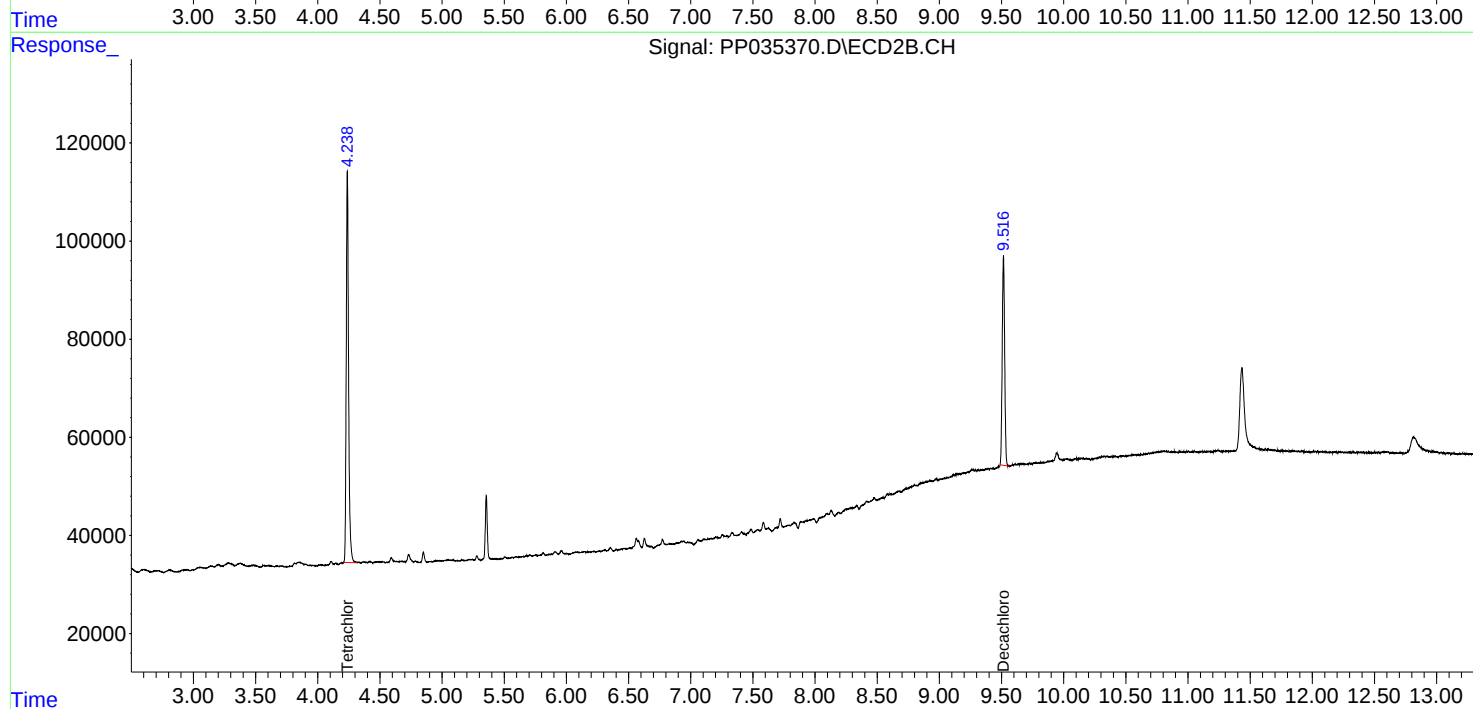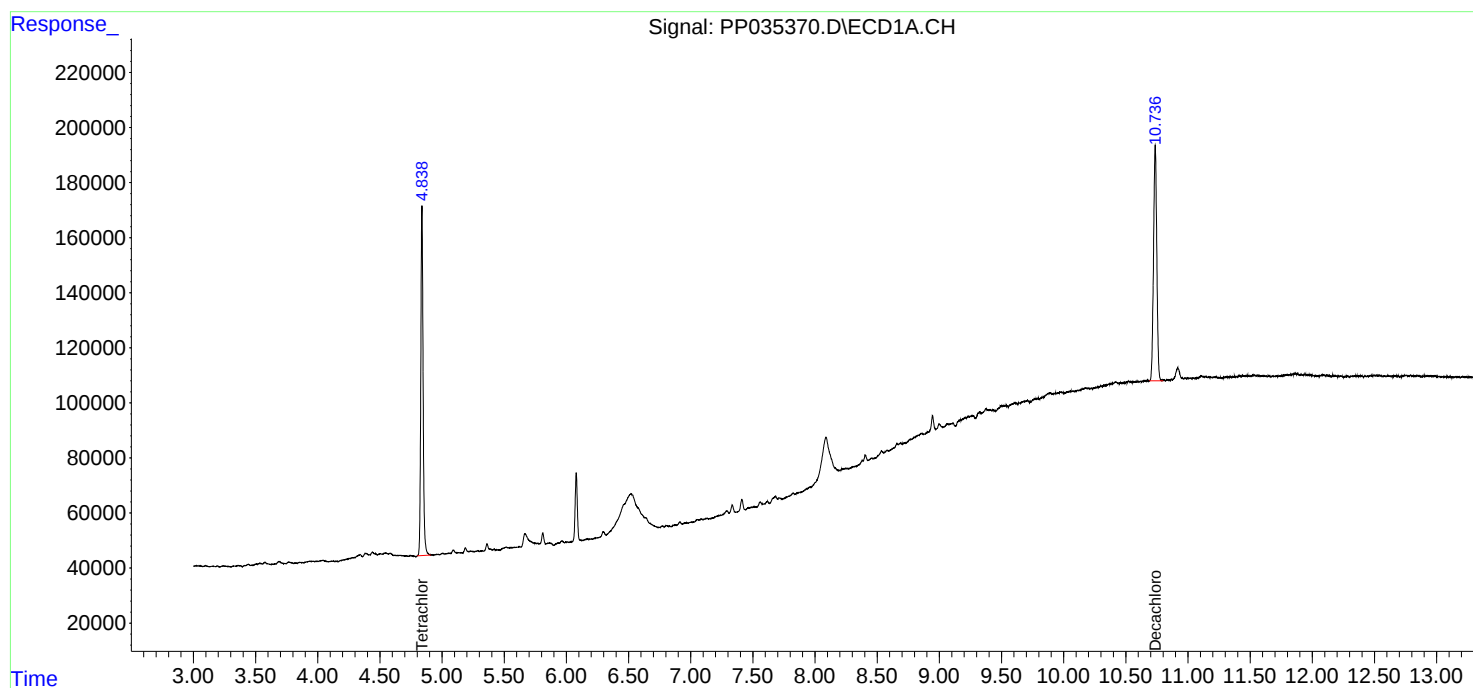


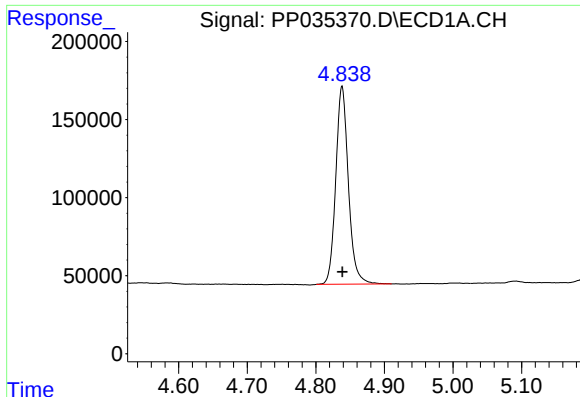

#1 Tetrachloro-m-xylene


R.T.: 4.838 min
Delta R.T.: 0.000 min
Response: 1624994
Conc: 20.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
WALL-D-4075-B

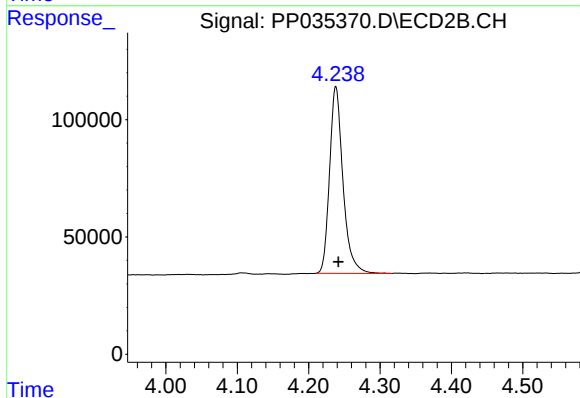


#1 Tetrachloro-m-xylene

R.T.: 4.238 min
Delta R.T.: -0.004 min
Response: 1038503
Conc: 19.89 ng/ml

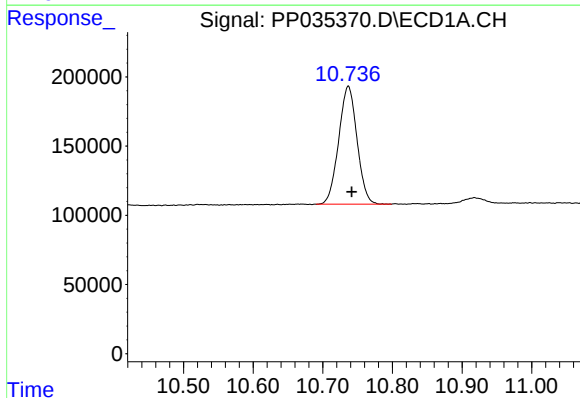

#2 Decachlorobiphenyl

R.T.: 10.737 min
Delta R.T.: -0.005 min
Response: 1560077
Conc: 21.84 ng/ml

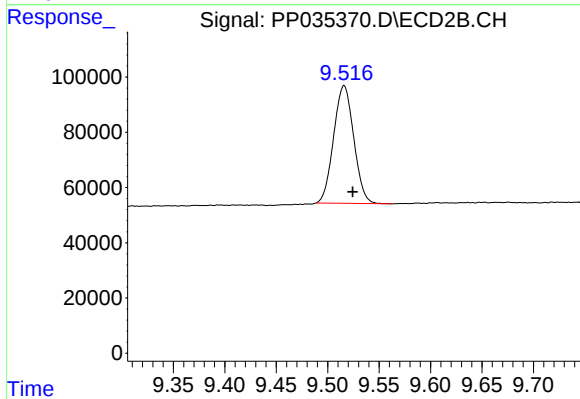

#2 Decachlorobiphenyl

R.T.: 9.516 min
Delta R.T.: -0.008 min
Response: 580207
Conc: 21.01 ng/ml