

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042821\
 Data File : PP035371.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Apr 2021 17:42
 Operator : DD\AJ
 Sample : M2198-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SAMPLE-1-GRAB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 28 18:44:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 27 07:44:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.838	4.238	1726329	1068487	21.312	20.463
2) SA Decachlor...	10.736	9.517	1678290	618972	23.496	22.419

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042821\
Data File : PP035371.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Apr 2021 17:42
Operator : DD\AJ
Sample : M2198-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SAMPLE-1-GRAB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 28 18:44:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042621.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 27 07:44:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

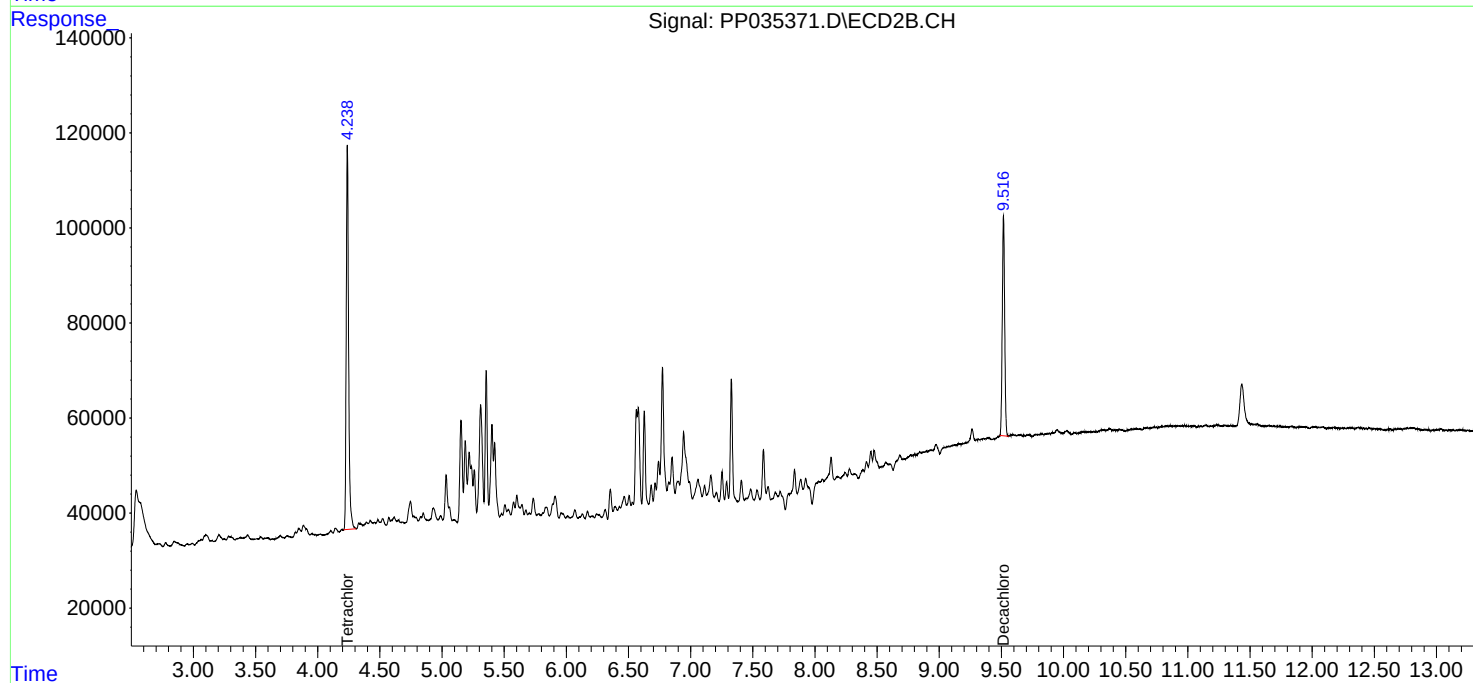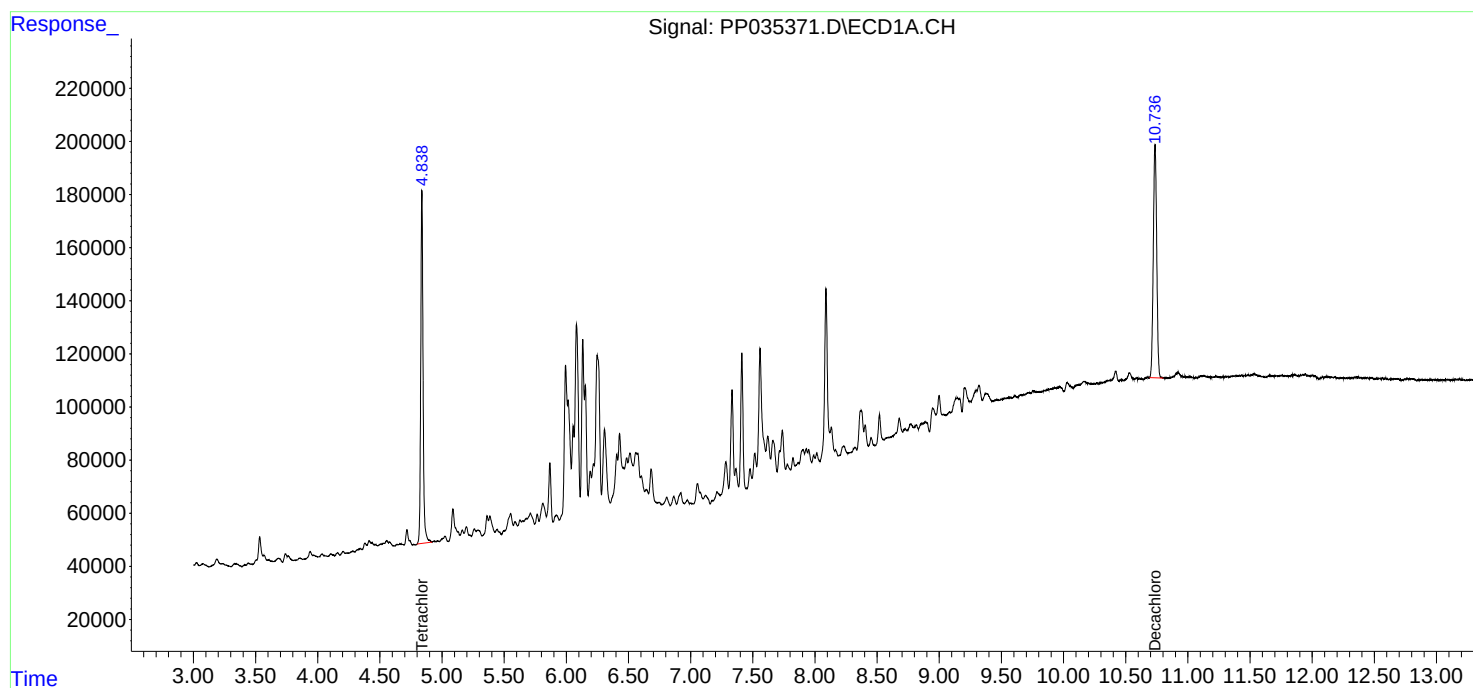


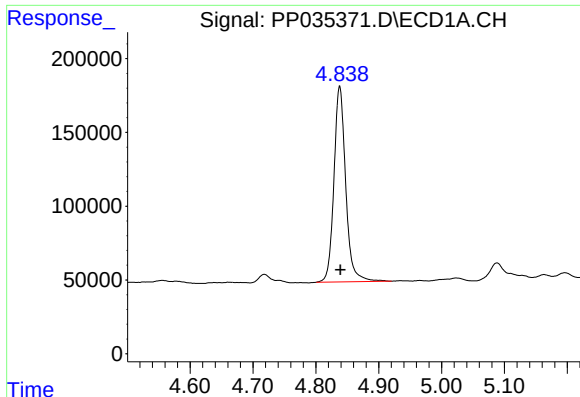

#1 Tetrachloro-m-xylene


R.T.: 4.838 min
Delta R.T.: -0.001 min
Response: 1726329
Conc: 21.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
SAMPLE-1-GRAB

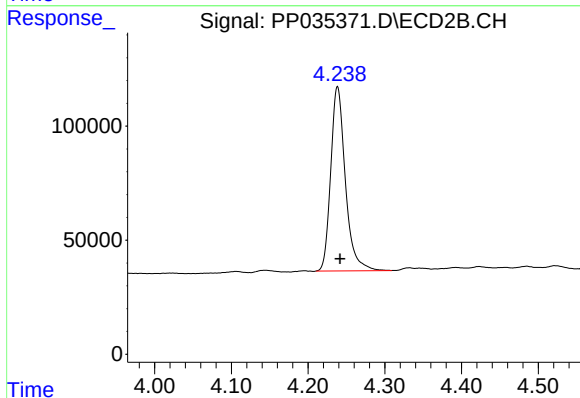


#1 Tetrachloro-m-xylene

R.T.: 4.238 min
Delta R.T.: -0.004 min
Response: 1068487
Conc: 20.46 ng/ml

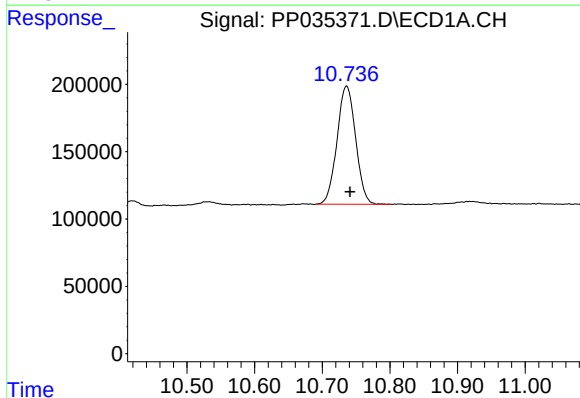

#2 Decachlorobiphenyl

R.T.: 10.736 min
Delta R.T.: -0.005 min
Response: 1678290
Conc: 23.50 ng/ml

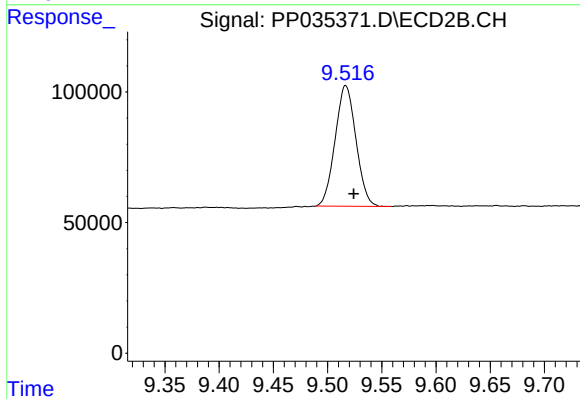

#2 Decachlorobiphenyl

R.T.: 9.517 min
Delta R.T.: -0.008 min
Response: 618972
Conc: 22.42 ng/ml