

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042821\
 Data File : PP035372.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Apr 2021 17:58
 Operator : DD\AJ
 Sample : M2199-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SAMPLE-3-COMP

Manual Integrations
 APPROVED

Ankita
 4/29/2021 3:51:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 28 18:44:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 27 07:44:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.838	4.238	1634986	1040096	20.184	19.919
2) SA Decachlor...	10.737	9.515	1428756	549490	20.003	19.902m
Target Compounds						
31) L7 AR-1260-1	7.823	7.057	30945	23370	8.575	12.004m#
32) L7 AR-1260-2	8.087	7.252	104007	23608	25.968	10.989m#
33) L7 AR-1260-3	8.452	7.409	38673	24415	13.847	11.559m
34) L7 AR-1260-4	8.681	7.885	44963	20661	13.467m	13.988m
35) L7 AR-1260-5	8.999	8.130	103349	58027	16.496	19.216

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042821\
Data File : PP035372.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Apr 2021 17:58
Operator : DD\AJ
Sample : M2199-03
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SAMPLE-3-COMP


Manual Integrations
APPROVED

Ankita
4/29/2021 3:51:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 28 18:44:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042621.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 27 07:44:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

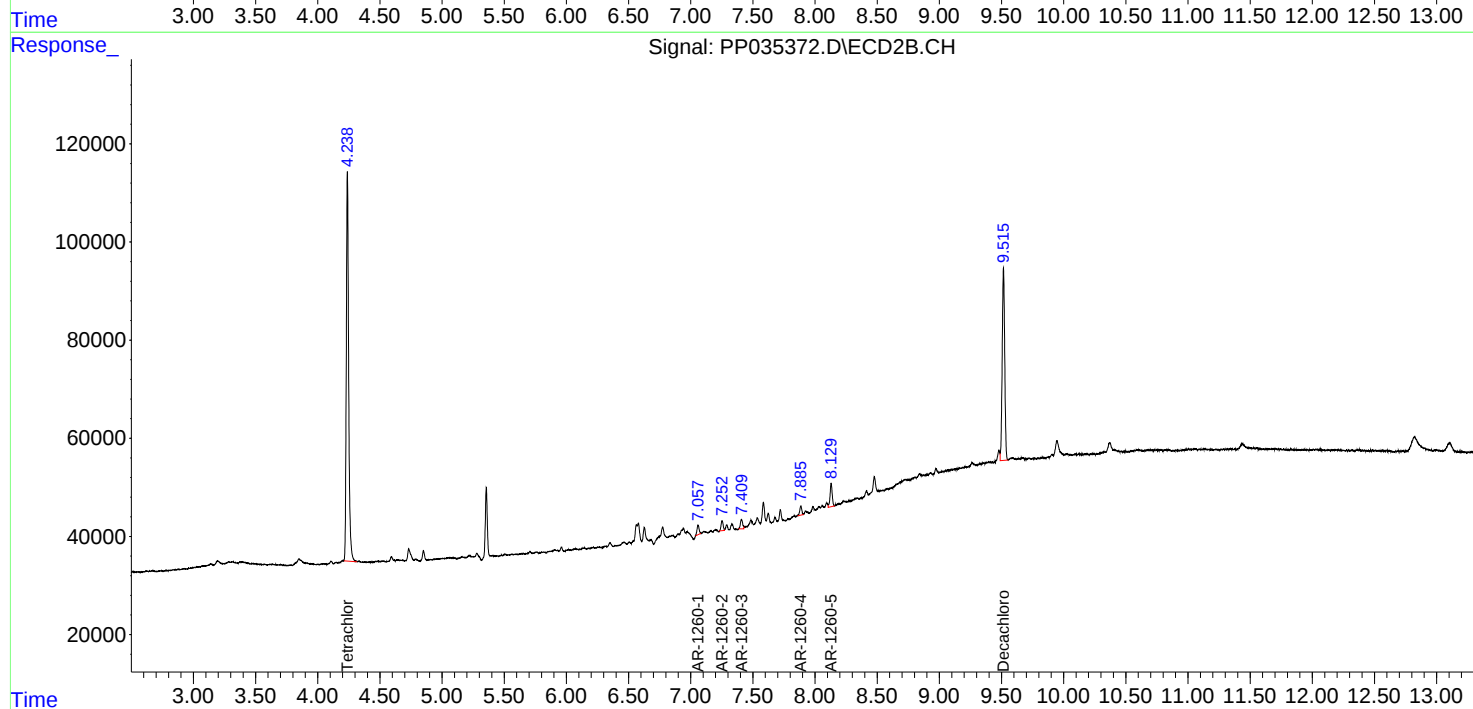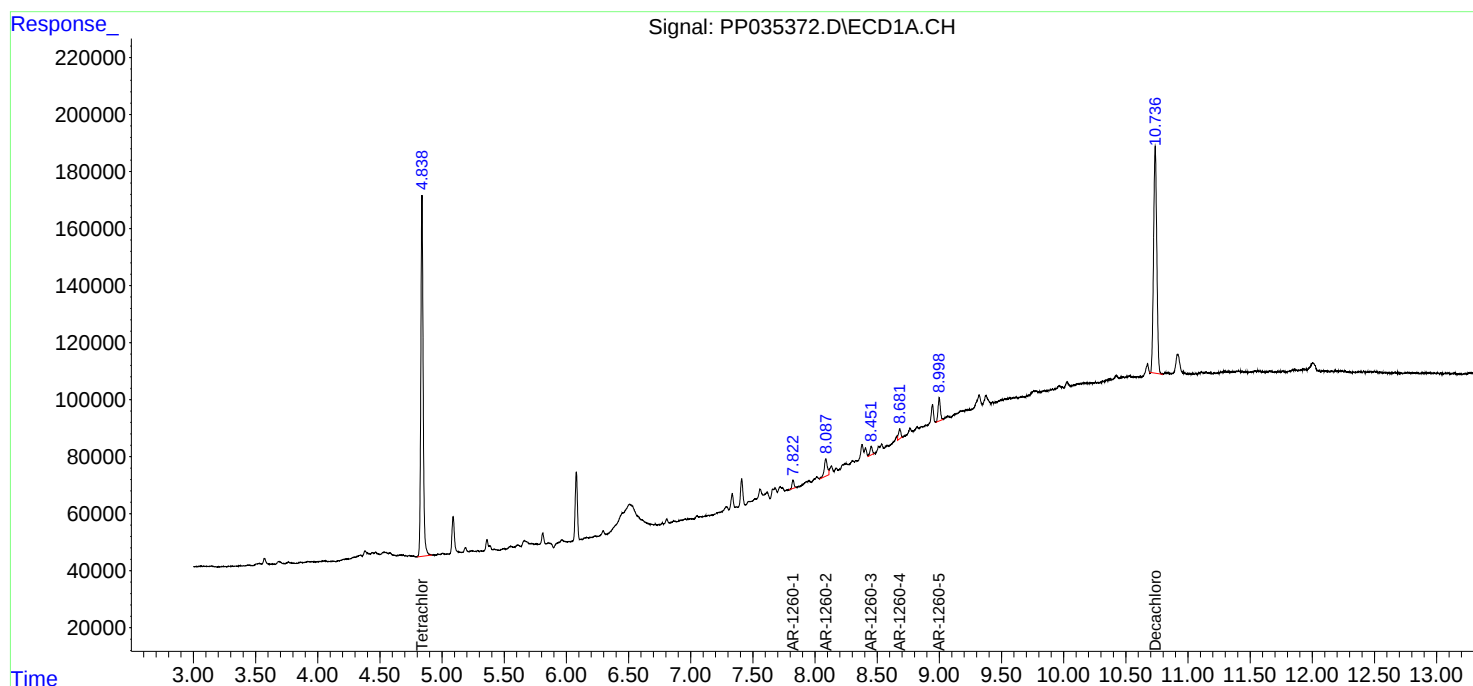

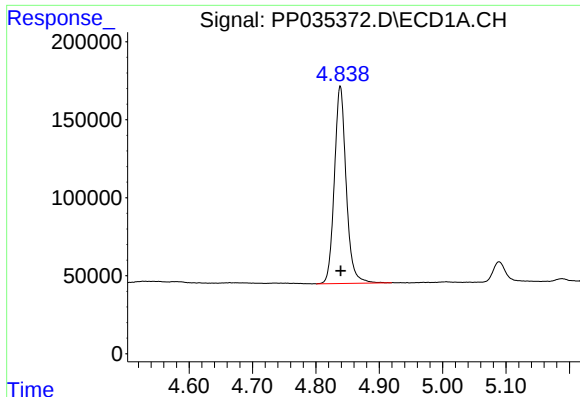


#1 Tetrachloro-m-xylene

R.T.: 4.838 min
Delta R.T.: 0.000 min
Response: 1634986
Conc: 20.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
SAMPLE-3-COMP


Manual Integrations
APPROVED

Ankita
4/29/2021 3:51:40 PM

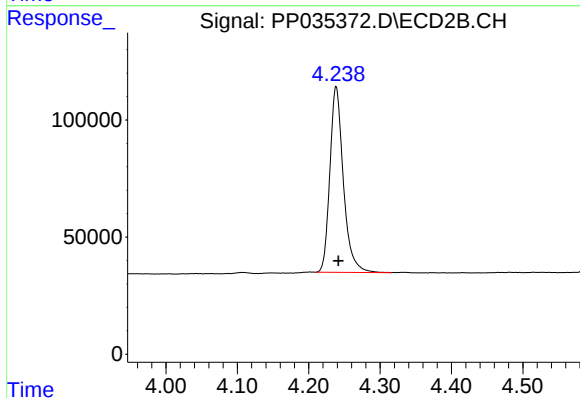


#1 Tetrachloro-m-xylene

R.T.: 4.238 min
Delta R.T.: -0.003 min
Response: 1040096
Conc: 19.92 ng/ml

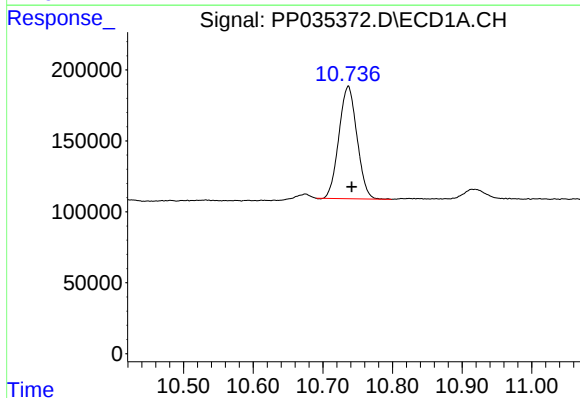


#2 Decachlorobiphenyl

R.T.: 10.737 min
Delta R.T.: -0.005 min
Response: 1428756
Conc: 20.00 ng/ml

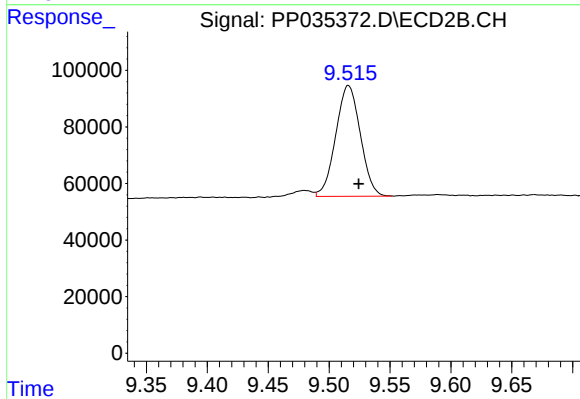

#2 Decachlorobiphenyl

R.T.: 9.515 min
Delta R.T.: -0.009 min
Response: 549490
Conc: 19.90 ng/ml m

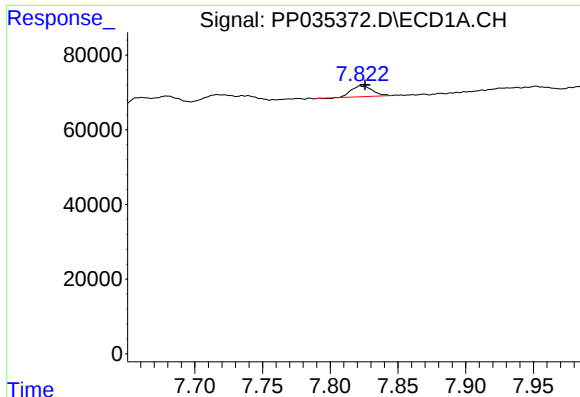


#31 AR-1260-1

R.T.: 7.823 min
Delta R.T.: -0.003 min
Response: 30945
Conc: 8.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
SAMPLE-3-COMP


Manual Integrations
APPROVED

Ankita
4/29/2021 3:51:40 PM

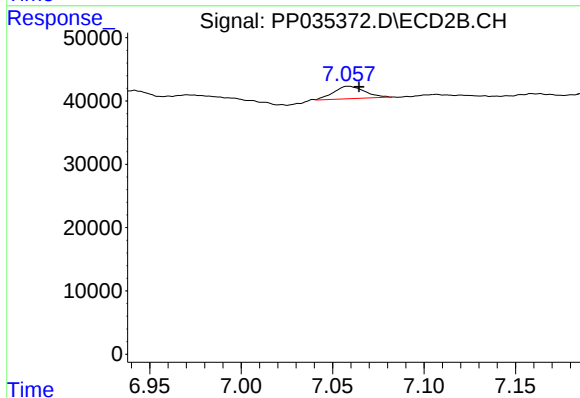


#31 AR-1260-1

R.T.: 7.057 min
Delta R.T.: -0.007 min
Response: 23370
Conc: 12.00 ng/ml m

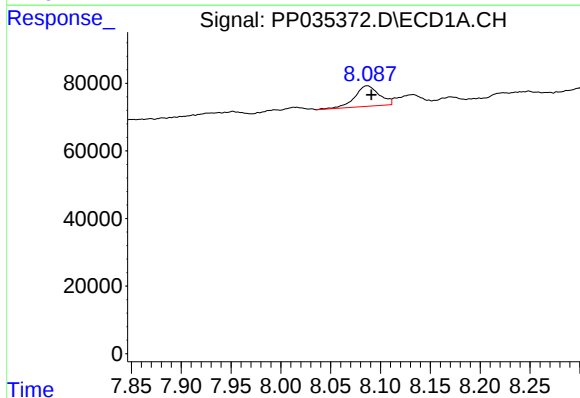


#32 AR-1260-2

R.T.: 8.087 min
Delta R.T.: -0.004 min
Response: 104007
Conc: 25.97 ng/ml

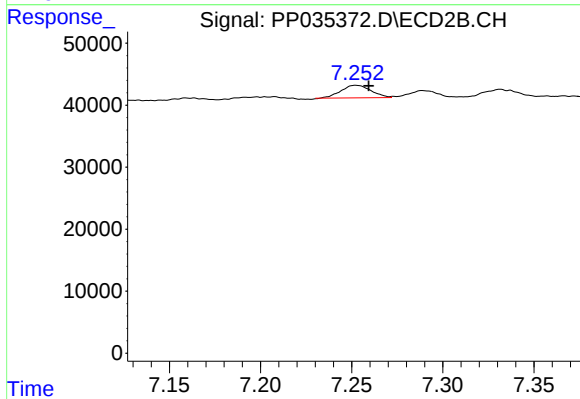

#32 AR-1260-2

R.T.: 7.252 min
Delta R.T.: -0.008 min
Response: 23608
Conc: 10.99 ng/ml m

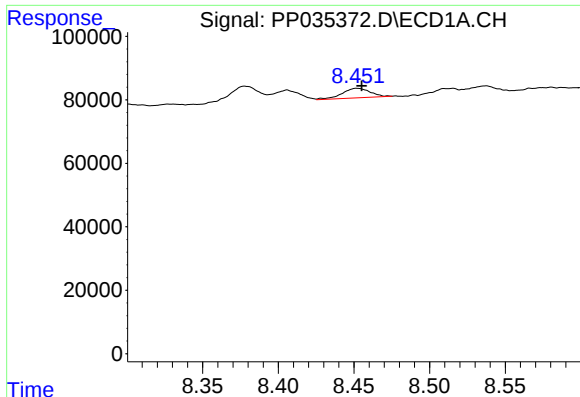


#33 AR-1260-3

R.T.: 8.452 min
Delta R.T.: -0.003 min
Response: 38673
Conc: 13.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
SAMPLE-3-COMP


Manual Integrations
APPROVED

Ankita
4/29/2021 3:51:40 PM

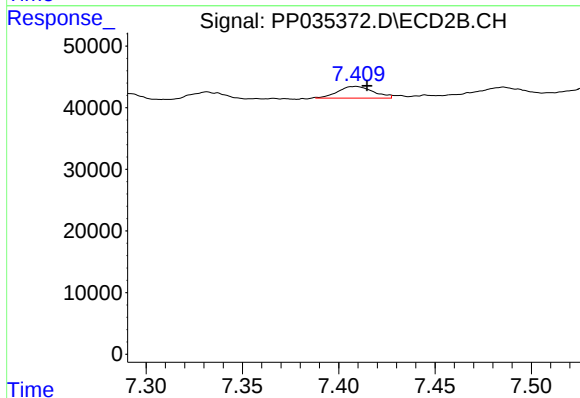


#33 AR-1260-3

R.T.: 7.409 min
Delta R.T.: -0.006 min
Response: 24415
Conc: 11.56 ng/ml m

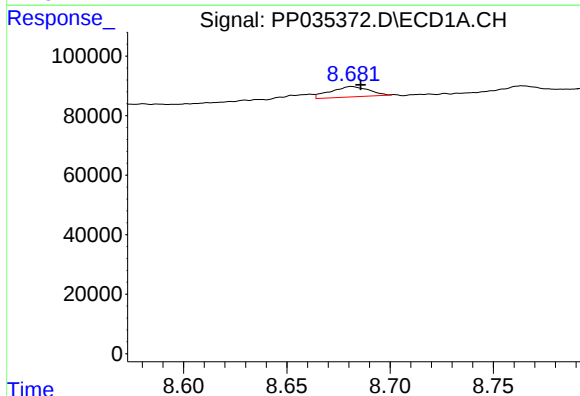


#34 AR-1260-4

R.T.: 8.681 min
Delta R.T.: -0.005 min
Response: 44963
Conc: 13.47 ng/ml m

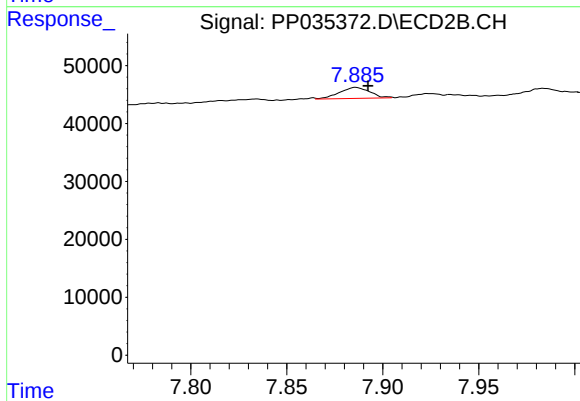

#34 AR-1260-4

R.T.: 7.885 min
Delta R.T.: -0.007 min
Response: 20661
Conc: 13.99 ng/ml m

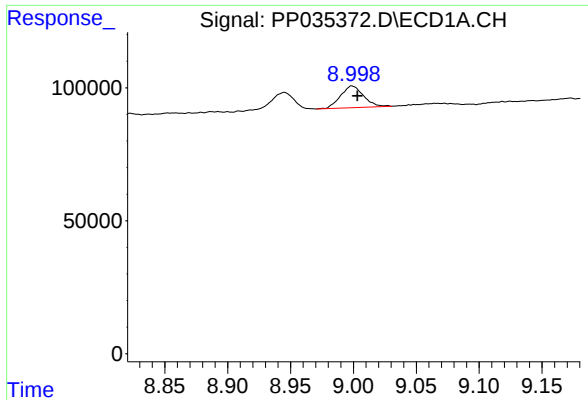


#35 AR-1260-5

R.T.: 8.999 min
Delta R.T.: -0.004 min
Response: 103349
Conc: 16.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
SAMPLE-3-COMP

Manual Integrations
APPROVED

Ankita
4/29/2021 3:51:40 PM

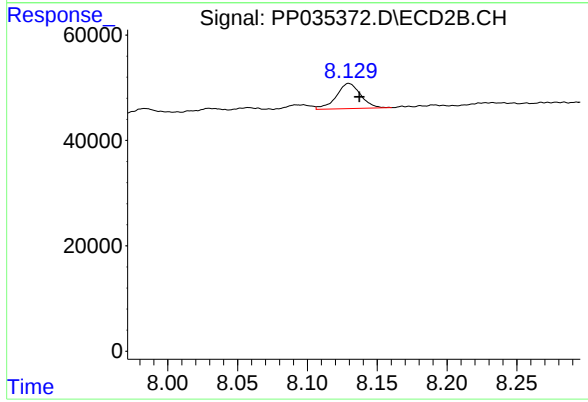

#35 AR-1260-5

R.T.: 8.130 min
Delta R.T.: -0.008 min
Response: 58027
Conc: 19.22 ng/ml