

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042821\
 Data File : PP035376.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Apr 2021 19:06
 Operator : DD\AJ
 Sample : M2154-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 33096

Manual Integrations
 APPROVED

Ankita
 4/29/2021 1:10:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 05:53:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 27 07:44:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.840	4.240	1265176	666449	15.619	12.763
2) SA Decachlor...	10.738	9.518	344114	123899	4.818	4.487
Target Compounds						
26) L6 AR-1254-1	7.052	6.352	775445	301224	285.648m	162.273m#
27) L6 AR-1254-2	7.281	6.508	596699	258299	144.279m	155.677m
28) L6 AR-1254-3	7.658	6.927	520688	280644	123.688m	120.927m
29) L6 AR-1254-4	7.953	7.162	707911	173169	260.688m	164.494m#
30) L6 AR-1254-5	8.380	7.587	591757	275191	175.173	133.094m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042821\
Data File : PP035376.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Apr 2021 19:06
Operator : DD\AJ
Sample : M2154-02
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
33096


Manual Integrations
APPROVED

Ankita
4/29/2021 1:10:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 05:53:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042621.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 27 07:44:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

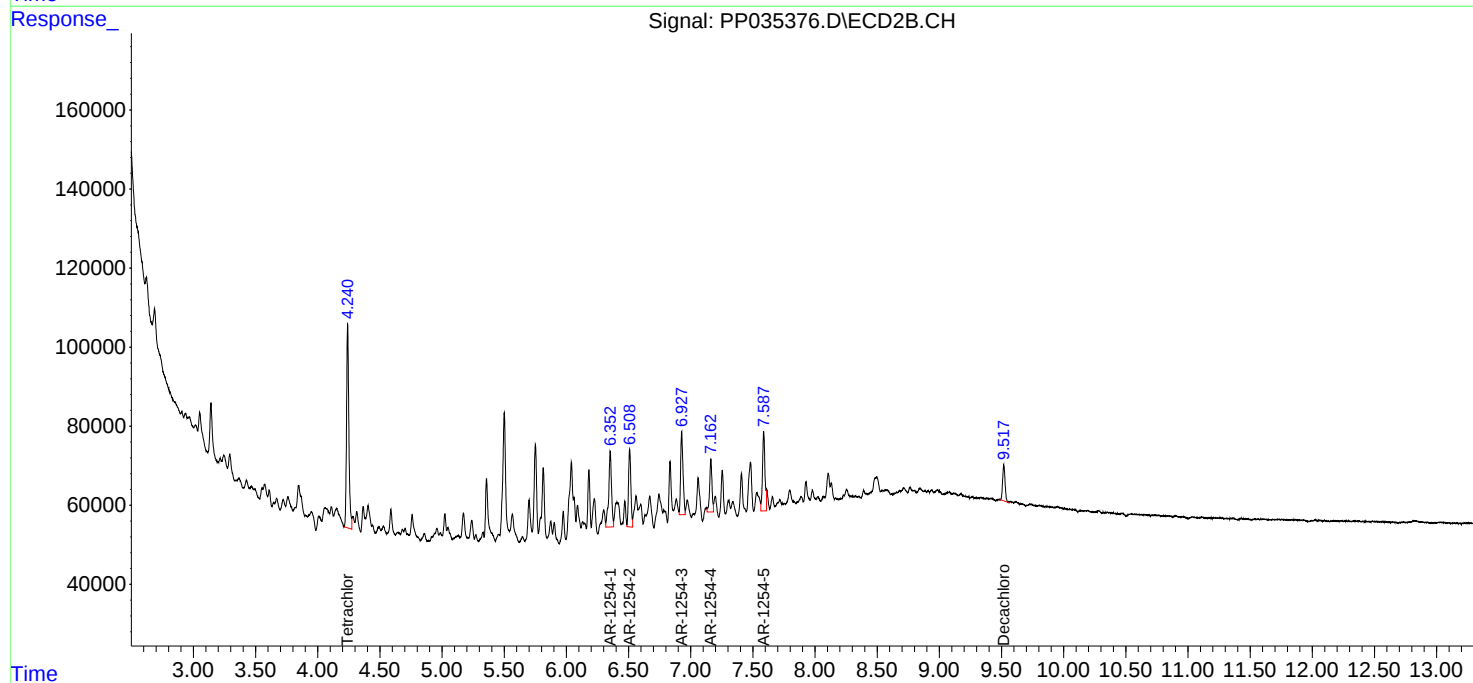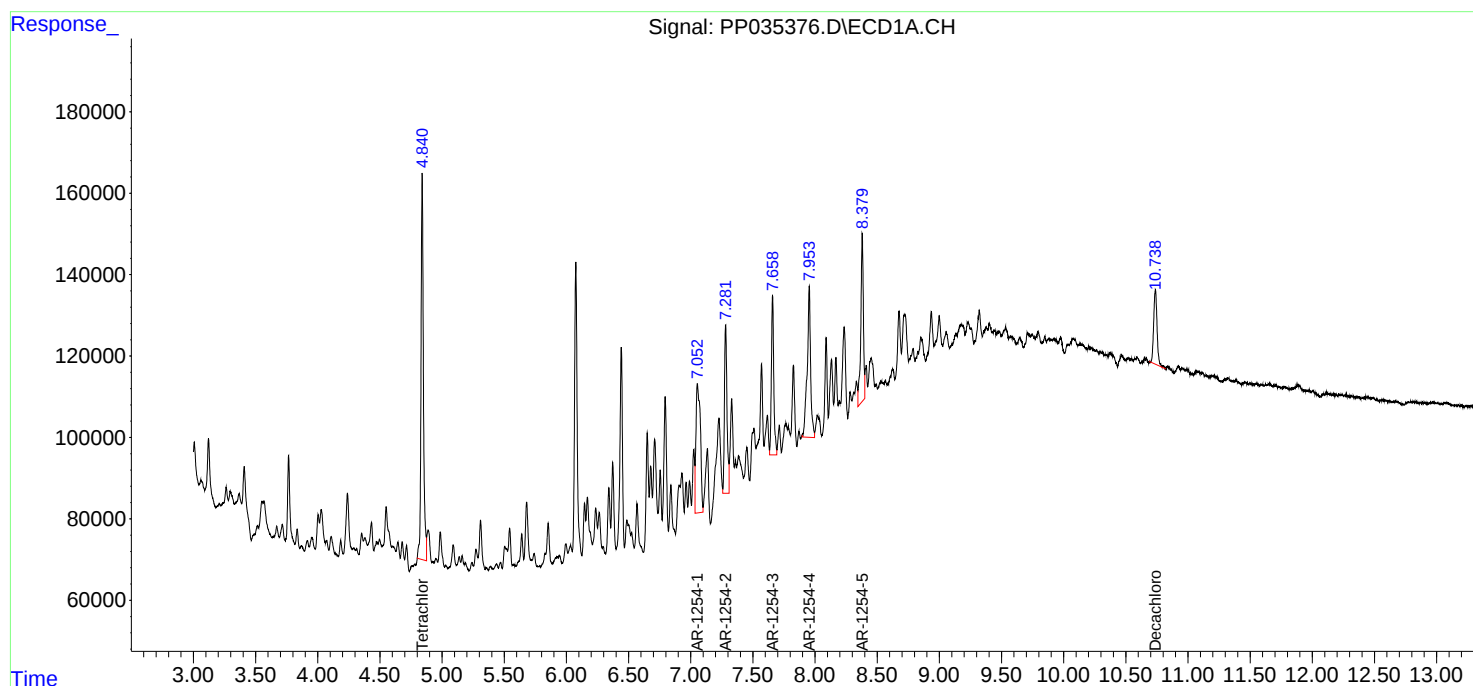

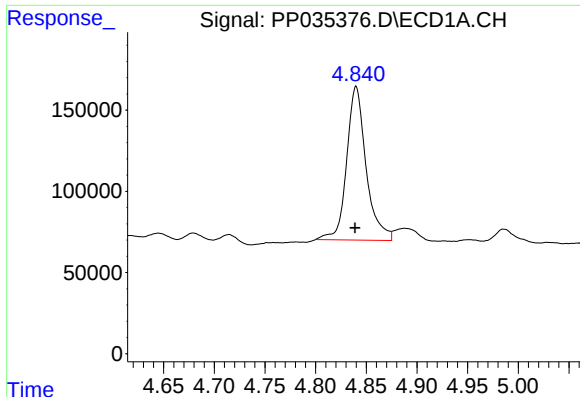


#1 Tetrachloro-m-xylene

R.T.: 4.840 min
Delta R.T.: 0.000 min
Response: 1265176
Conc: 15.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
33096


Manual Integrations
APPROVED

Ankita
4/29/2021 1:10:15 PM

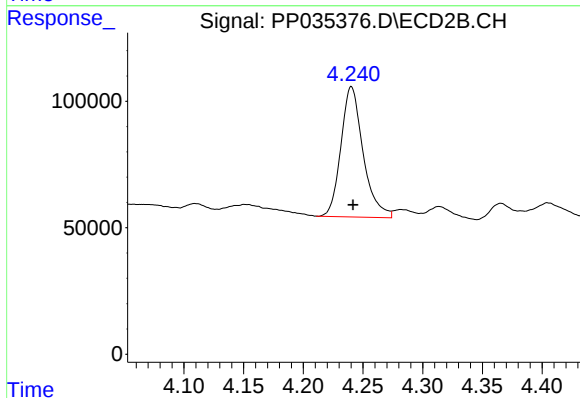


#1 Tetrachloro-m-xylene

R.T.: 4.240 min
Delta R.T.: -0.002 min
Response: 666449
Conc: 12.76 ng/ml

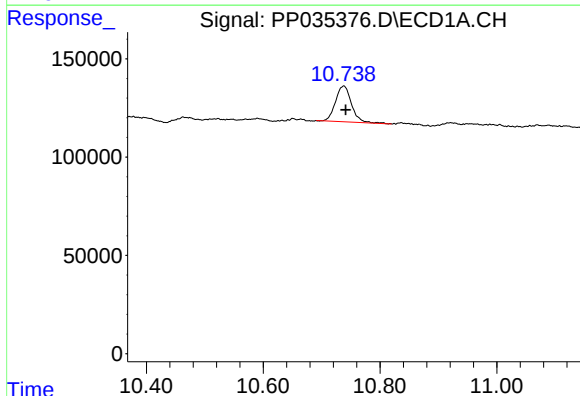


#2 Decachlorobiphenyl

R.T.: 10.738 min
Delta R.T.: -0.003 min
Response: 344114
Conc: 4.82 ng/ml

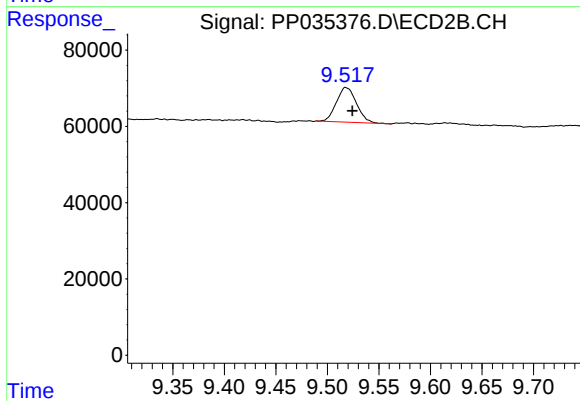

#2 Decachlorobiphenyl

R.T.: 9.518 min
Delta R.T.: -0.006 min
Response: 123899
Conc: 4.49 ng/ml

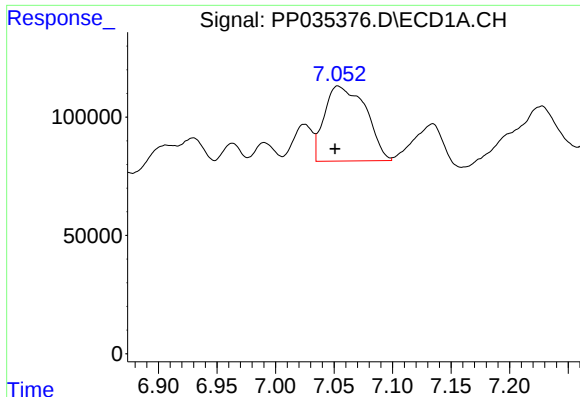


#26 AR-1254-1

R.T.: 7.052 min
Delta R.T.: 0.001 min
Response: 775445
Conc: 285.65 ng/ml m

Instrument :
ECD_P
ClientSampleId :
33096


Manual Integrations
APPROVED

Ankita
4/29/2021 1:10:15 PM

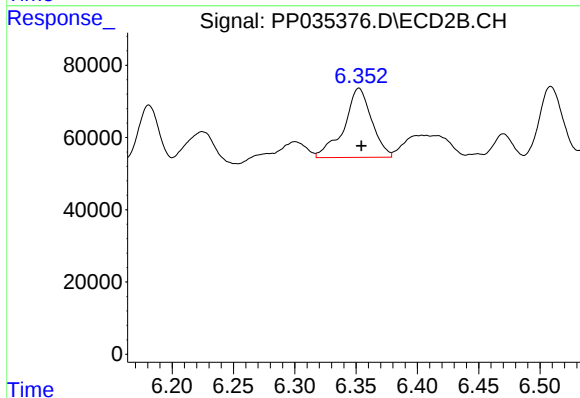


#26 AR-1254-1

R.T.: 6.352 min
Delta R.T.: -0.002 min
Response: 301224
Conc: 162.27 ng/ml m

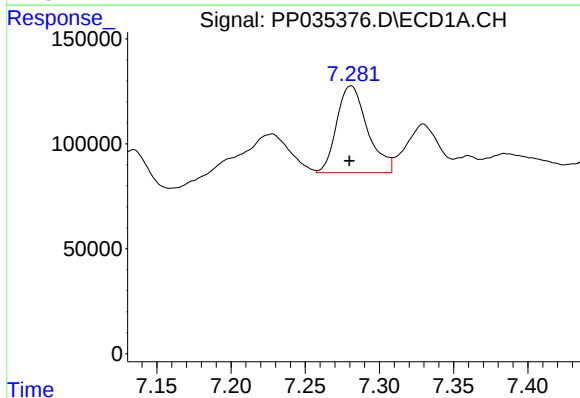


#27 AR-1254-2

R.T.: 7.281 min
Delta R.T.: 0.000 min
Response: 596699
Conc: 144.28 ng/ml m

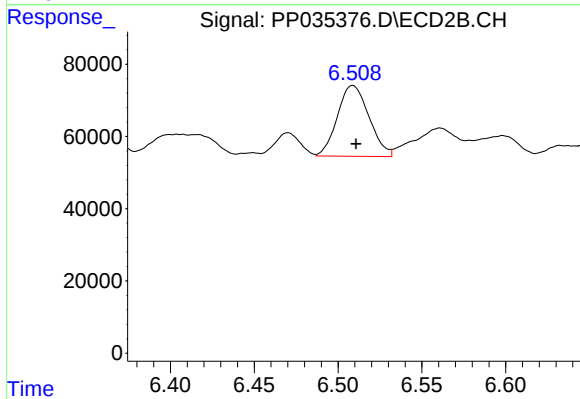

#27 AR-1254-2

R.T.: 6.508 min
Delta R.T.: -0.002 min
Response: 258299
Conc: 155.68 ng/ml m

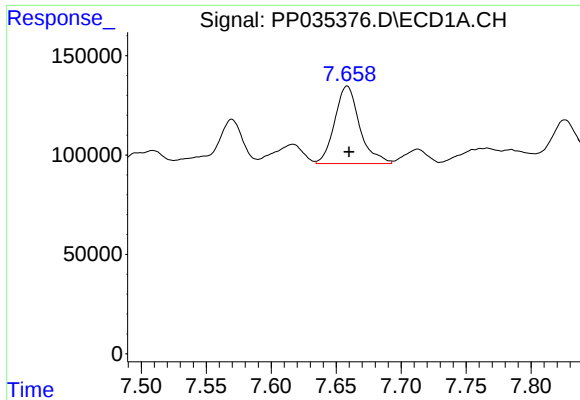


#28 AR-1254-3

R.T.: 7.658 min
Delta R.T.: -0.002 min
Response: 520688
Conc: 123.69 ng/ml m

Instrument :
ECD_P
ClientSampleId :
33096


Manual Integrations
APPROVED

Ankita
4/29/2021 1:10:15 PM

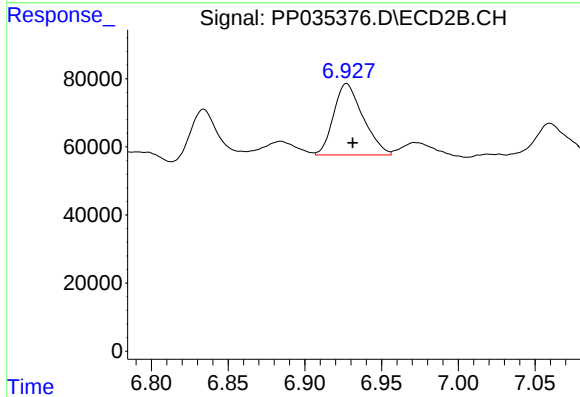


#28 AR-1254-3

R.T.: 6.927 min
Delta R.T.: -0.004 min
Response: 280644
Conc: 120.93 ng/ml m

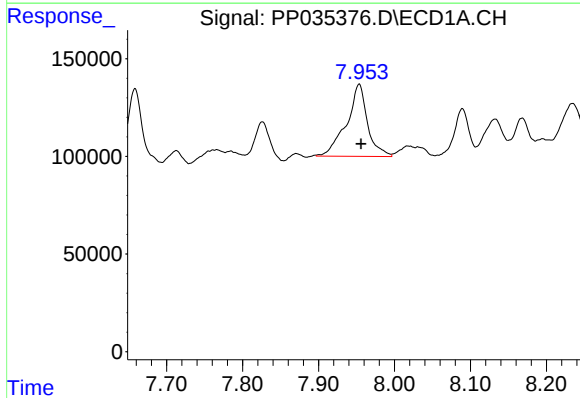


#29 AR-1254-4

R.T.: 7.953 min
Delta R.T.: -0.003 min
Response: 707911
Conc: 260.69 ng/ml m

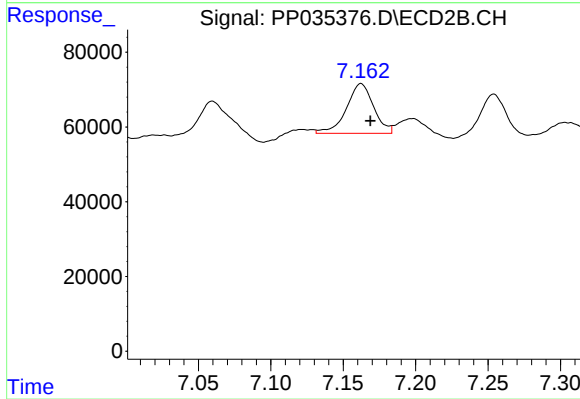

#29 AR-1254-4

R.T.: 7.162 min
Delta R.T.: -0.007 min
Response: 173169
Conc: 164.49 ng/ml m

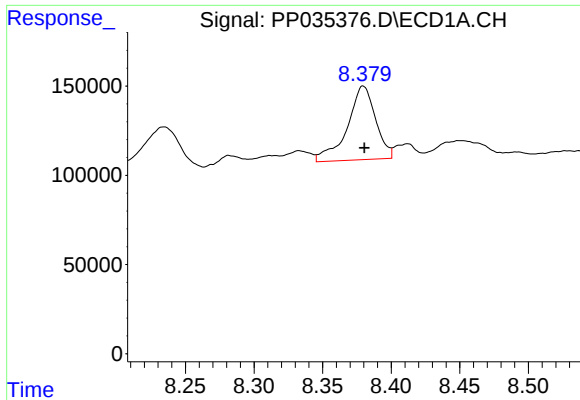


#30 AR-1254-5

R.T.: 8.380 min
Delta R.T.: 0.000 min
Response: 591757
Conc: 175.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
33096

Manual Integrations
APPROVED

Ankita
4/29/2021 1:10:15 PM

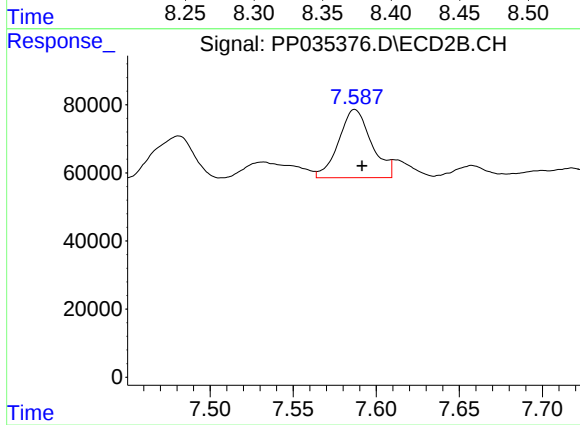

#30 AR-1254-5

R.T.: 7.587 min
Delta R.T.: -0.005 min
Response: 275191
Conc: 133.09 ng/ml m