

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042821\
 Data File : PP035377.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Apr 2021 19:22
 Operator : DD\AJ
 Sample : M2156-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 33066

Manual Integrations
 APPROVED

Ankita
 4/29/2021 1:10:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 05:53:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 27 07:44:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.839	4.240	754604	953136	9.316	18.254m#
2) SA Decachlor...	10.738	9.516	744520	282104	10.423	10.218

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042821\
Data File : PP035377.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Apr 2021 19:22
Operator : DD\AJ
Sample : M2156-01
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
33066


Manual Integrations
APPROVED

Ankita
4/29/2021 1:10:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 05:53:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042621.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 27 07:44:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

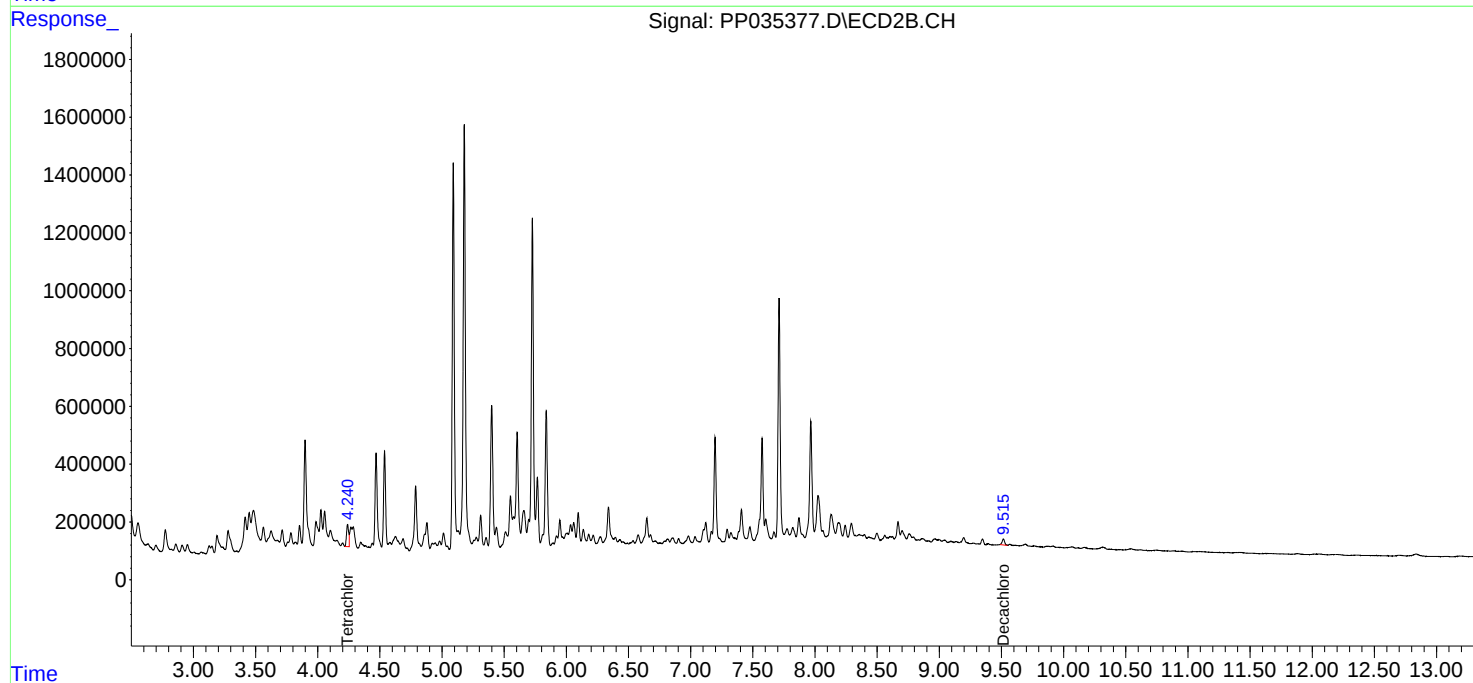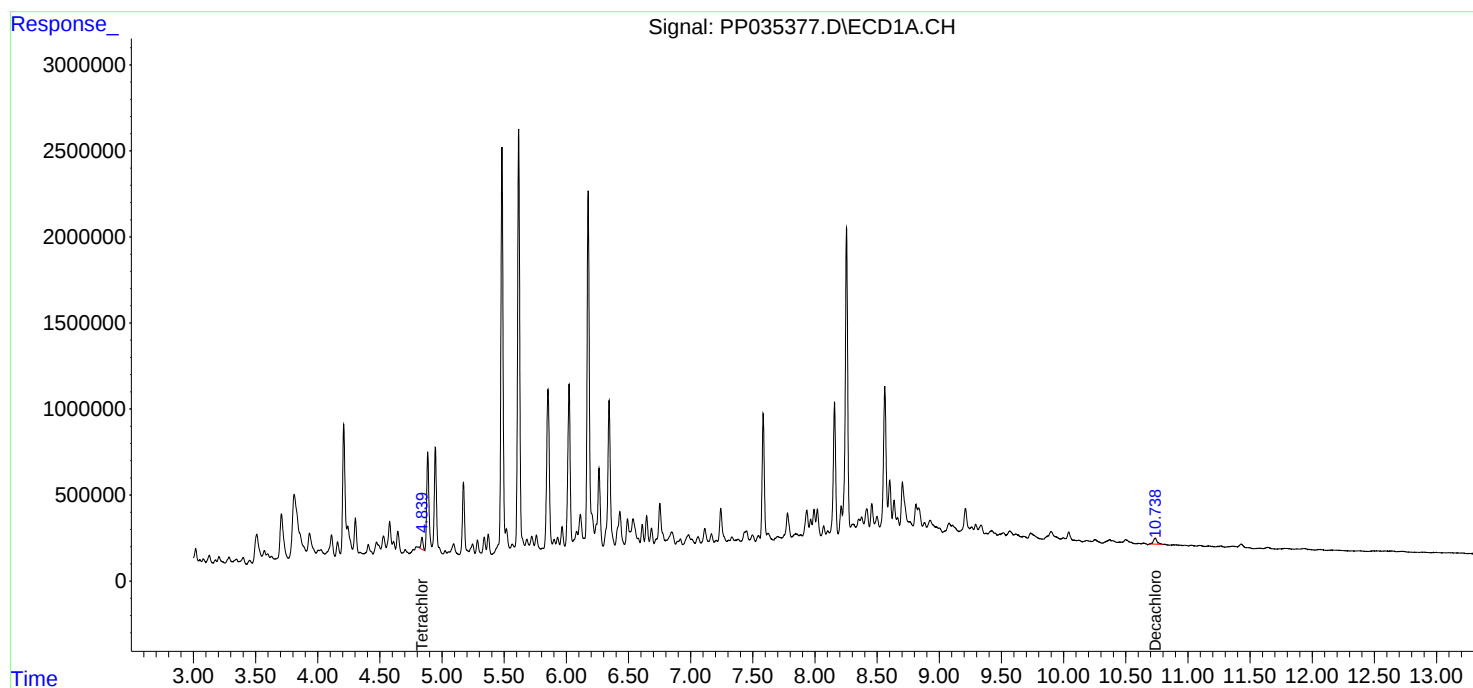

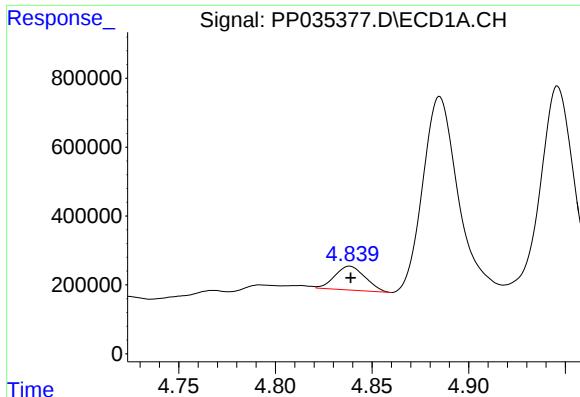


#1 Tetrachloro-m-xylene

R.T.: 4.839 min
Delta R.T.: 0.000 min
Response: 754604
Conc: 9.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
33066


Manual Integrations
APPROVED

Ankita
4/29/2021 1:10:17 PM

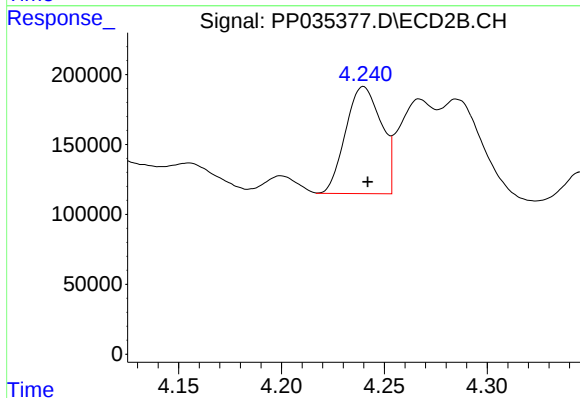


#1 Tetrachloro-m-xylene

R.T.: 4.240 min
Delta R.T.: -0.002 min
Response: 953136
Conc: 18.25 ng/ml m

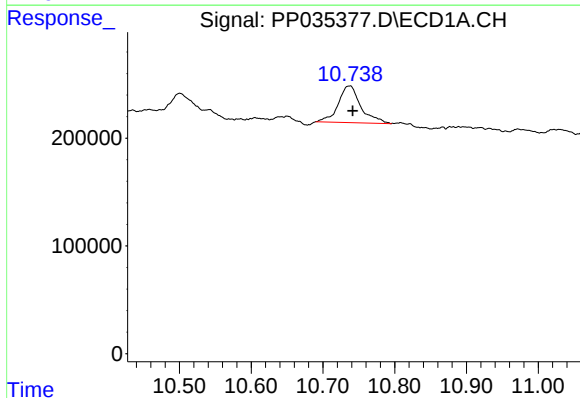

#2 Decachlorobiphenyl

R.T.: 10.738 min
Delta R.T.: -0.004 min
Response: 744520
Conc: 10.42 ng/ml

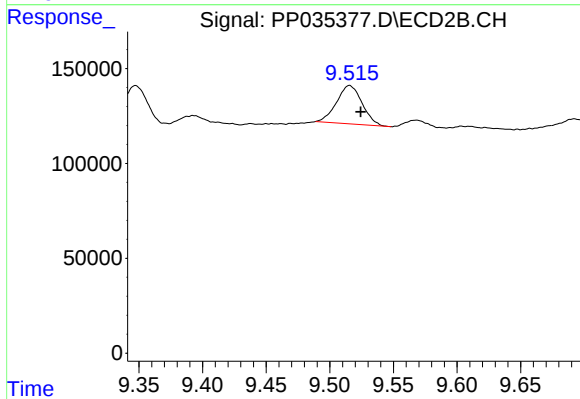

#2 Decachlorobiphenyl

R.T.: 9.516 min
Delta R.T.: -0.009 min
Response: 282104
Conc: 10.22 ng/ml