

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042822\
 Data File : PP046790.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Apr 2022 21:49
 Operator : YP\AJ
 Sample : N2597-02 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KMH332L-END-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/29/2022
 Supervised By :mohammad ahmed 04/29/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 04:56:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 22 19:00:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.857	3.124	4098982	6527381	1.698m	1.990
2) SA Decachlor...	9.938	8.442	3877911	5585680	2.635	2.342

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042822\
Data File : PP046790.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Apr 2022 21:49
Operator : YP\AJ
Sample : N2597-02 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KMH332L-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/29/2022
Supervised By :mohammad ahmed 04/29/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 04:56:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 22 19:00:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

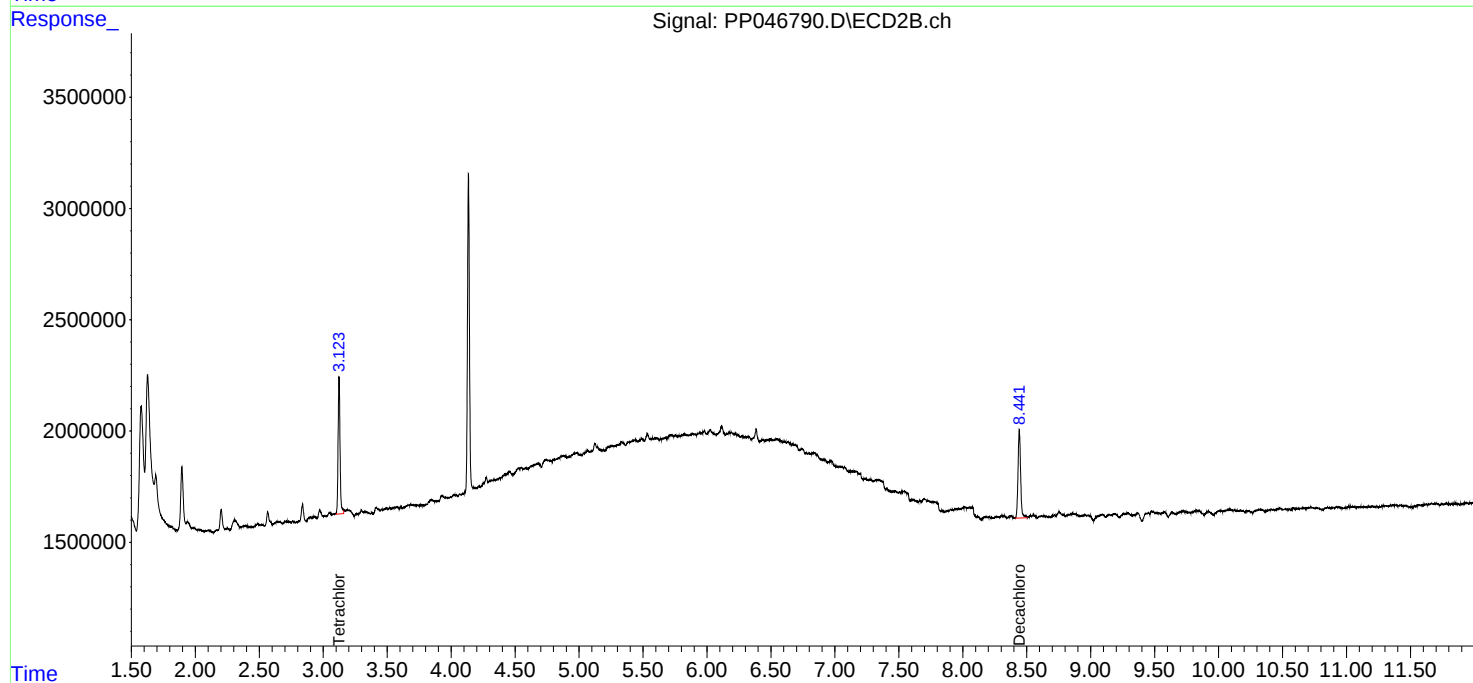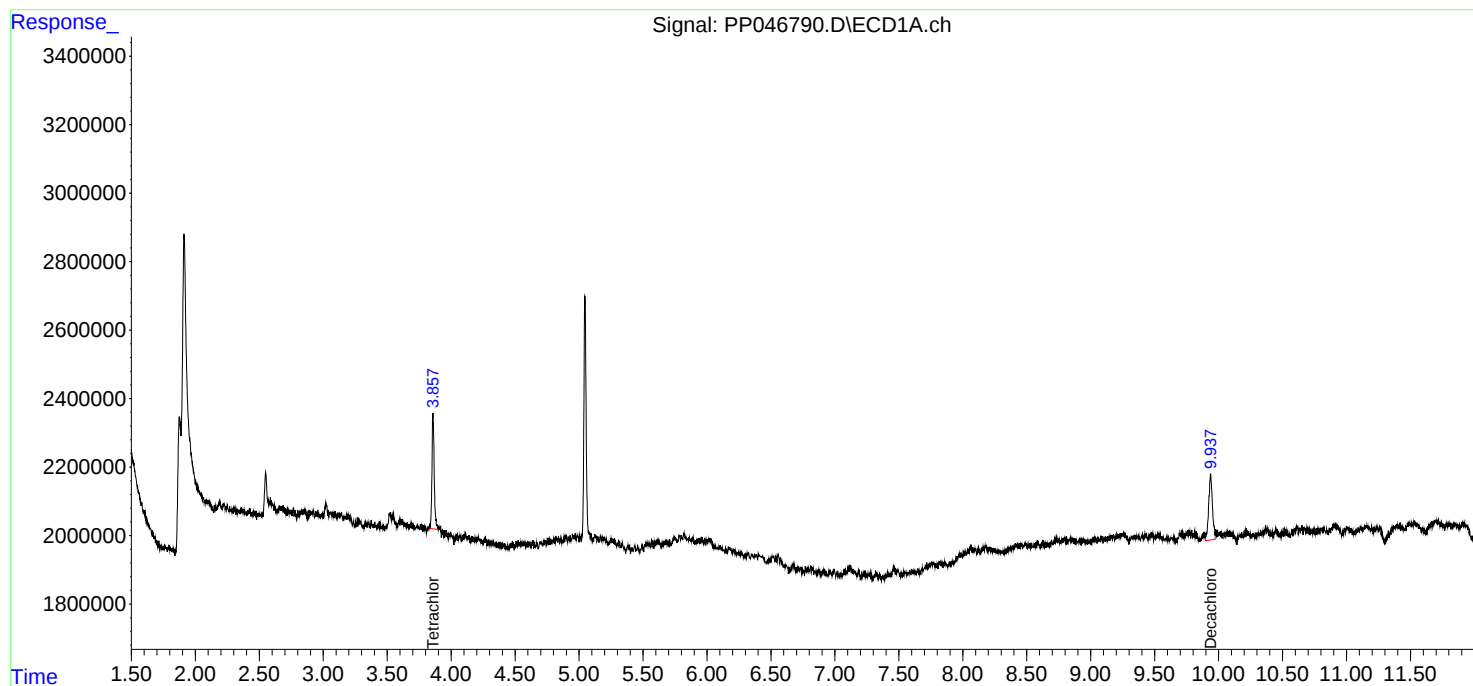

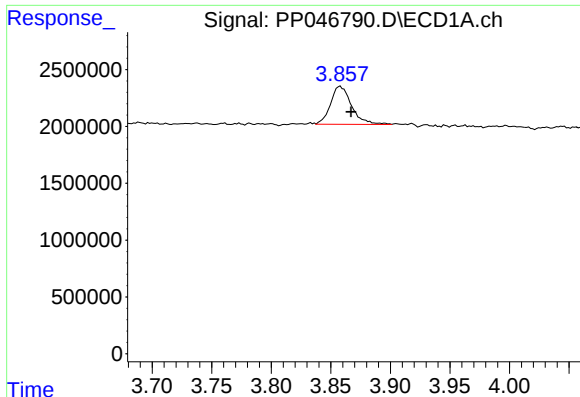

#1 Tetrachloro-m-xylene

R.T.: 3.857 min
Delta R.T.: -0.010 min
Response: 4098982
Conc: 1.70 ng/ml

Instrument :

ECD_P

ClientSampleId :


KMH332L-END-1-2

Manual Integrations

APPROVED


Reviewed By :Yogesh Patel 04/29/2022

Supervised By :mohammad ahmed 04/29/2022

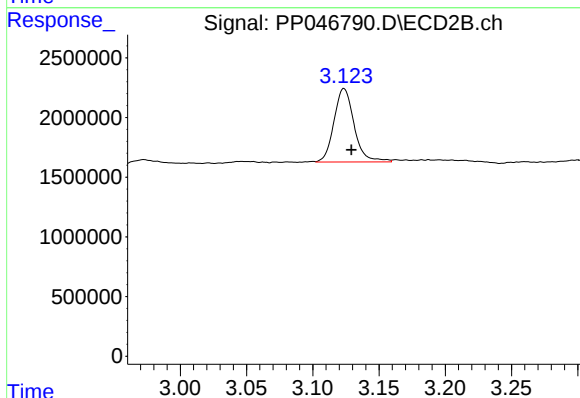


#1 Tetrachloro-m-xylene

R.T.: 3.124 min
Delta R.T.: -0.006 min
Response: 6527381
Conc: 1.99 ng/ml

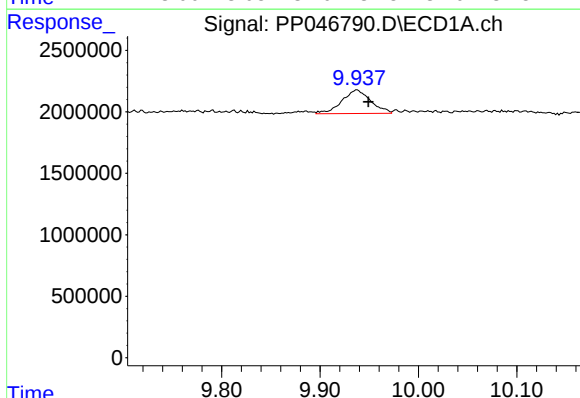

#2 Decachlorobiphenyl

R.T.: 9.938 min
Delta R.T.: -0.011 min
Response: 3877911
Conc: 2.64 ng/ml

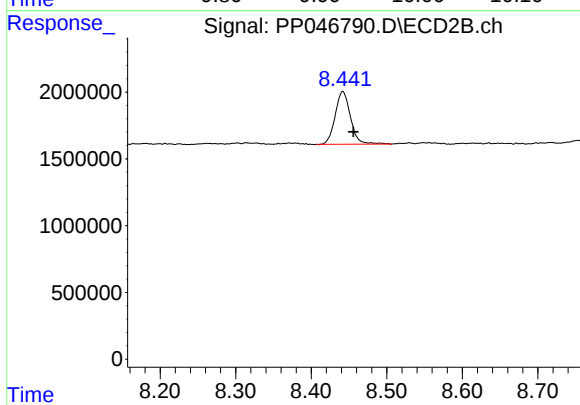

#2 Decachlorobiphenyl

R.T.: 8.442 min
Delta R.T.: -0.014 min
Response: 5585680
Conc: 2.34 ng/ml