

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042822\
 Data File : PP046801.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2022 02:50
 Operator : YP\AJ
 Sample : N2597-08 10X
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KMH249C-END-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/29/2022
 Supervised By :mohammad ahmed 04/29/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 05:01:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 22 19:00:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.859	3.124	2912629	4454990	1.207m	1.358
2) SA Decachlor...	9.942	8.442	3461630	5099520	2.352m	2.138

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042822\
Data File : PP046801.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2022 02:50
Operator : YP\AJ
Sample : N2597-08 10X
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KMH249C-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/29/2022
Supervised By :mohammad ahmed 04/29/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 05:01:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 22 19:00:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

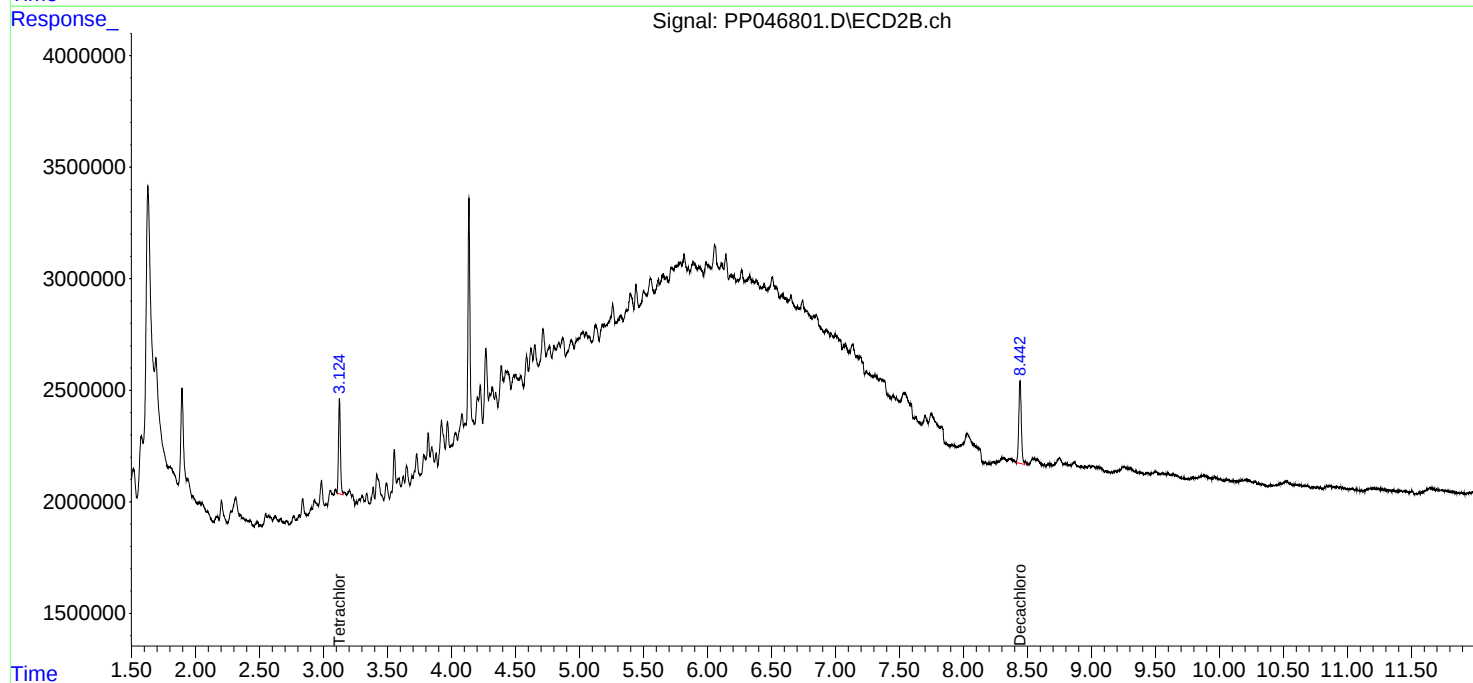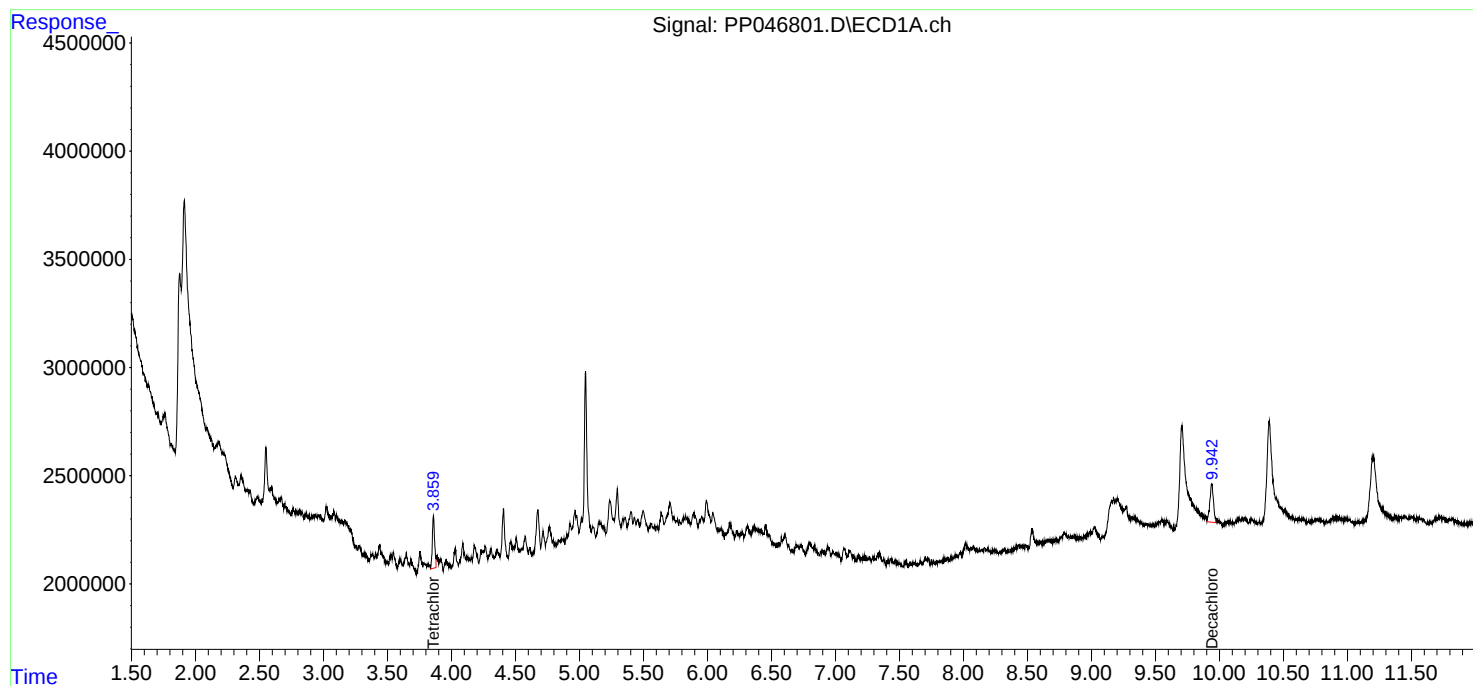

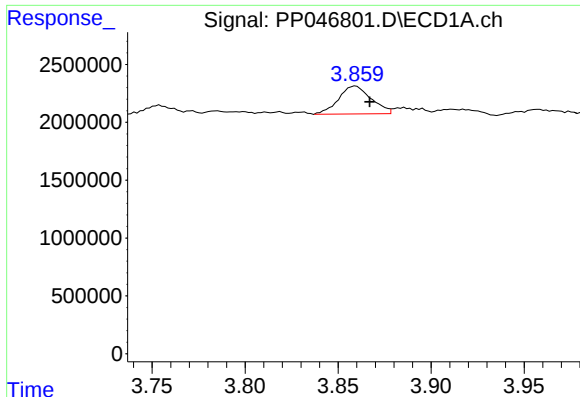


#1 Tetrachloro-m-xylene

R.T.: 3.859 min
Delta R.T.: -0.008 min
Response: 2912629
Conc: 1.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
KMH249C-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/29/2022
Supervised By :mohammad ahmed 04/29/2022

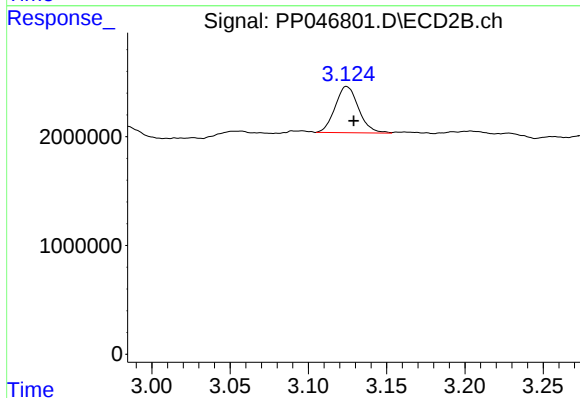


#1 Tetrachloro-m-xylene

R.T.: 3.124 min
Delta R.T.: -0.005 min
Response: 4454990
Conc: 1.36 ng/ml

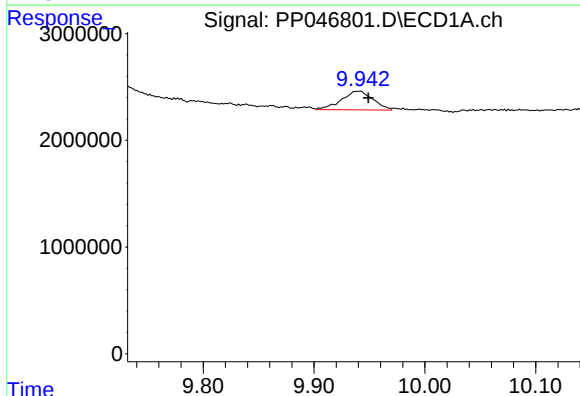

#2 Decachlorobiphenyl

R.T.: 9.942 min
Delta R.T.: -0.007 min
Response: 3461630
Conc: 2.35 ng/ml m

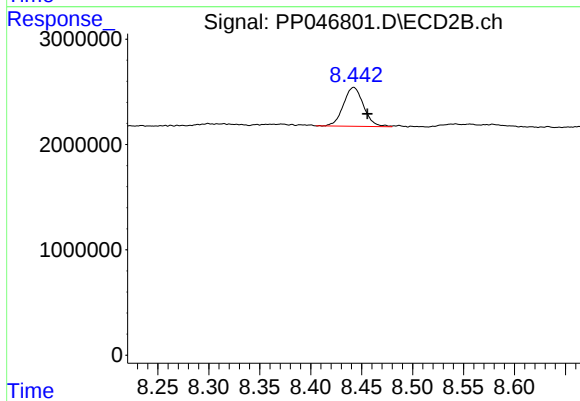

#2 Decachlorobiphenyl

R.T.: 8.442 min
Delta R.T.: -0.014 min
Response: 5099520
Conc: 2.14 ng/ml