

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042921\
 Data File : PP035410.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Apr 2021 22:03
 Operator : DD\AJ
 Sample : AR1254ICC250
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254ICC250

Manual Integrations
 APPROVED

Ankita
 4/30/2021 2:27:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 06:06:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 30 05:58:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.790	4.208	1199755	845809	25.417	25.758
2) SA Decachlor...	10.665	9.475	1077350	539538	26.169	27.231
Target Compounds						
26) L6 AR-1254-1	6.999	6.315	466964	387928	268.395m	269.712
27) L6 AR-1254-2	7.228	6.471	719369	345707	267.568	269.462
28) L6 AR-1254-3	7.609	6.891	758625	531691	264.406	268.729
29) L6 AR-1254-4	7.904	7.128	531045	318610	263.079	265.769
30) L6 AR-1254-5	8.330	7.553	625143	488796	260.673	266.691

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042921\
Data File : PP035410.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Apr 2021 22:03
Operator : DD\AJ
Sample : AR1254ICC250
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
AR1254ICC250


Manual Integrations
APPROVED

Ankita
4/30/2021 2:27:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 06:06:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 30 05:58:56 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

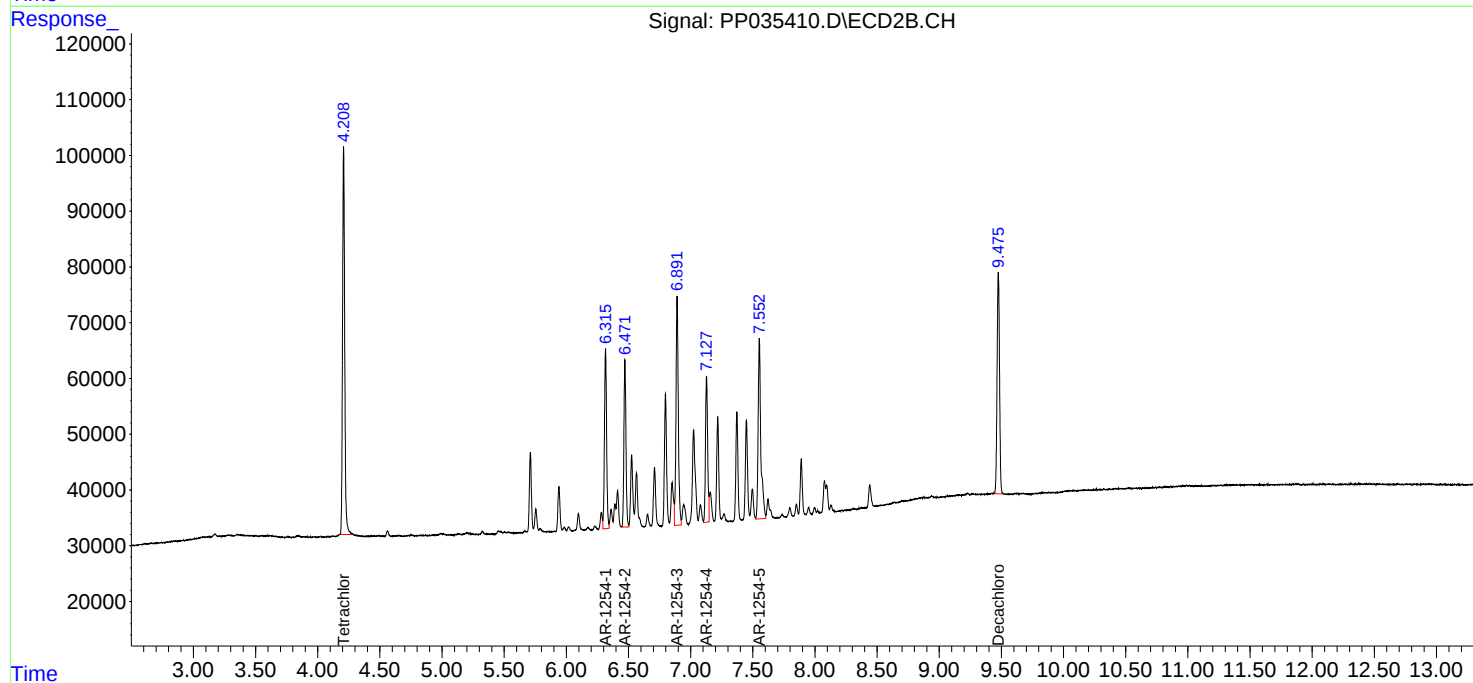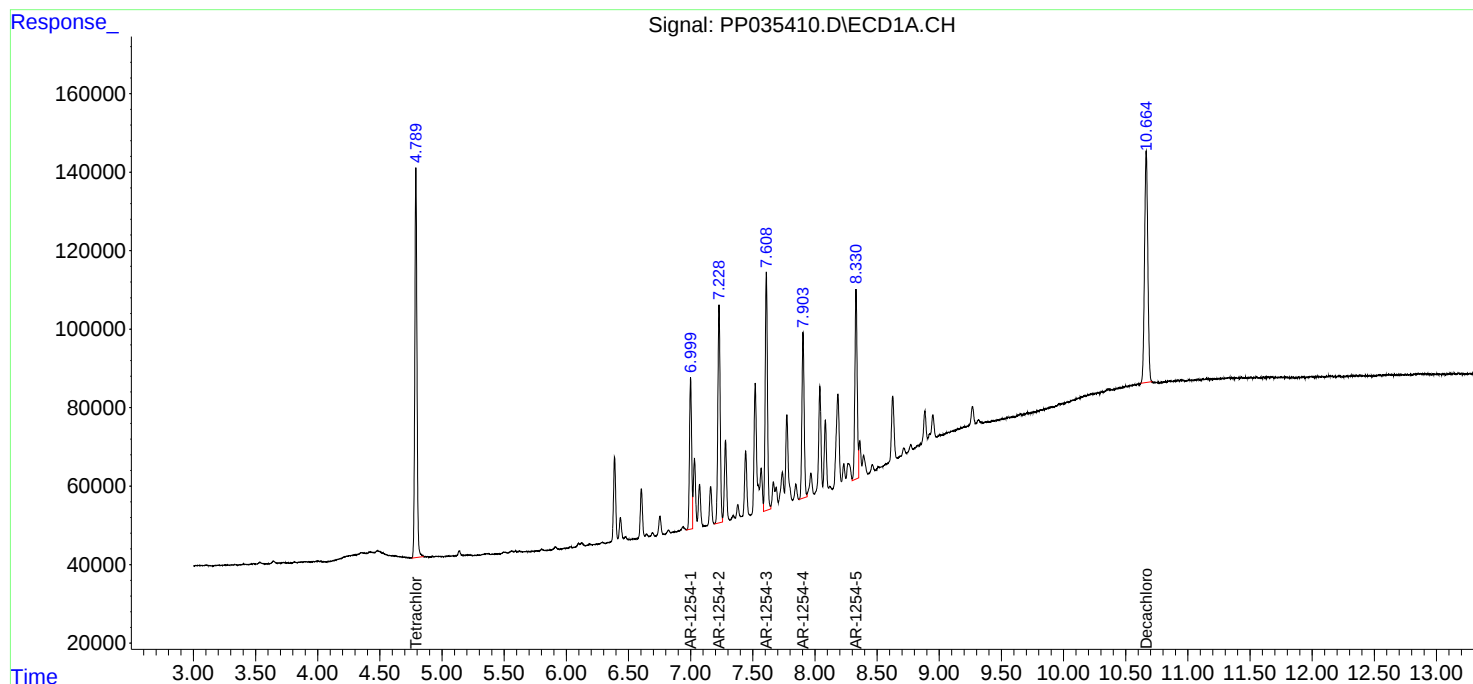

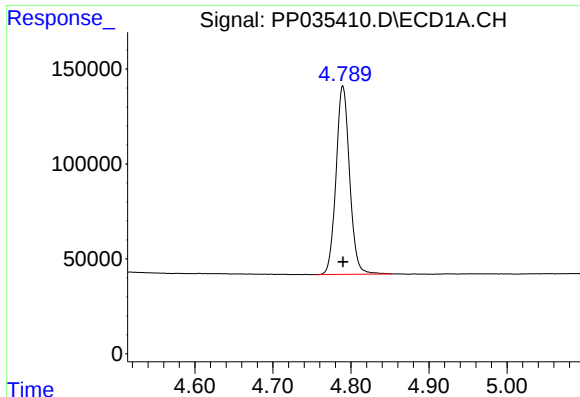


#1 Tetrachloro-m-xylene

R.T.: 4.790 min
Delta R.T.: 0.000 min
Response: 1199755
Conc: 25.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC250


Manual Integrations
APPROVED

Ankita
4/30/2021 2:27:13 PM

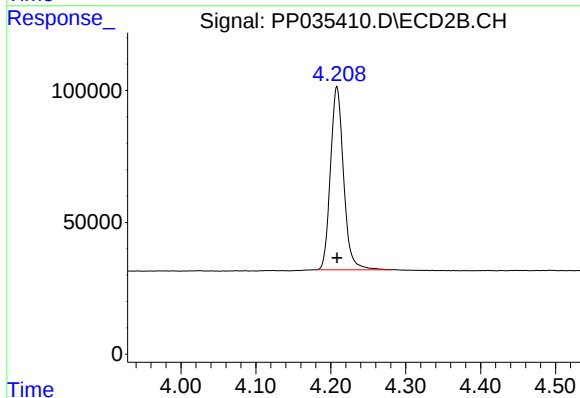


#1 Tetrachloro-m-xylene

R.T.: 4.208 min
Delta R.T.: 0.000 min
Response: 845809
Conc: 25.76 ng/ml

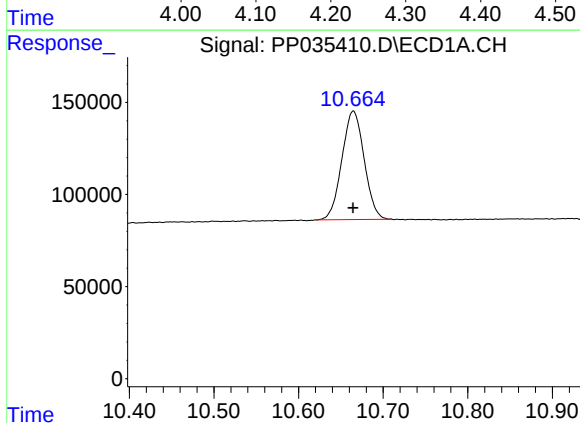


#2 Decachlorobiphenyl

R.T.: 10.665 min
Delta R.T.: 0.000 min
Response: 1077350
Conc: 26.17 ng/ml

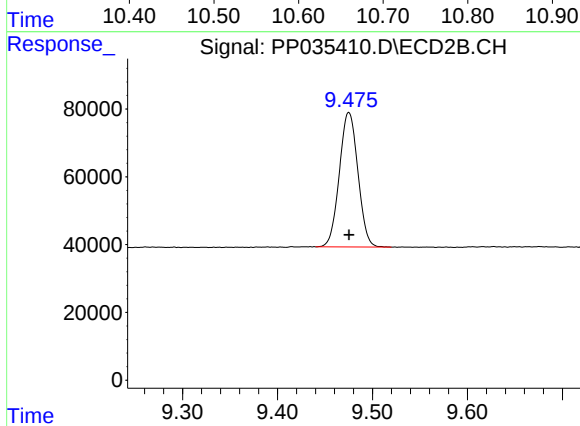

#2 Decachlorobiphenyl

R.T.: 9.475 min
Delta R.T.: 0.000 min
Response: 539538
Conc: 27.23 ng/ml

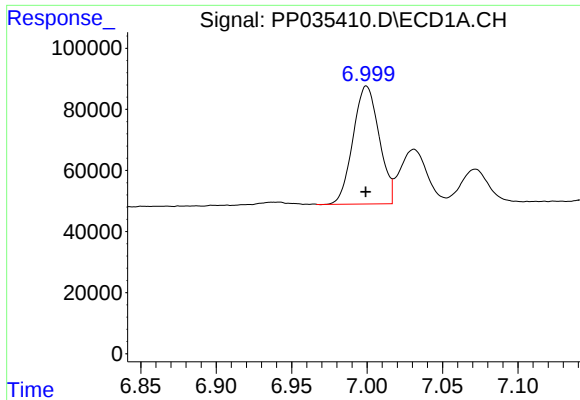


#26 AR-1254-1

R.T.: 6.999 min
Delta R.T.: 0.000 min
Response: 466964
Conc: 268.40 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1254ICC250


Manual Integrations
APPROVED

Ankita
4/30/2021 2:27:13 PM

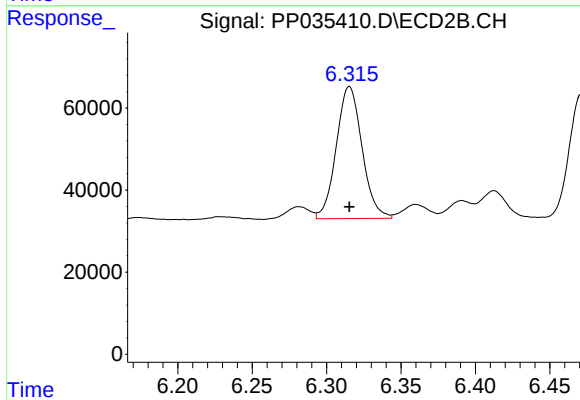


#26 AR-1254-1

R.T.: 6.315 min
Delta R.T.: 0.000 min
Response: 387928
Conc: 269.71 ng/ml

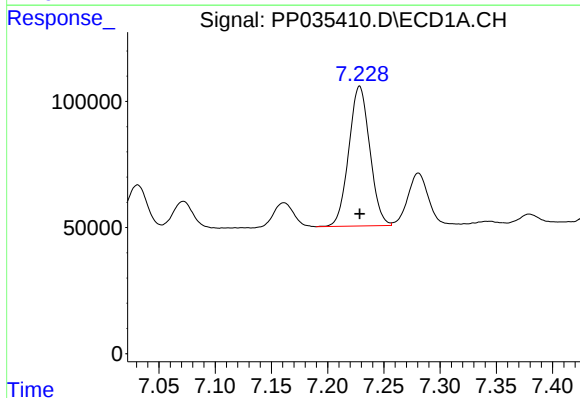


#27 AR-1254-2

R.T.: 7.228 min
Delta R.T.: 0.000 min
Response: 719369
Conc: 267.57 ng/ml

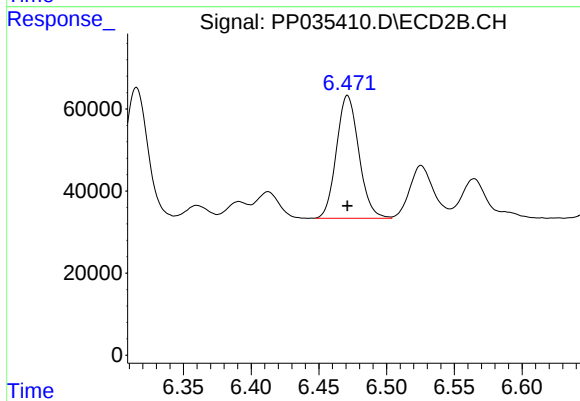

#27 AR-1254-2

R.T.: 6.471 min
Delta R.T.: 0.000 min
Response: 345707
Conc: 269.46 ng/ml

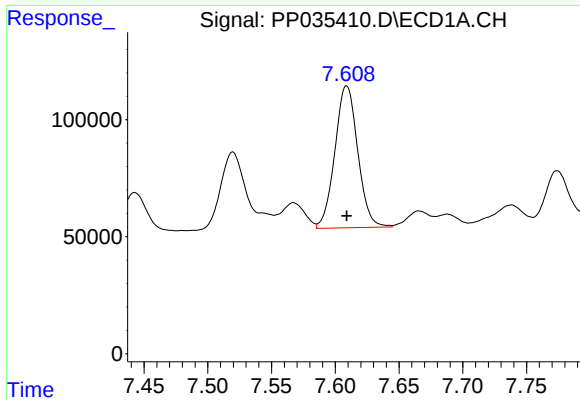


#28 AR-1254-3

R.T.: 7.609 min
Delta R.T.: 0.000 min
Response: 758625
Conc: 264.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC250


Manual Integrations
APPROVED

Ankita
4/30/2021 2:27:13 PM

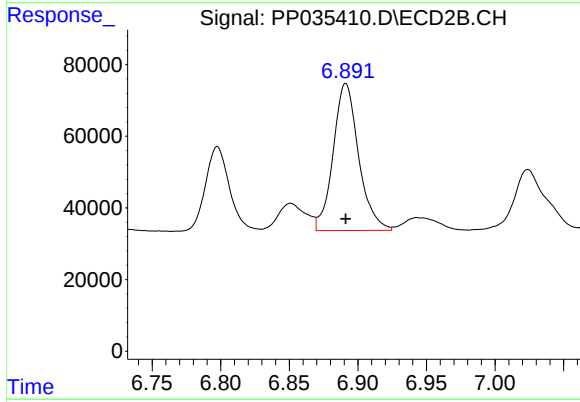


#28 AR-1254-3

R.T.: 6.891 min
Delta R.T.: 0.000 min
Response: 531691
Conc: 268.73 ng/ml

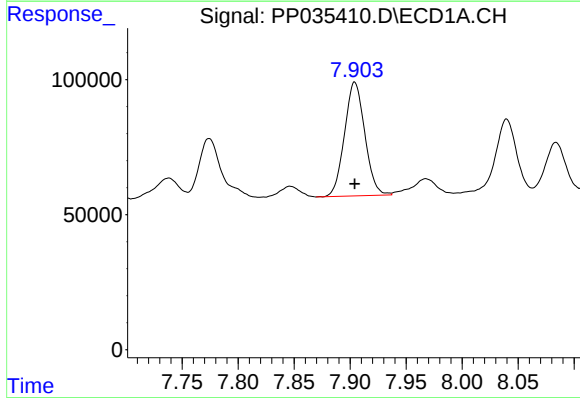


#29 AR-1254-4

R.T.: 7.904 min
Delta R.T.: 0.000 min
Response: 531045
Conc: 263.08 ng/ml

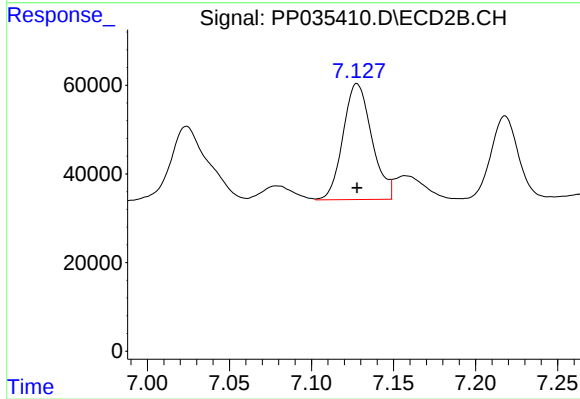

#29 AR-1254-4

R.T.: 7.128 min
Delta R.T.: 0.000 min
Response: 318610
Conc: 265.77 ng/ml

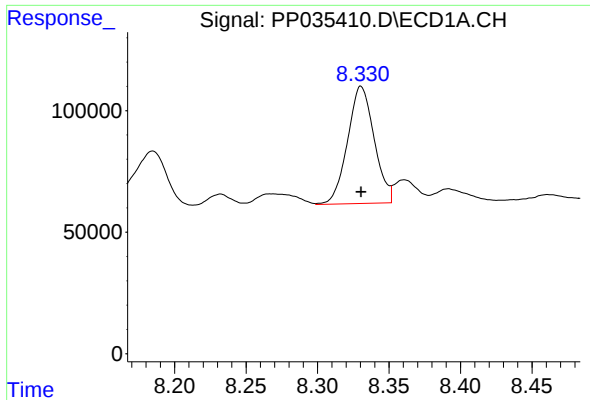


#30 AR-1254-5

R.T.: 8.330 min
Delta R.T.: 0.000 min
Response: 625143
Conc: 260.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254ICC250

Manual Integrations
APPROVED

Ankita
4/30/2021 2:27:13 PM

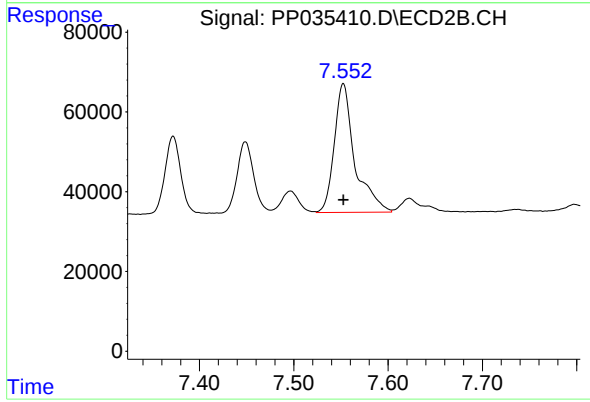

#30 AR-1254-5

R.T.: 7.553 min
Delta R.T.: 0.000 min
Response: 488796
Conc: 266.69 ng/ml