

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042922\
 Data File : PP046852.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2022 00:23
 Operator : YP\AJ
 Sample : N2609-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WC-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh
 Patel
 05/02/2022

Supervised By :mohammad
 ahmed
 05/02/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 05:28:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 22 19:00:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.869	3.124	51545328	80278828	21.353m	24.473
2) SA Decachlor...	9.956	8.446	23965884	39047509	16.287	16.370

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042922\
Data File : PP046852.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2022 00:23
Operator : YP\AJ
Sample : N2609-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
WC-2



Manual Integrations
APPROVED


Reviewed By :Yogesh
Patel
05/02/2022

Supervised By :mohammad
ahmed
05/02/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 05:28:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 22 19:00:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

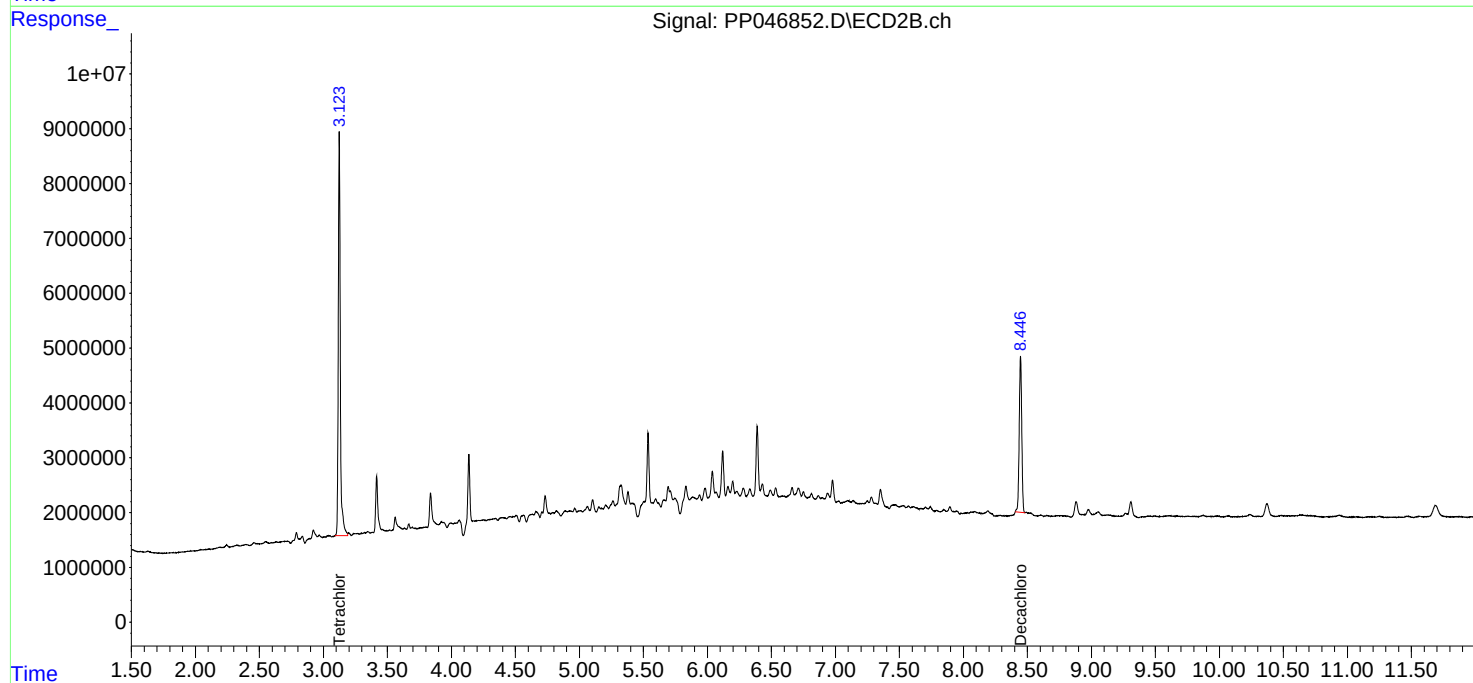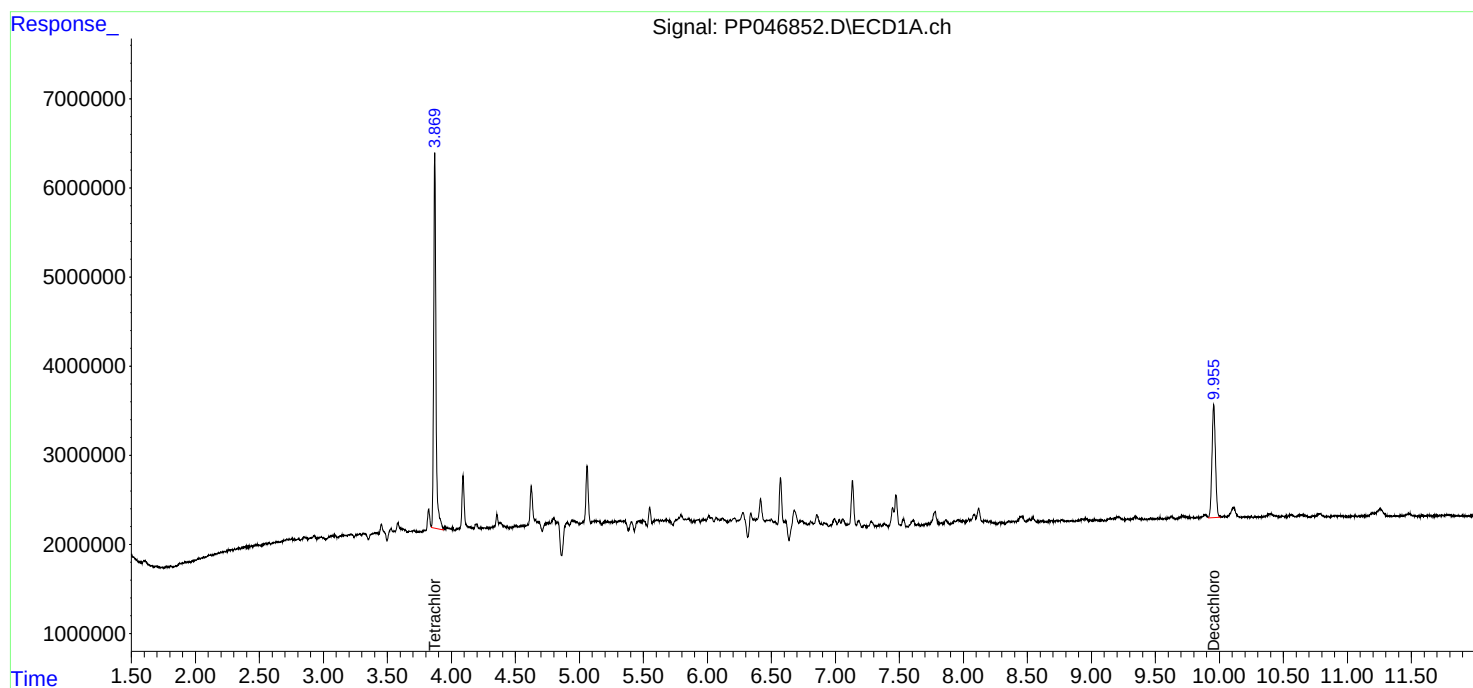

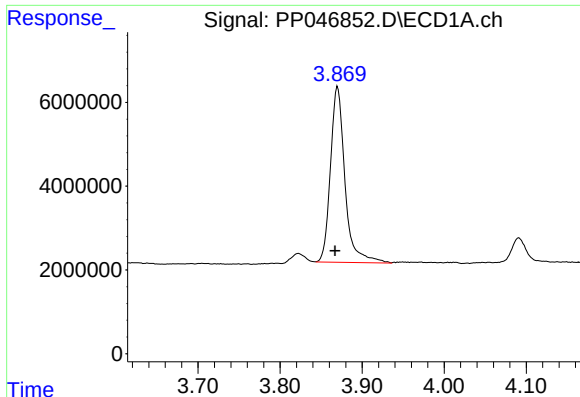

#1 Tetrachloro-m-xylene


R.T.: 3.869 min
Delta R.T.: 0.002 min
Response: 51545328
Conc: 21.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
WC-2

Manual Integrations
APPROVED


Reviewed By :Yogesh
Patel
05/02/2022

Supervised By :mohammad
ahmed
05/02/2022

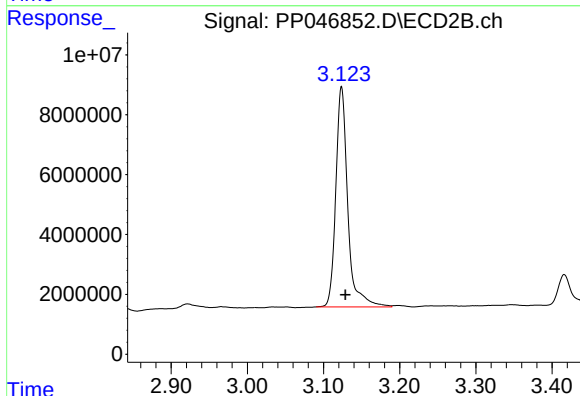


#1 Tetrachloro-m-xylene

R.T.: 3.124 min
Delta R.T.: -0.005 min
Response: 80278828
Conc: 24.47 ng/ml

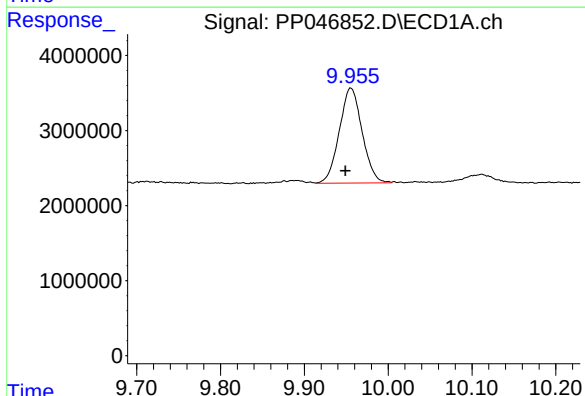

#2 Decachlorobiphenyl

R.T.: 9.956 min
Delta R.T.: 0.007 min
Response: 23965884
Conc: 16.29 ng/ml

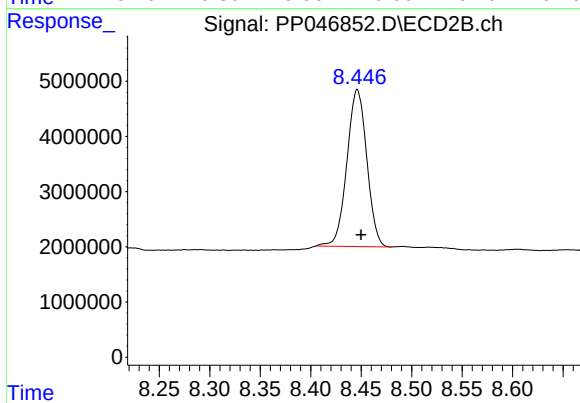

#2 Decachlorobiphenyl

R.T.: 8.446 min
Delta R.T.: -0.004 min
Response: 39047509
Conc: 16.37 ng/ml