

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP043021\
 Data File : PP035431.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Apr 2021 11:06
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 15:16:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 30 07:23:18 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.790	4.208	1008430	725331	19.862	21.305
2) SA Decachlor...	10.660	9.473	937344	486530	23.082	25.107
Target Compounds						
9) L2 AR-1221-2	0.000	4.561	0	8700	N.D.	29.301 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP043021\
Data File : PP035431.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Apr 2021 11:06
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 15:16:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 30 07:23:18 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

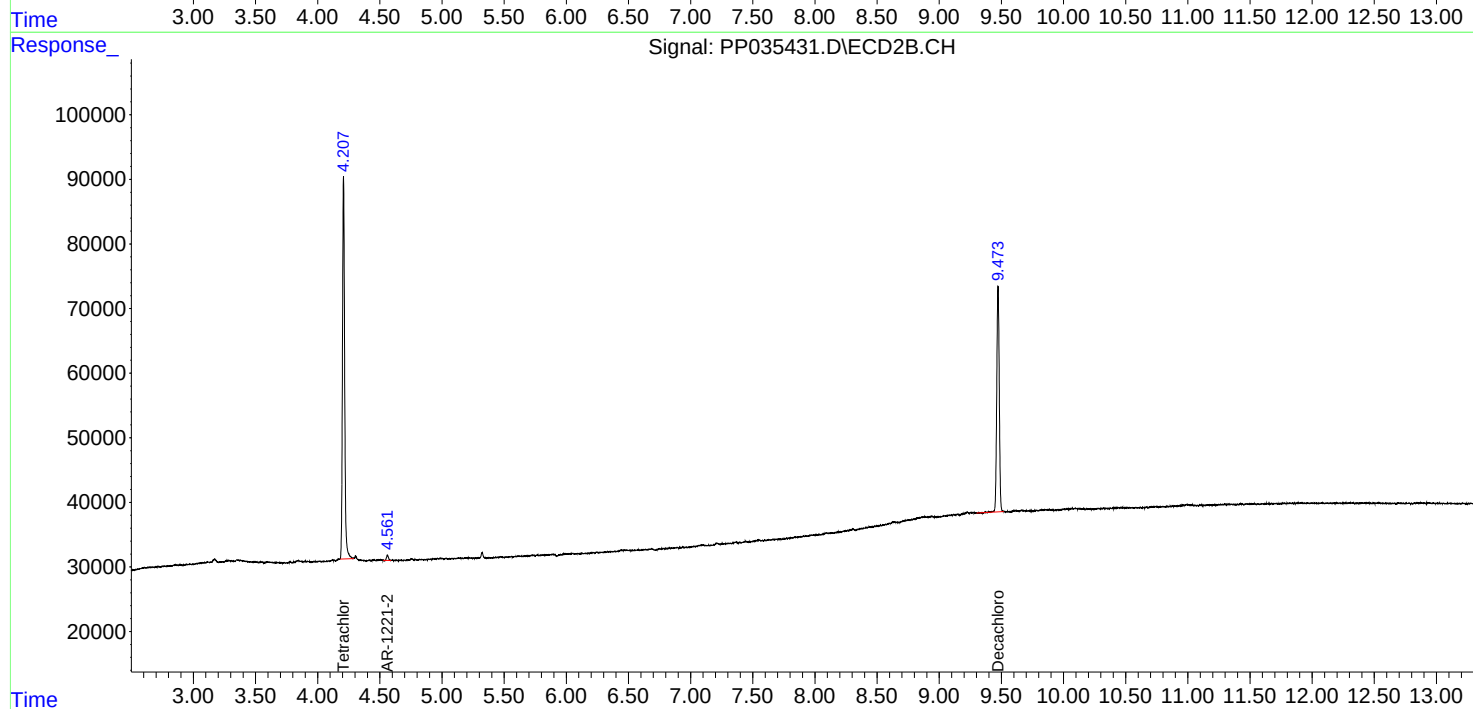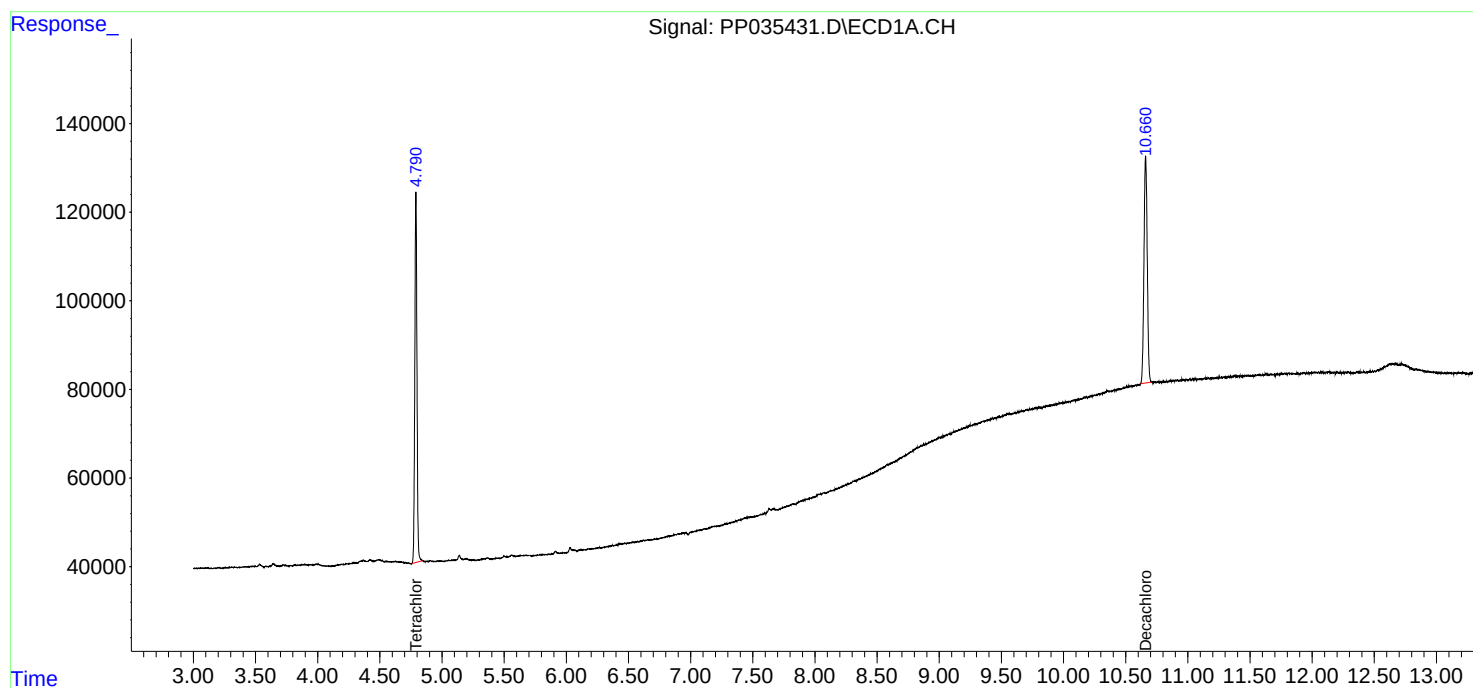


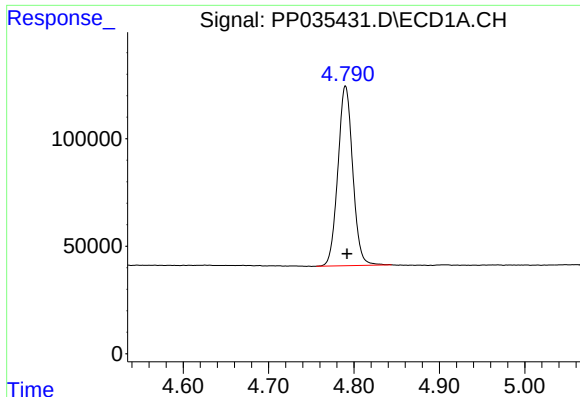

#1 Tetrachloro-m-xylene


R.T.: 4.790 min
Delta R.T.: -0.002 min
Response: 1008430
Conc: 19.86 ng/ml

Instrument :
ECD_P
ClientSampleId :

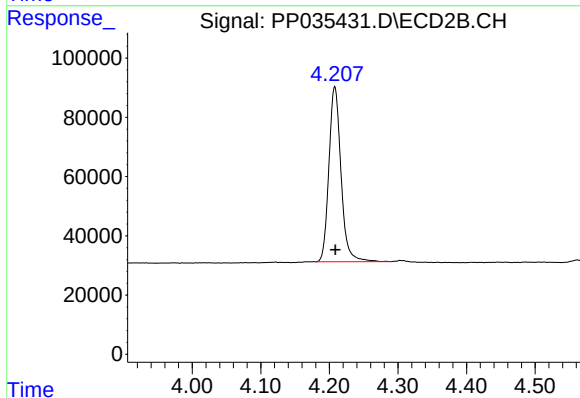


#1 Tetrachloro-m-xylene

R.T.: 4.208 min
Delta R.T.: -0.001 min
Response: 725331
Conc: 21.31 ng/ml

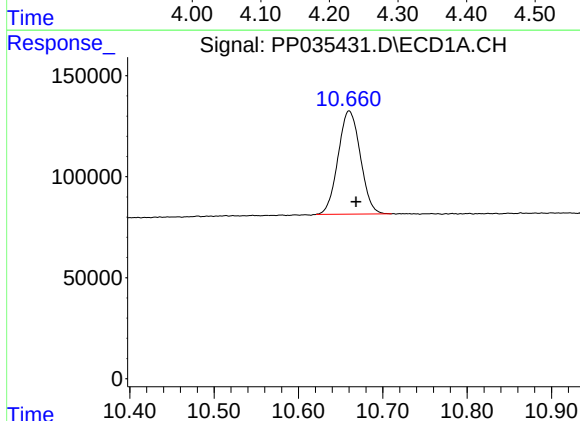


#2 Decachlorobiphenyl

R.T.: 10.660 min
Delta R.T.: -0.008 min
Response: 937344
Conc: 23.08 ng/ml

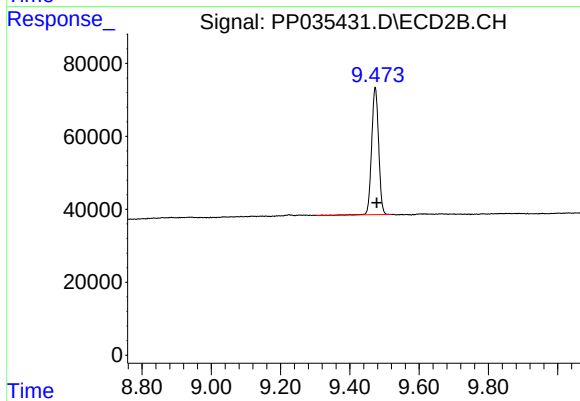

#2 Decachlorobiphenyl


R.T.: 9.473 min
Delta R.T.: -0.004 min
Response: 486530
Conc: 25.11 ng/ml

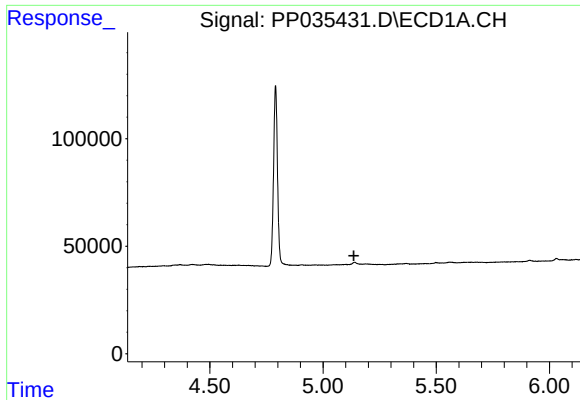

#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 5.136 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

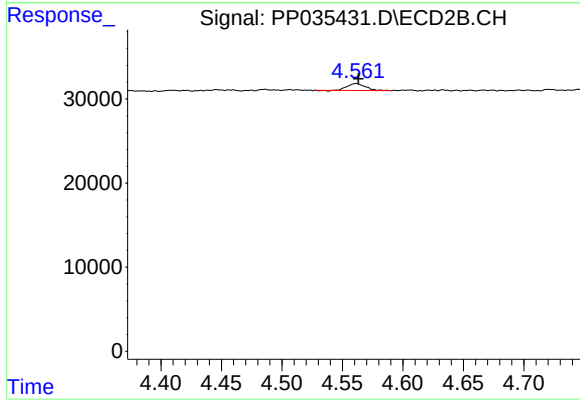

#9 AR-1221-2

R.T.: 4.561 min
Delta R.T.: -0.002 min
Response: 8700
Conc: 29.30 ng/ml