

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP043021\
 Data File : PP035446.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Apr 2021 17:41
 Operator : DD\AJ
 Sample : M2205-14 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 18:52:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 30 07:23:18 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.790	4.209	89245	76057	1.758	2.234 #
2) SA Decachlor...	0.000	9.475	0	43751	N.D.	2.258 #
Target Compounds						
34) L7 AR-1260-4	0.000	7.848	0	16480	N.D.	14.897 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP043021\
Data File : PP035446.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Apr 2021 17:41
Operator : DD\AJ
Sample : M2205-14 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 18:52:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 30 07:23:18 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

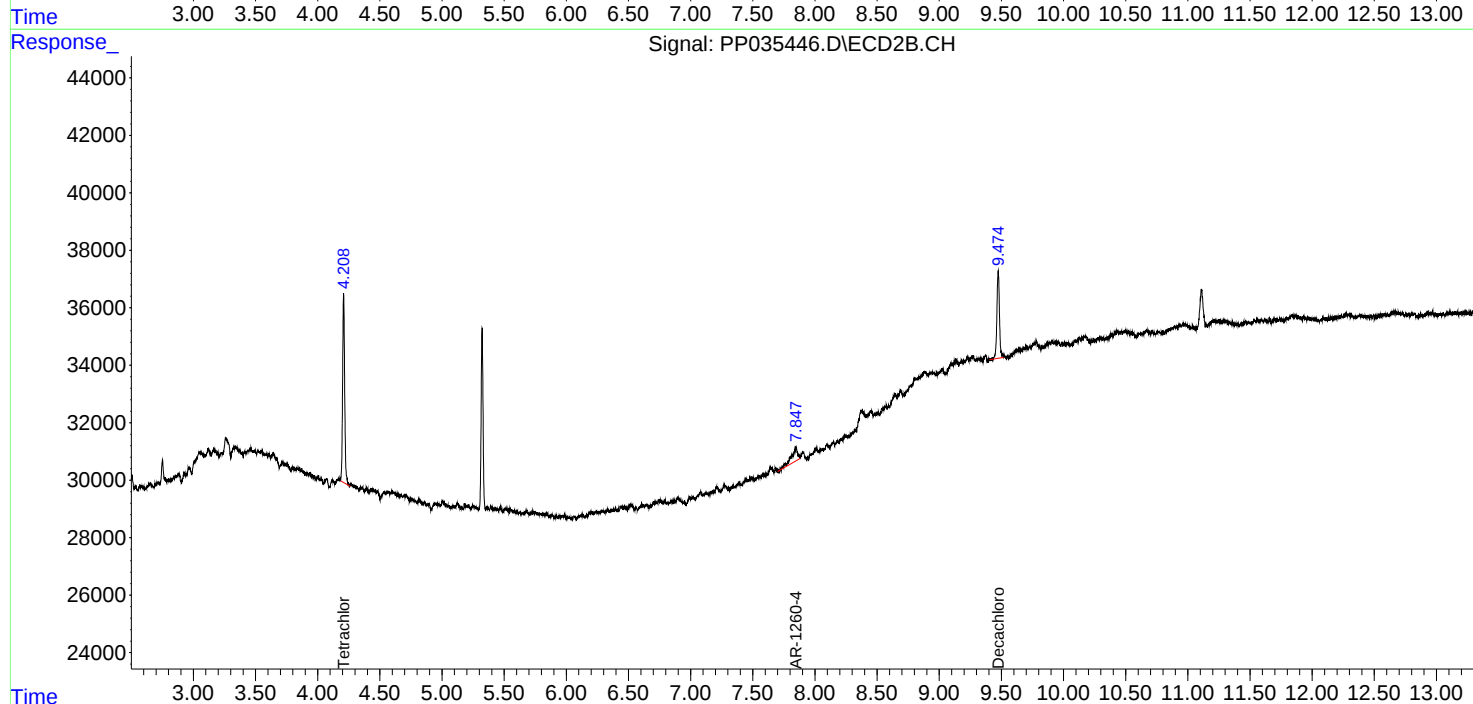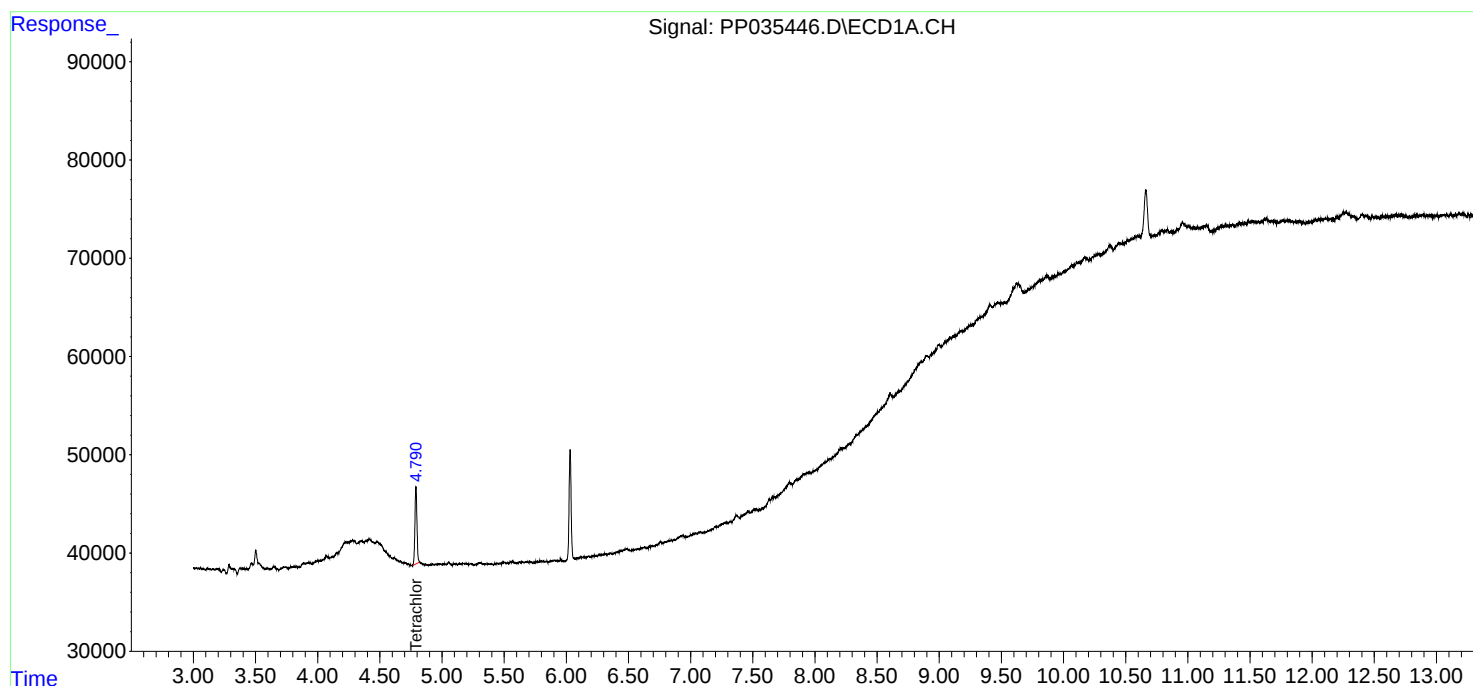


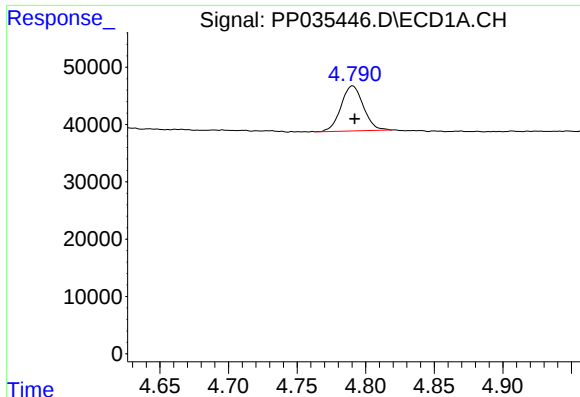

#1 Tetrachloro-m-xylene


R.T.: 4.790 min
Delta R.T.: -0.002 min
Response: 89245
Conc: 1.76 ng/ml

Instrument :
ECD_P
ClientSampleId :

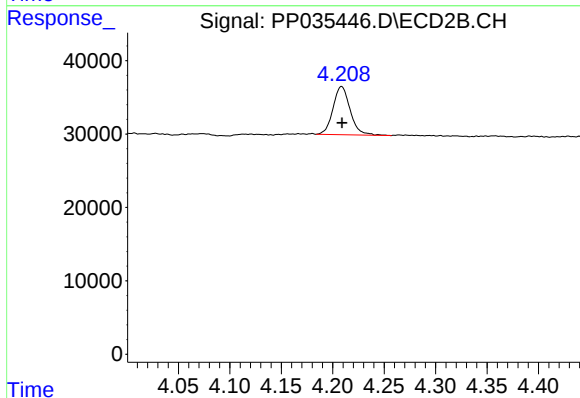


#1 Tetrachloro-m-xylene

R.T.: 4.209 min
Delta R.T.: 0.000 min
Response: 76057
Conc: 2.23 ng/ml

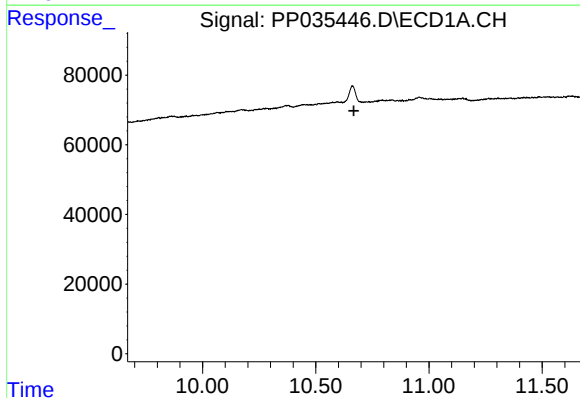


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.668 min
Response: 0
Conc: N.D.

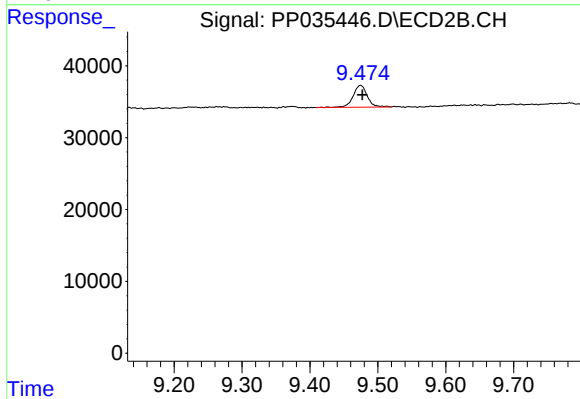

#2 Decachlorobiphenyl


R.T.: 9.475 min
Delta R.T.: -0.003 min
Response: 43751
Conc: 2.26 ng/ml

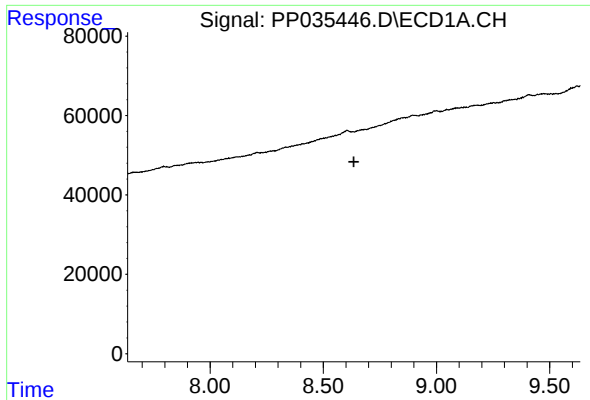

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 8.635 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

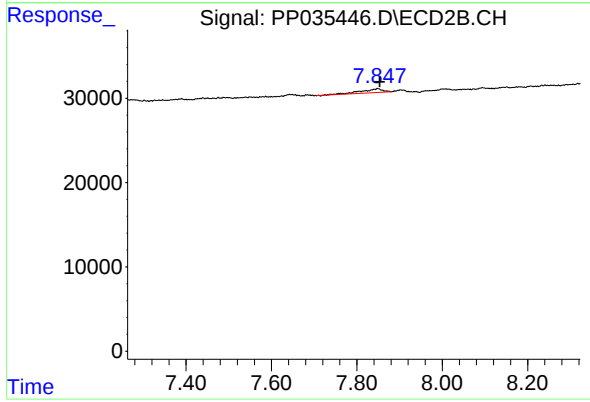

#34 AR-1260-4

R.T.: 7.848 min
Delta R.T.: -0.005 min
Response: 16480
Conc: 14.90 ng/ml