

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP043021\
 Data File : PP035444.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Apr 2021 17:07
 Operator : DD\AJ
 Sample : M2205-11 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KQA103H-END-1-2

Manual Integrations
 APPROVED

Ankita
 5/3/2021 3:25:08 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 17:19:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 30 07:23:18 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.790	4.208	90950	72825	1.791m	2.139m
2) SA Decachlor...	10.659	9.473	87259	42840	2.149m	2.211m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP043021\
Data File : PP035444.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Apr 2021 17:07
Operator : DD\AJ
Sample : M2205-11 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KQA103H-END-1-2


Manual Integrations
APPROVED

Ankita
5/3/2021 3:25:08 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 17:19:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 30 07:23:18 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

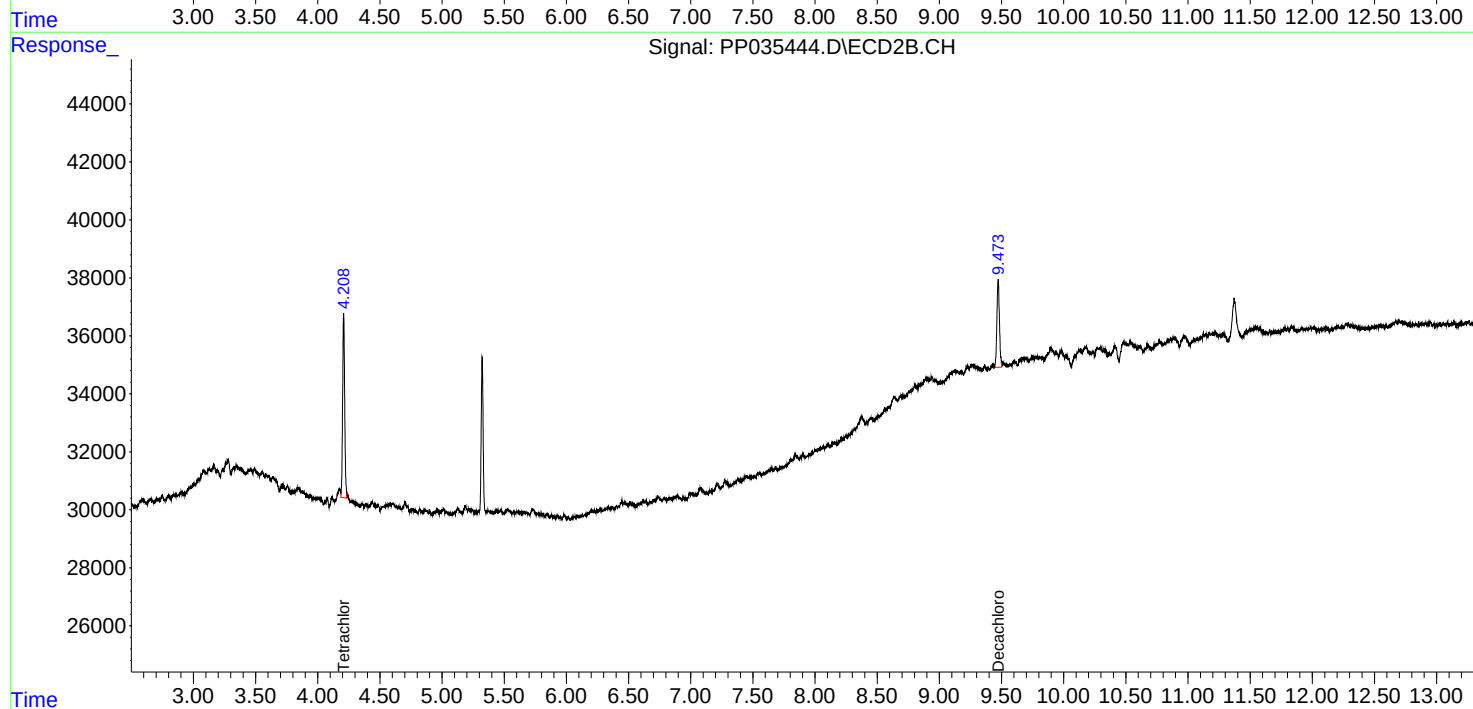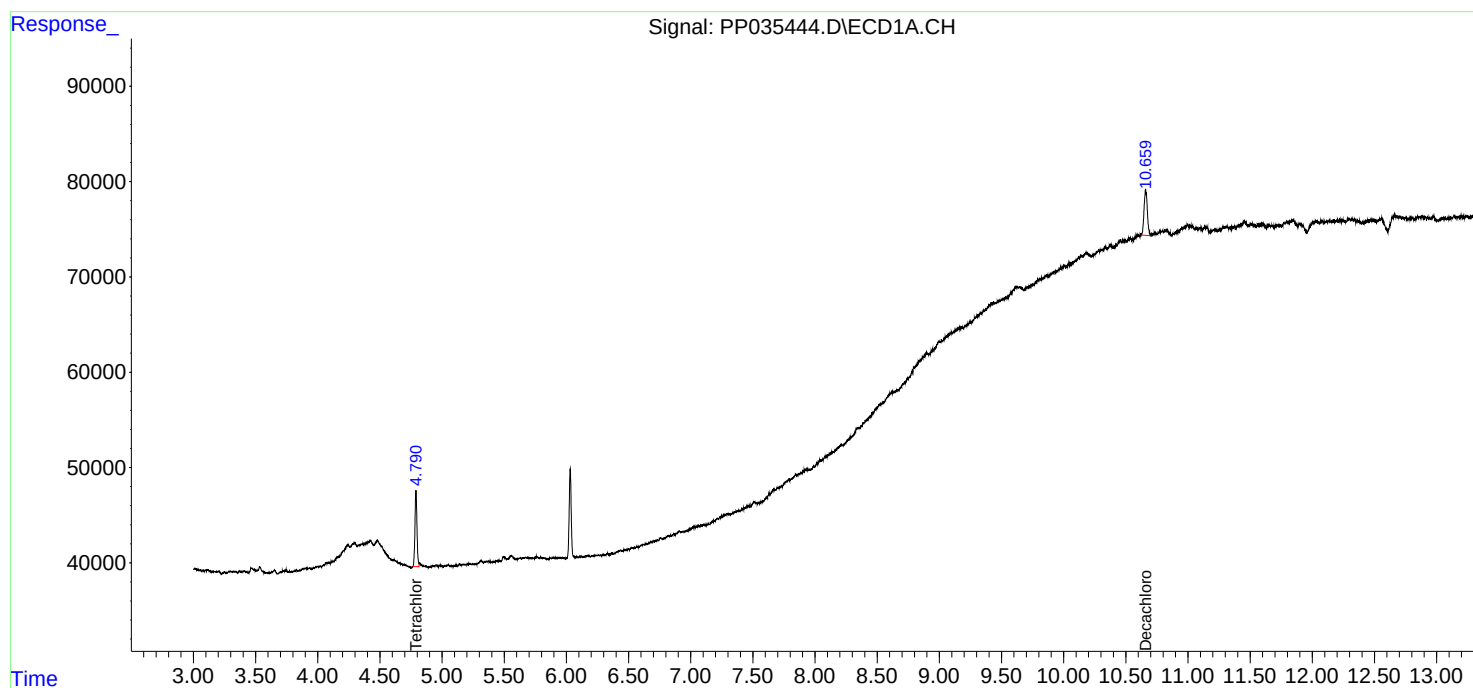

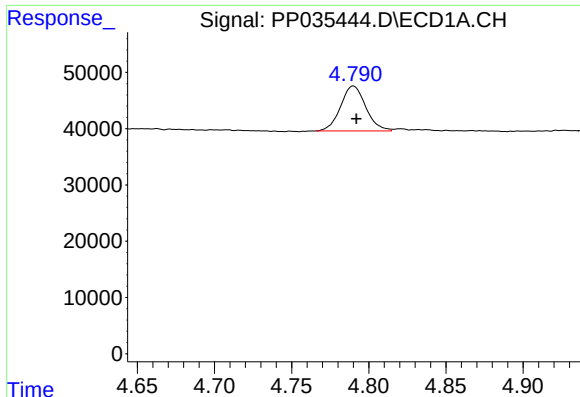


#1 Tetrachloro-m-xylene

R.T.: 4.790 min
Delta R.T.: -0.002 min
Response: 90950
Conc: 1.79 ng/ml m

Instrument :
ECD_P
ClientSampleId :
KQA103H-END-1-2


Manual Integrations
APPROVED

Ankita
5/3/2021 3:25:08 PM

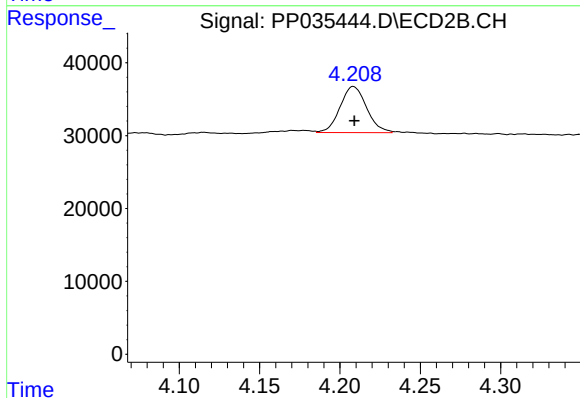


#1 Tetrachloro-m-xylene

R.T.: 4.208 min
Delta R.T.: -0.001 min
Response: 72825
Conc: 2.14 ng/ml m

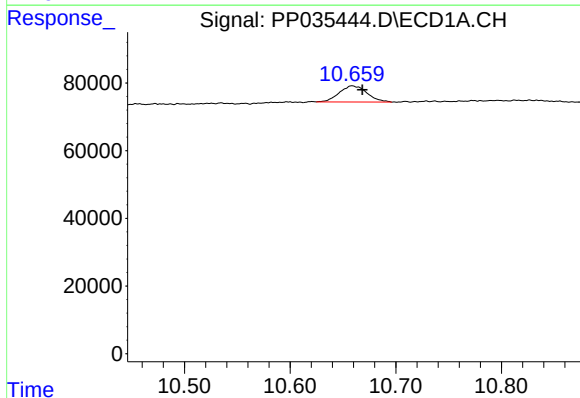

#2 Decachlorobiphenyl

R.T.: 10.659 min
Delta R.T.: -0.010 min
Response: 87259
Conc: 2.15 ng/ml m

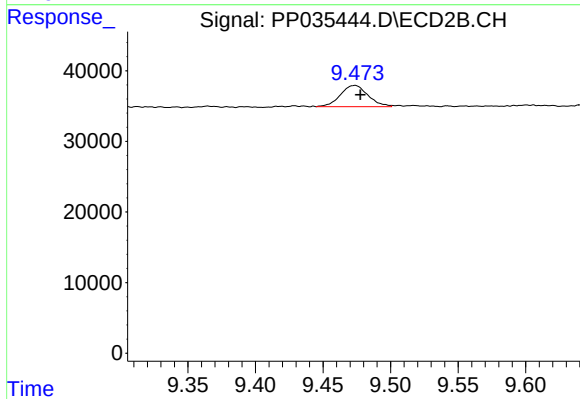

#2 Decachlorobiphenyl

R.T.: 9.473 min
Delta R.T.: -0.004 min
Response: 42840
Conc: 2.21 ng/ml m