

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP043021\
 Data File : PP035450.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Apr 2021 18:49
 Operator : DD\AJ
 Sample : M2216-01 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KZH01ZP-END-1-1

Manual Integrations
 APPROVED

Ankita
 5/3/2021 3:25:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 19:08:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 30 07:23:18 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.790	4.208	141962	96948	2.796m	2.848m
2) SA Decachlor...	10.660	9.472	113815	55886	2.803m	2.884m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP043021\
Data File : PP035450.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Apr 2021 18:49
Operator : DD\AJ
Sample : M2216-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KZH01ZP-END-1-1


Manual Integrations
APPROVED

Ankita
5/3/2021 3:25:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 19:08:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 30 07:23:18 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

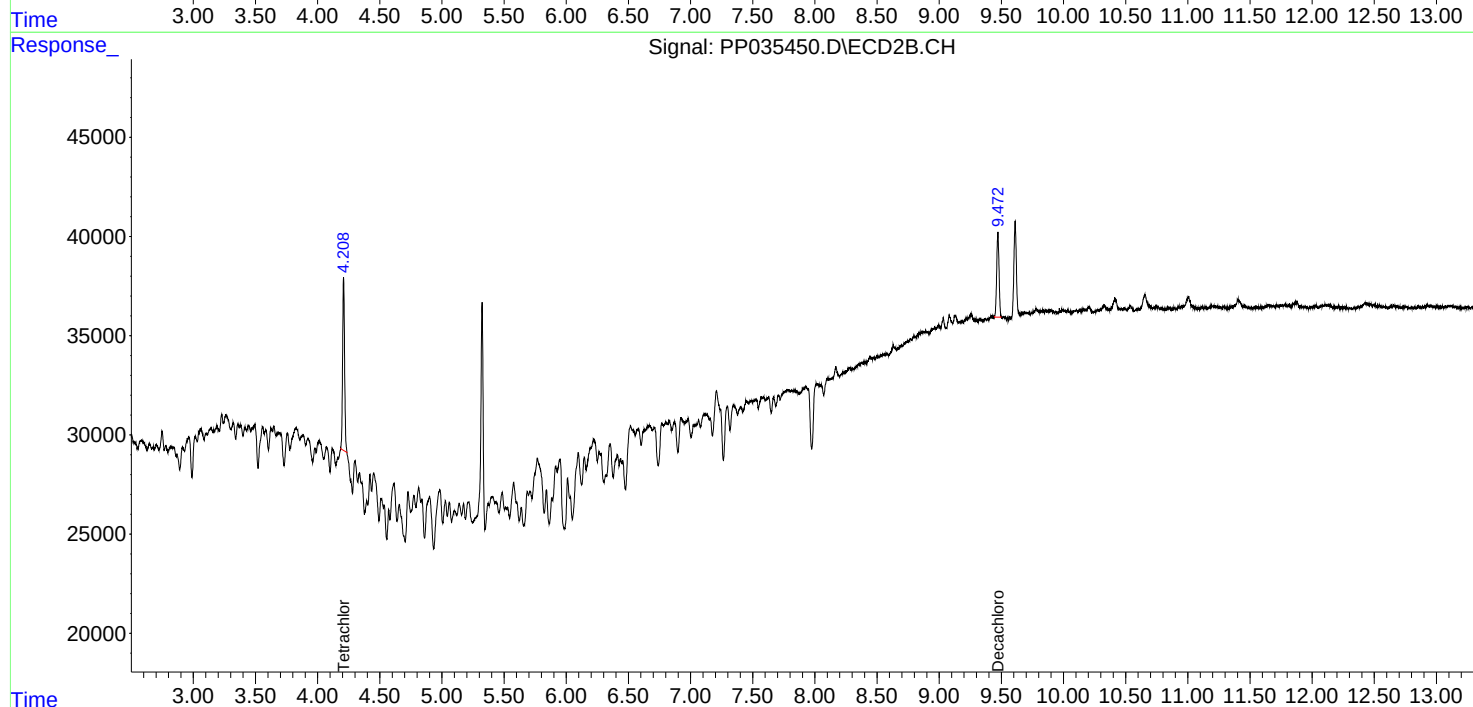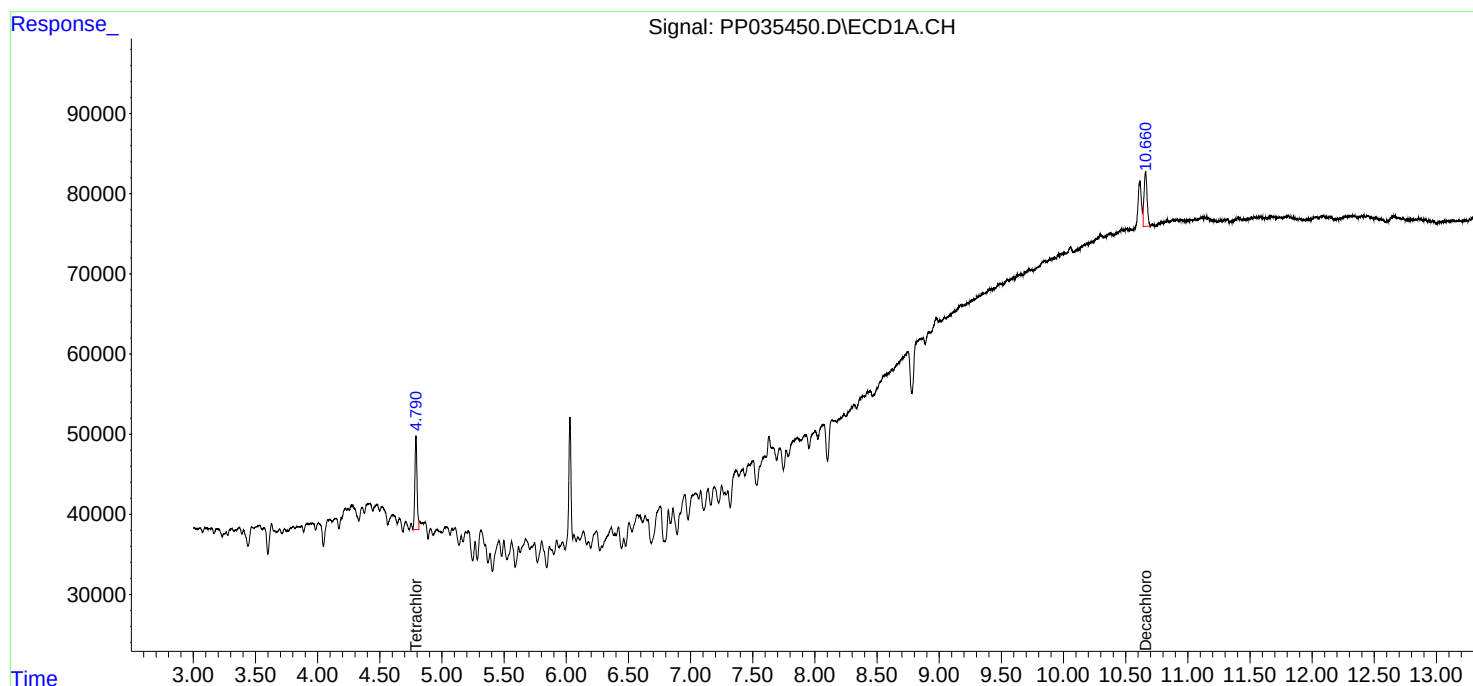

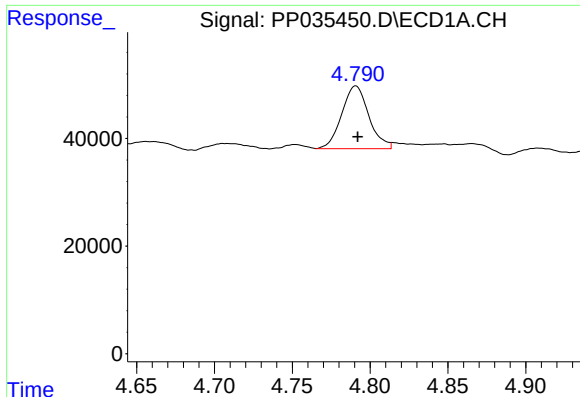


#1 Tetrachloro-m-xylene

R.T.: 4.790 min
Delta R.T.: -0.002 min
Response: 141962
Conc: 2.80 ng/ml m

Instrument :
ECD_P
ClientSampleId :
KZH01ZP-END-1-1


Manual Integrations
APPROVED

Ankita
5/3/2021 3:25:20 PM

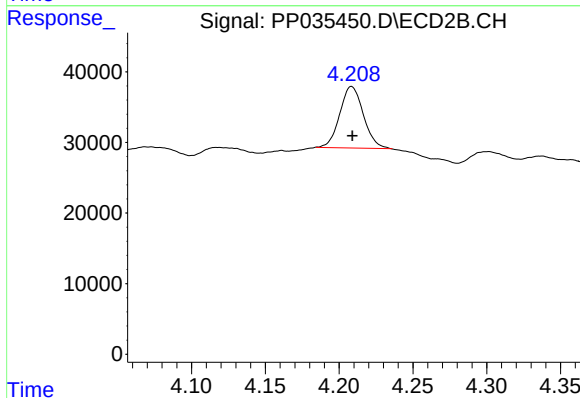


#1 Tetrachloro-m-xylene

R.T.: 4.208 min
Delta R.T.: 0.000 min
Response: 96948
Conc: 2.85 ng/ml m

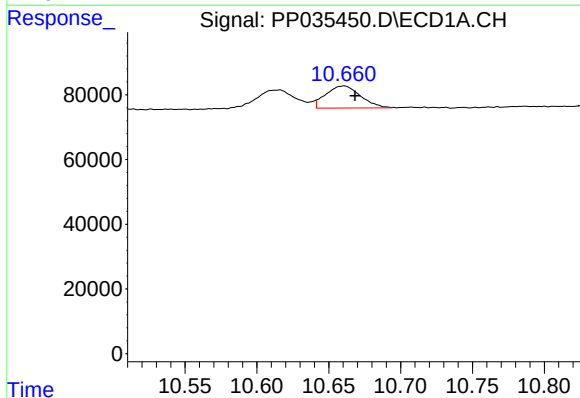

#2 Decachlorobiphenyl

R.T.: 10.660 min
Delta R.T.: -0.008 min
Response: 113815
Conc: 2.80 ng/ml m

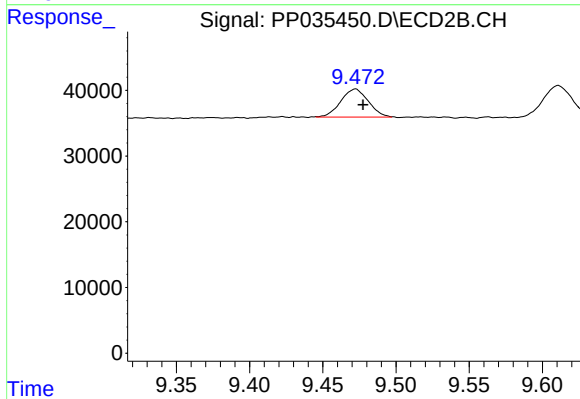

#2 Decachlorobiphenyl

R.T.: 9.472 min
Delta R.T.: -0.005 min
Response: 55886
Conc: 2.88 ng/ml m