

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP043021\
 Data File : PP035452.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Apr 2021 19:22
 Operator : DD\AJ
 Sample : M2216-03 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KZH01ZP-END-2-1

Manual Integrations
 APPROVED

Ankita
 5/3/2021 3:25:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 02:42:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 30 07:23:18 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.792	4.209	125126	108839	2.464	3.197m#
2) SA Decachlor...	10.663	9.474	121361	56673	2.988m	2.925m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP043021\
Data File : PP035452.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Apr 2021 19:22
Operator : DD\AJ
Sample : M2216-03 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KZH01ZP-END-2-1


Manual Integrations
APPROVED

Ankita
5/3/2021 3:25:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 02:42:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 30 07:23:18 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

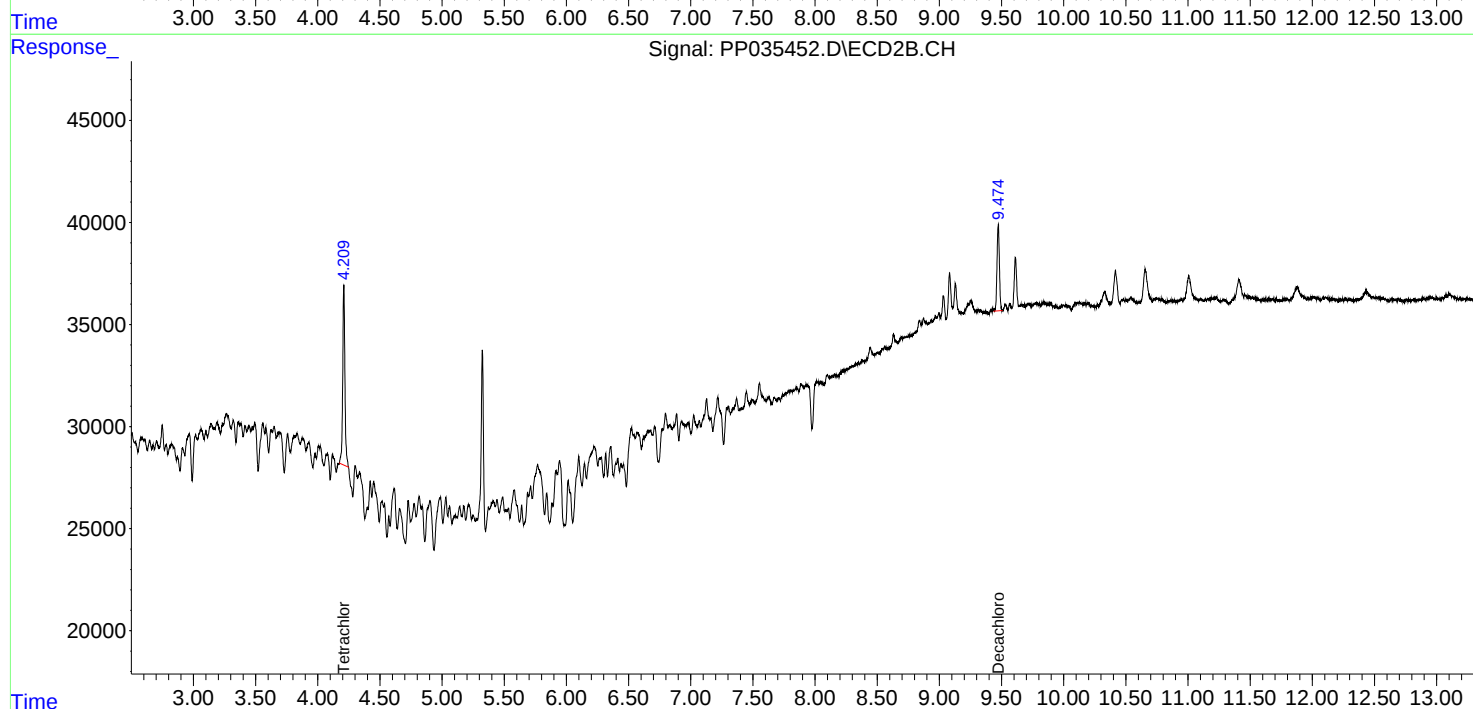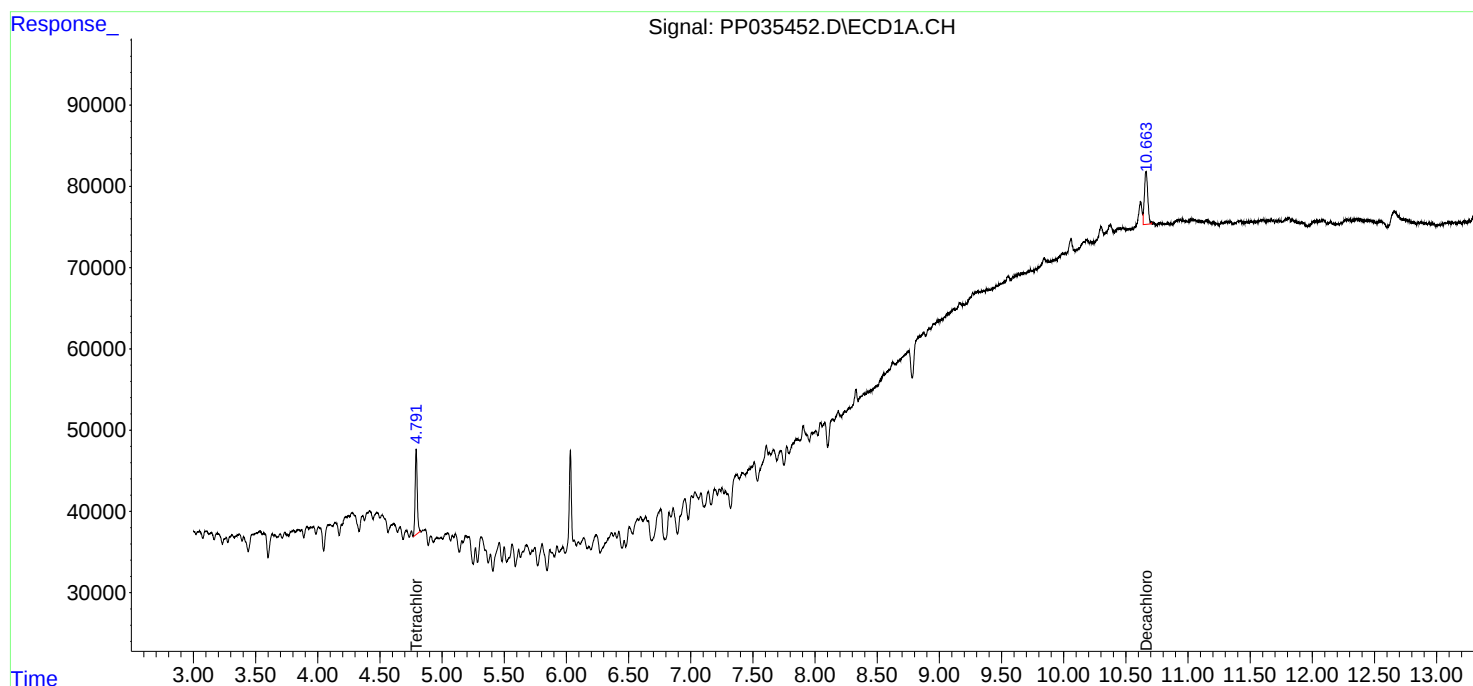

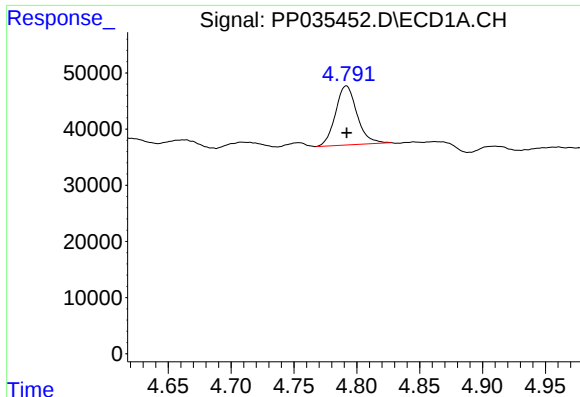


#1 Tetrachloro-m-xylene

R.T.: 4.792 min
Delta R.T.: 0.000 min
Response: 125126
Conc: 2.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
KZH01ZP-END-2-1


Manual Integrations
APPROVED

Ankita
5/3/2021 3:25:23 PM

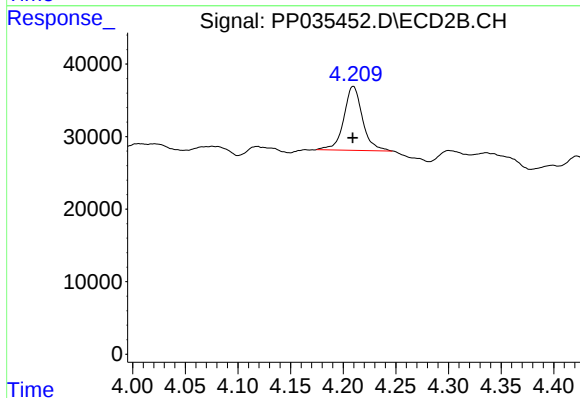


#1 Tetrachloro-m-xylene

R.T.: 4.209 min
Delta R.T.: 0.000 min
Response: 108839
Conc: 3.20 ng/ml m

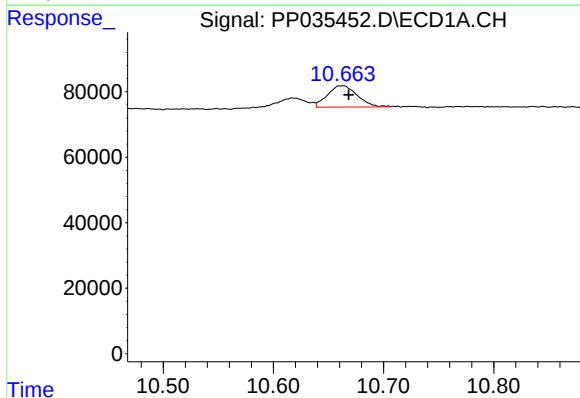

#2 Decachlorobiphenyl

R.T.: 10.663 min
Delta R.T.: -0.005 min
Response: 121361
Conc: 2.99 ng/ml m

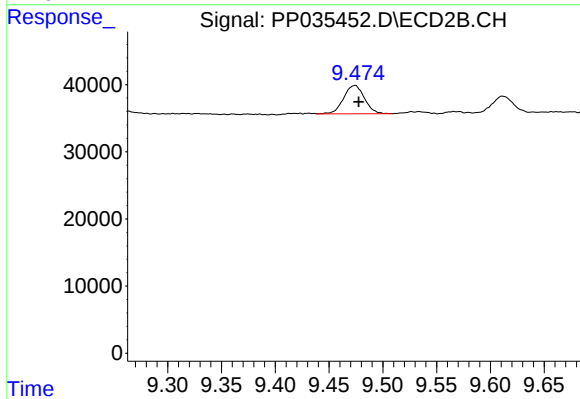

#2 Decachlorobiphenyl

R.T.: 9.474 min
Delta R.T.: -0.003 min
Response: 56673
Conc: 2.92 ng/ml m