

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050123\
 Data File : PP057307.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2023 09:45
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 05:36:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 01 18:39:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.416	3.641	56368788	43182586	23.935	24.356
2) SA Decachlor...	10.263	8.714	43227184	50342105	26.202	25.653

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050123\
Data File : PP057307.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2023 09:45
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 05:36:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050123.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 01 18:39:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

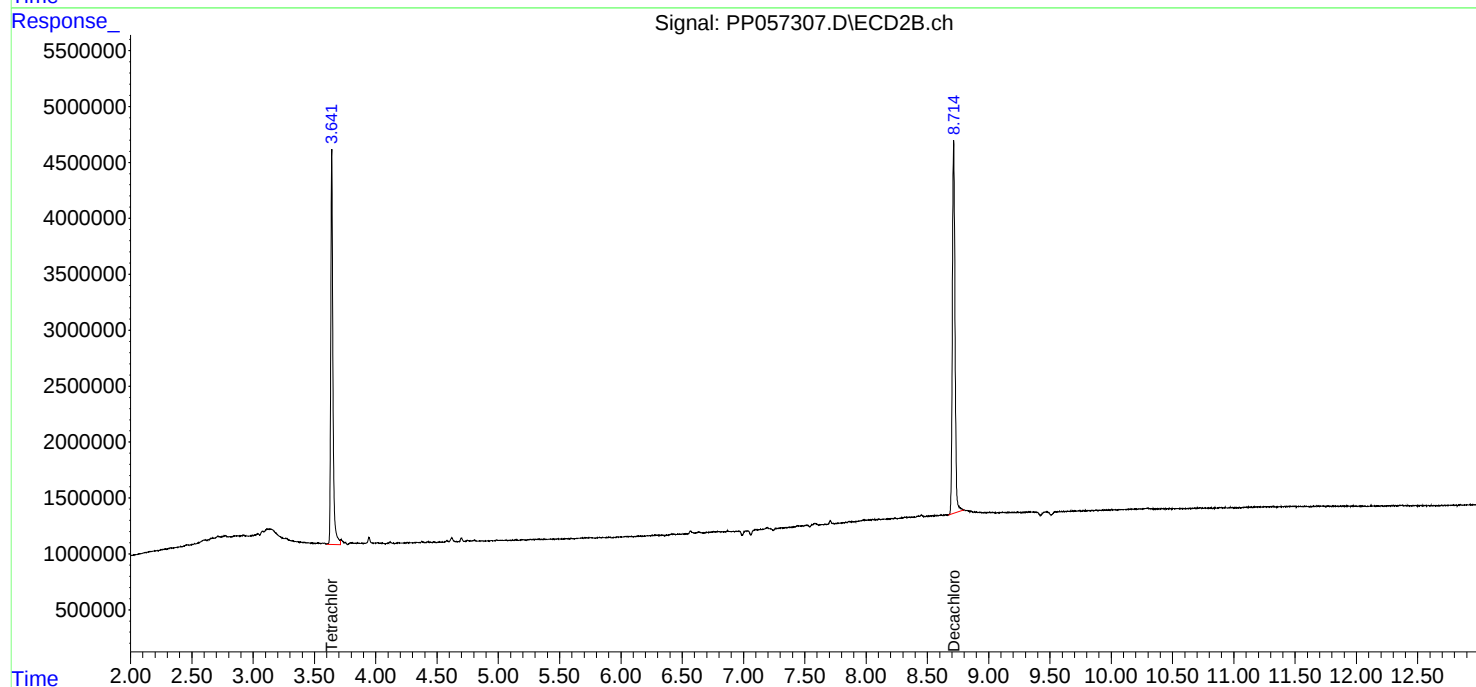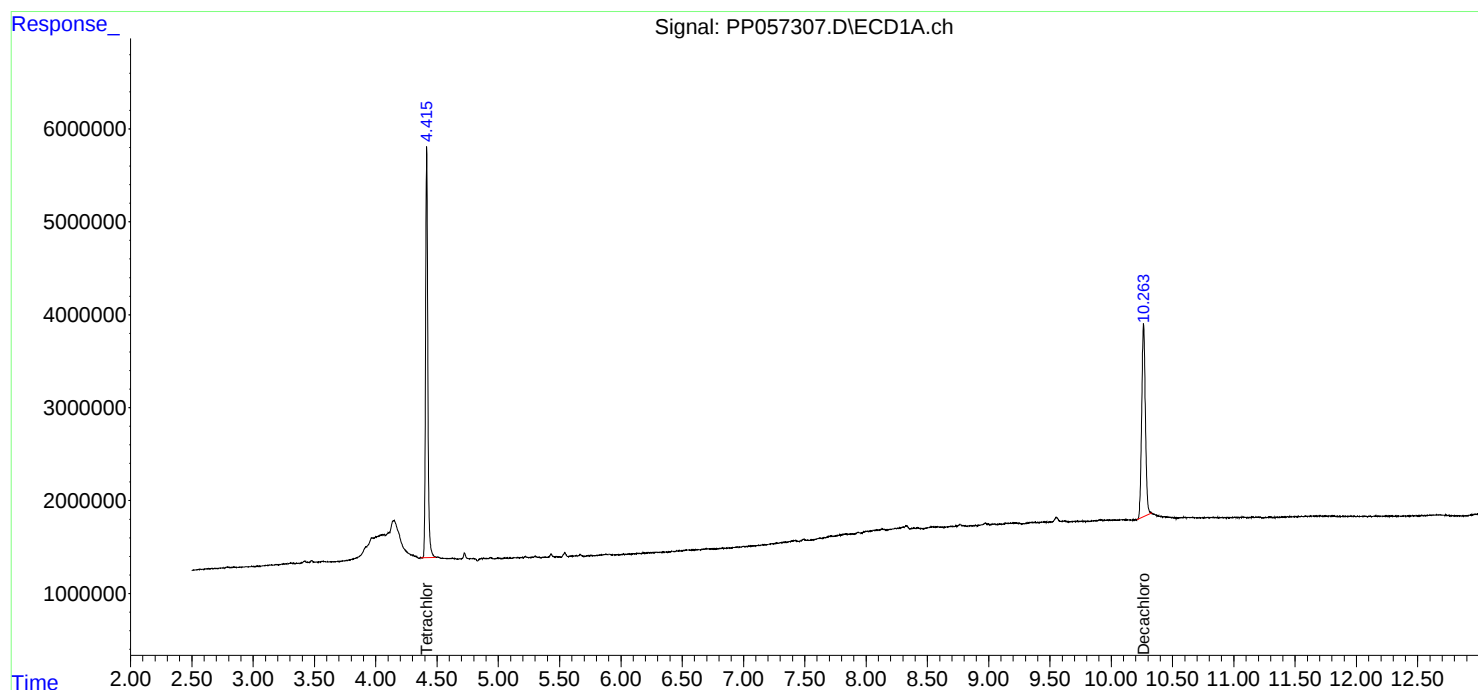


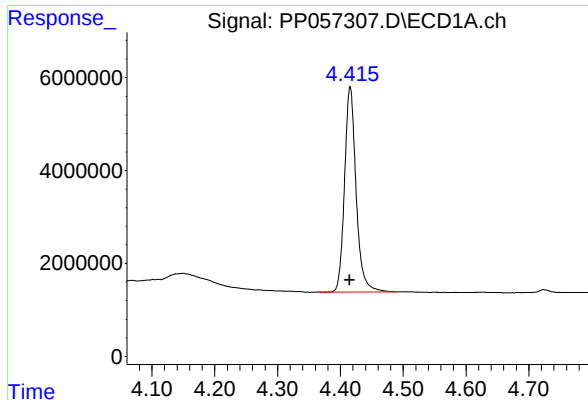

#1 Tetrachloro-m-xylene


R.T.: 4.416 min
Delta R.T.: 0.000 min
Response: 56368788
Conc: 23.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

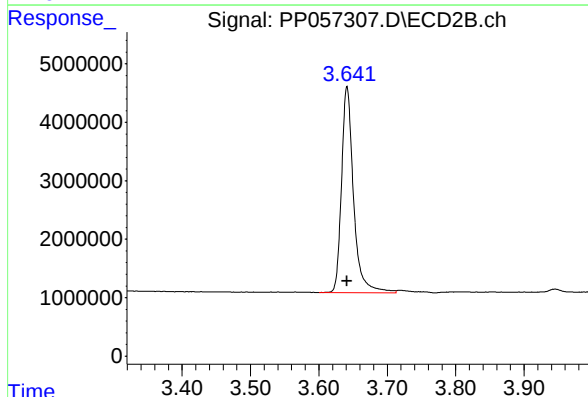


#1 Tetrachloro-m-xylene

R.T.: 3.641 min
Delta R.T.: 0.000 min
Response: 43182586
Conc: 24.36 ng/ml

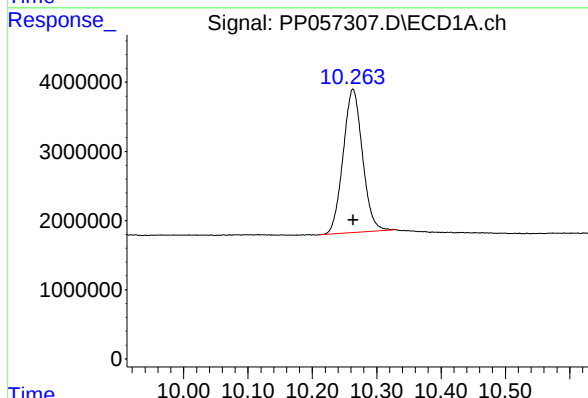

#2 Decachlorobiphenyl

R.T.: 10.263 min
Delta R.T.: 0.000 min
Response: 43227184
Conc: 26.20 ng/ml

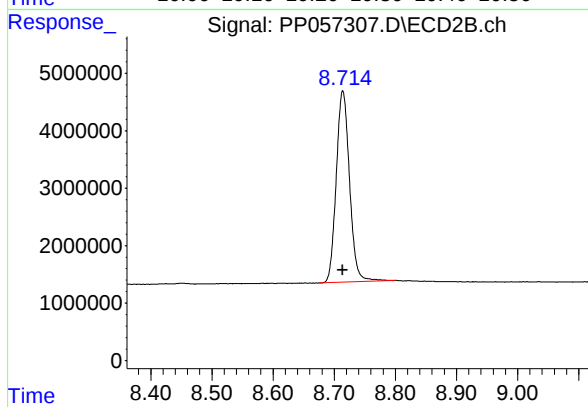

#2 Decachlorobiphenyl

R.T.: 8.714 min
Delta R.T.: 0.000 min
Response: 50342105
Conc: 25.65 ng/ml