

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050123\
 Data File : PP057335.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2023 18:18
 Operator : YP\AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1268ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/02/2023
 Supervised By :Ankita Jodhani 05/02/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 18:32:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 01 18:23:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.415	3.641	10575256	8086682	4.481	4.592
2) SA Decachlor...	10.260	8.713	13161886	17096325	4.888	5.281
Target Compounds						
41) L9 AR-1268-1	8.706	7.588	10006258	14300264	46.885	50.358m
42) L9 AR-1268-2	8.802	7.653	7692621	12358960	47.217	48.772
43) L9 AR-1268-3	9.038	7.862	8547251	11458282	45.450	49.562
44) L9 AR-1268-4	9.476	8.152	2397643	3761894	46.196	46.419
45) L9 AR-1268-5	9.907	8.451	23033680	29119858	45.180	47.646

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050123\
Data File : PP057335.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2023 18:18
Operator : YP\AJ
Sample : AR1268ICC050
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/02/2023
Supervised By :Ankita Jodhani 05/02/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 18:32:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050123.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 01 18:23:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

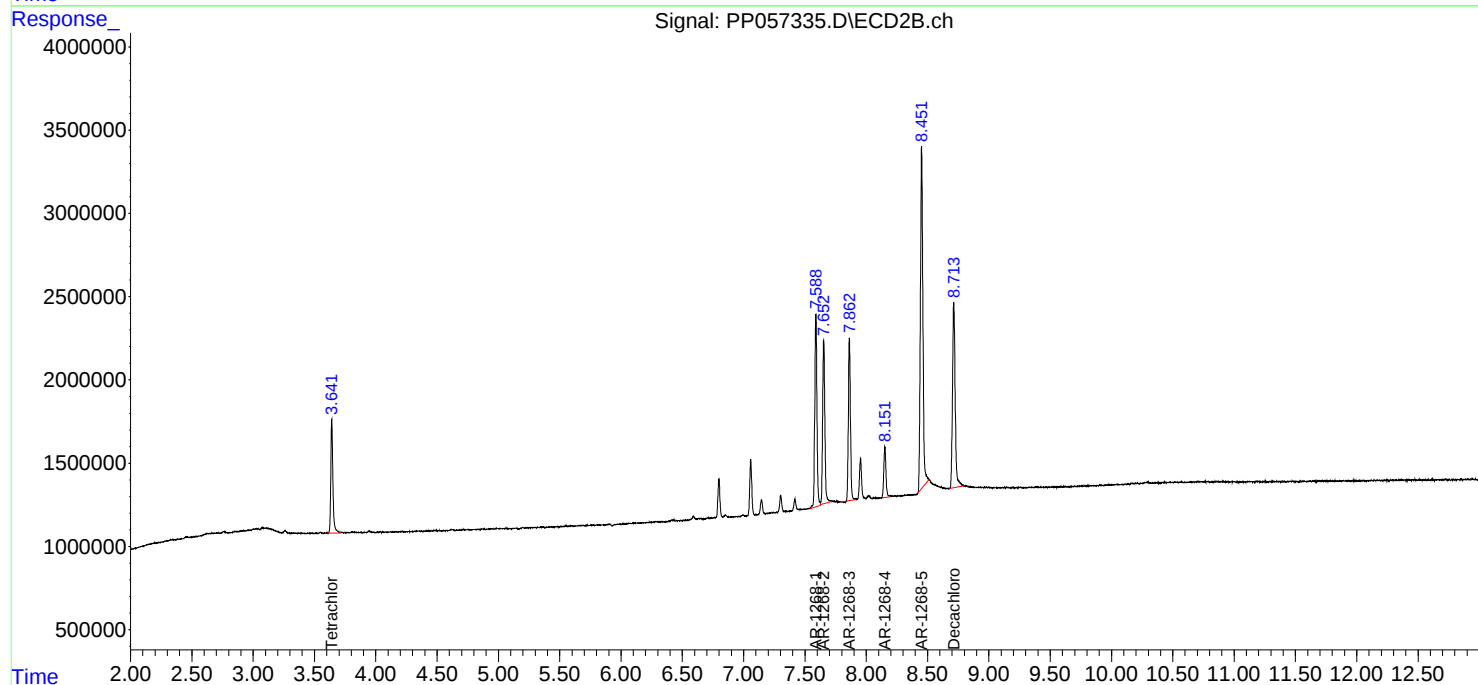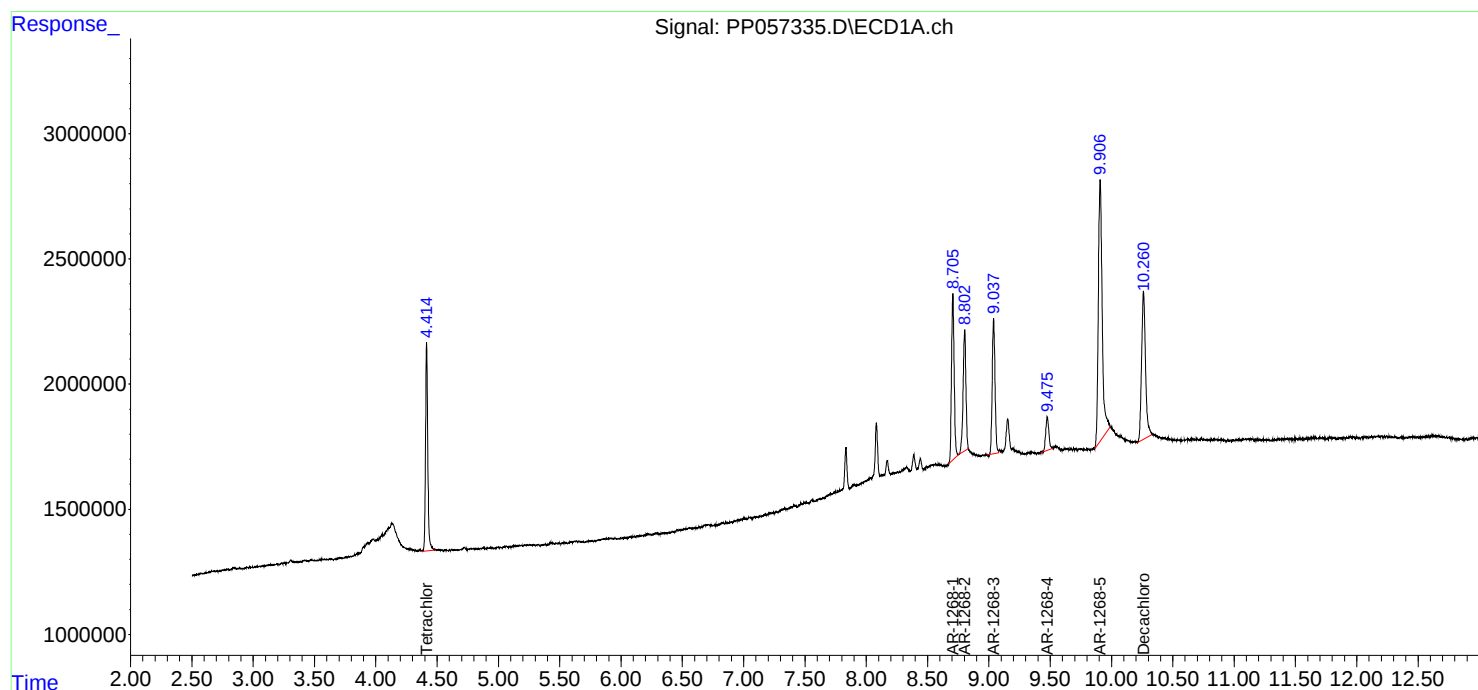

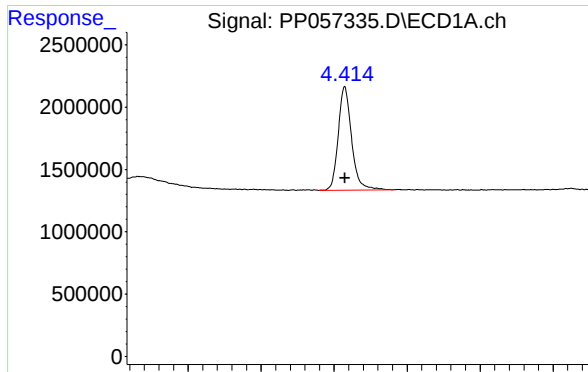


#1 Tetrachloro-m-xylene

R.T.: 4.415 min
Delta R.T.: 0.000 min
Response: 10575256
Conc: 4.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/02/2023
Supervised By :Ankita Jodhani 05/02/2023

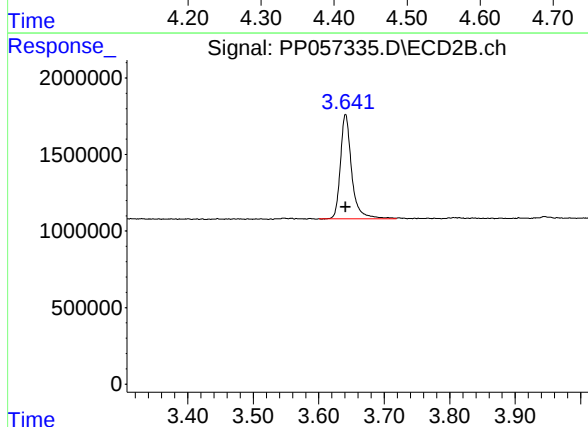


#1 Tetrachloro-m-xylene

R.T.: 3.641 min
Delta R.T.: 0.000 min
Response: 8086682
Conc: 4.59 ng/ml

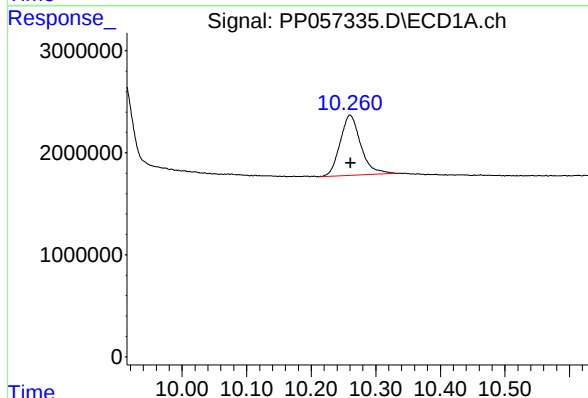


#2 Decachlorobiphenyl

R.T.: 10.260 min
Delta R.T.: -0.001 min
Response: 13161886
Conc: 4.89 ng/ml

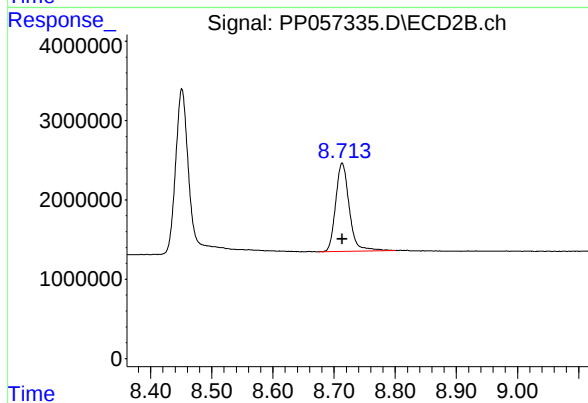

#2 Decachlorobiphenyl

R.T.: 8.713 min
Delta R.T.: 0.000 min
Response: 17096325
Conc: 5.28 ng/ml

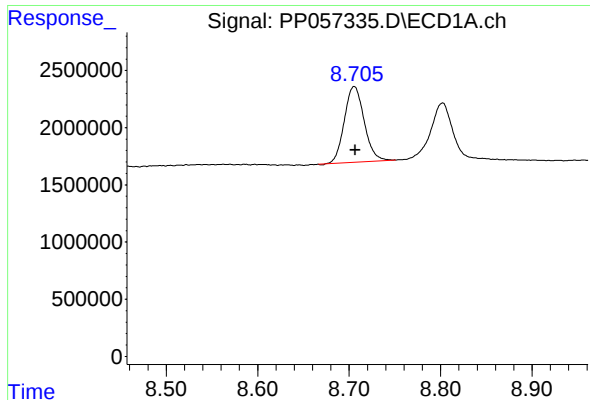


#41 AR-1268-1

R.T.: 8.706 min
Delta R.T.: 0.000 min
Response: 10006258
Conc: 46.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/02/2023
Supervised By :Ankita Jodhani 05/02/2023

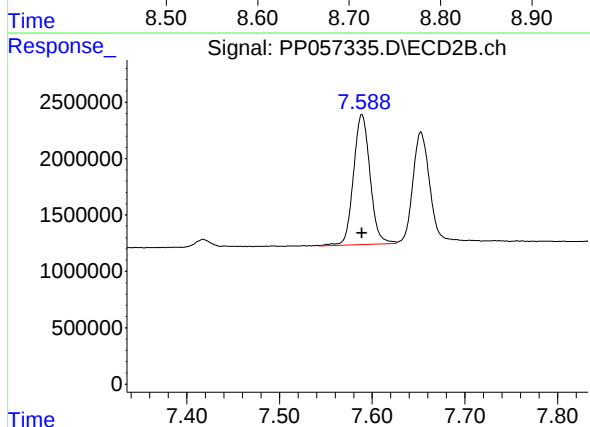


#41 AR-1268-1

R.T.: 7.588 min
Delta R.T.: 0.000 min
Response: 14300264
Conc: 50.36 ng/ml

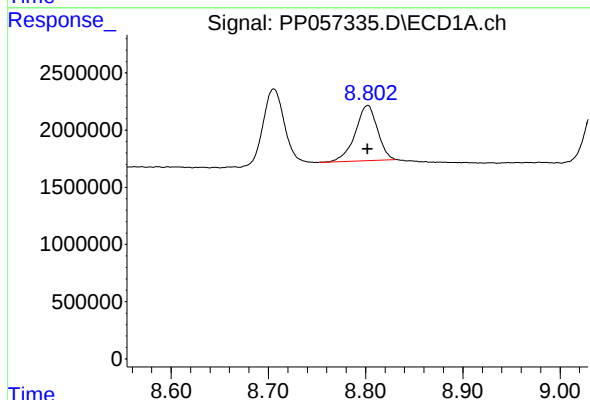


#42 AR-1268-2

R.T.: 8.802 min
Delta R.T.: 0.000 min
Response: 7692621
Conc: 47.22 ng/ml

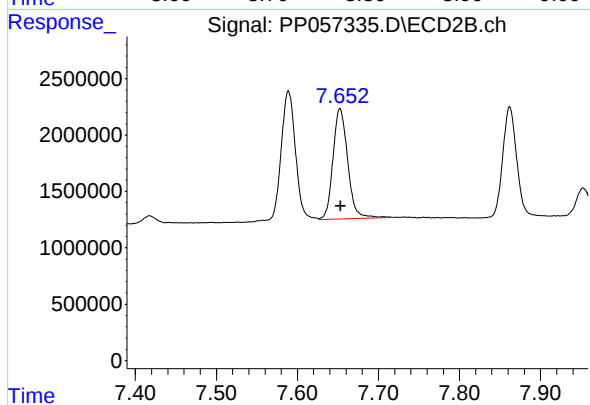

#42 AR-1268-2

R.T.: 7.653 min
Delta R.T.: 0.000 min
Response: 12358960
Conc: 48.77 ng/ml

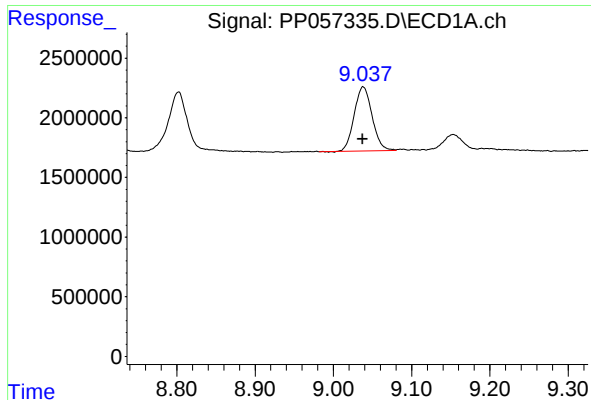


#43 AR-1268-3

R.T.: 9.038 min
Delta R.T.: 0.000 min
Response: 8547251
Conc: 45.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/02/2023
Supervised By :Ankita Jodhani 05/02/2023

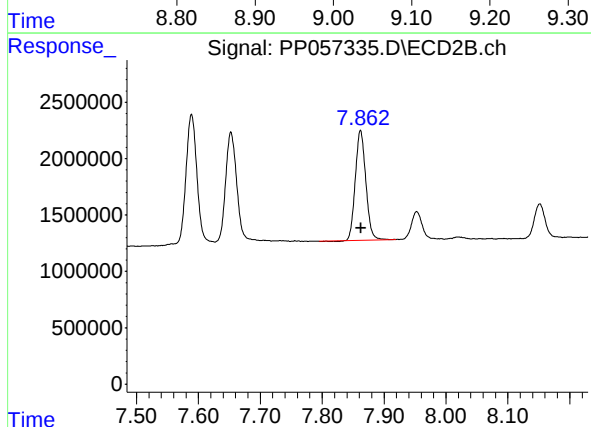


#43 AR-1268-3

R.T.: 7.862 min
Delta R.T.: 0.000 min
Response: 11458282
Conc: 49.56 ng/ml

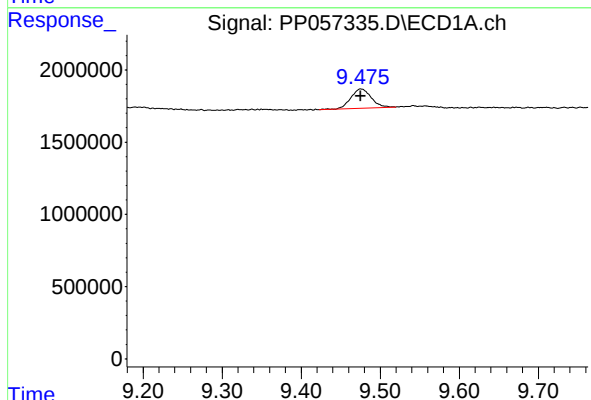


#44 AR-1268-4

R.T.: 9.476 min
Delta R.T.: 0.000 min
Response: 2397643
Conc: 46.20 ng/ml

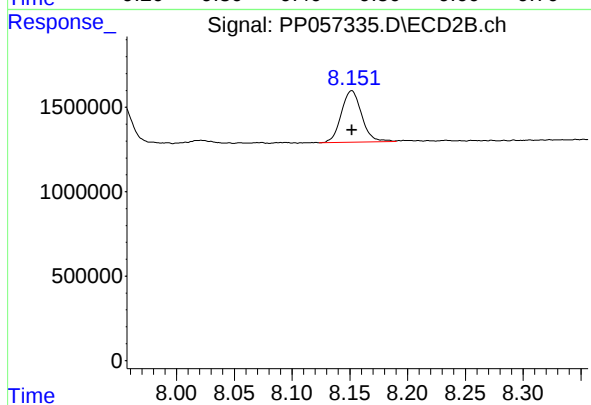

#44 AR-1268-4

R.T.: 8.152 min
Delta R.T.: 0.000 min
Response: 3761894
Conc: 46.42 ng/ml

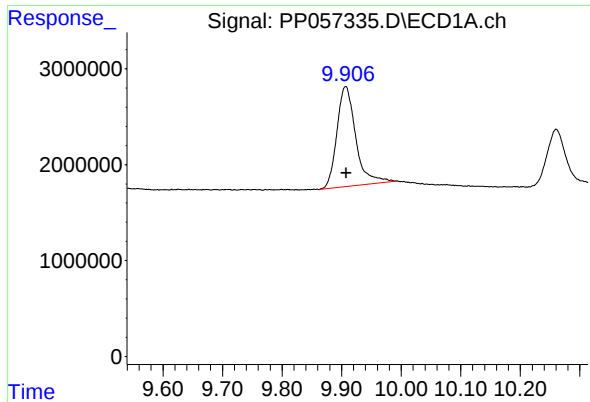


#45 AR-1268-5

R.T.: 9.907 min
Delta R.T.: -0.001 min
Response: 23033680
Conc: 45.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/02/2023
Supervised By :Ankita Jodhani 05/02/2023

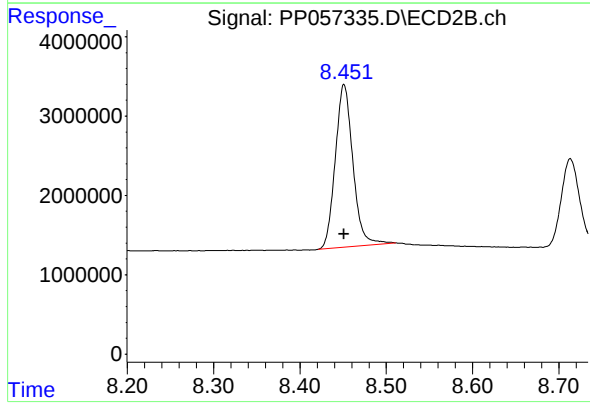

#45 AR-1268-5

R.T.: 8.451 min
Delta R.T.: 0.000 min
Response: 29119858
Conc: 47.65 ng/ml