

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050123\
 Data File : PP057351.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2023 22:44
 Operator : YP\AJ
 Sample : 02543-01
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 011

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/02/2023
 Supervised By :Ankita Jodhani 05/02/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 02:08:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 01 18:39:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.421	3.657	35742979	29246558	15.177m	16.495m
2) SA Decachlor...	10.255	8.728	44006444	70135043	26.675	35.739m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050123\
Data File : PP057351.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2023 22:44
Operator : YP\AJ
Sample : 02543-01
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
011


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/02/2023
Supervised By :Ankita Jodhani 05/02/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 02:08:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050123.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 01 18:39:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

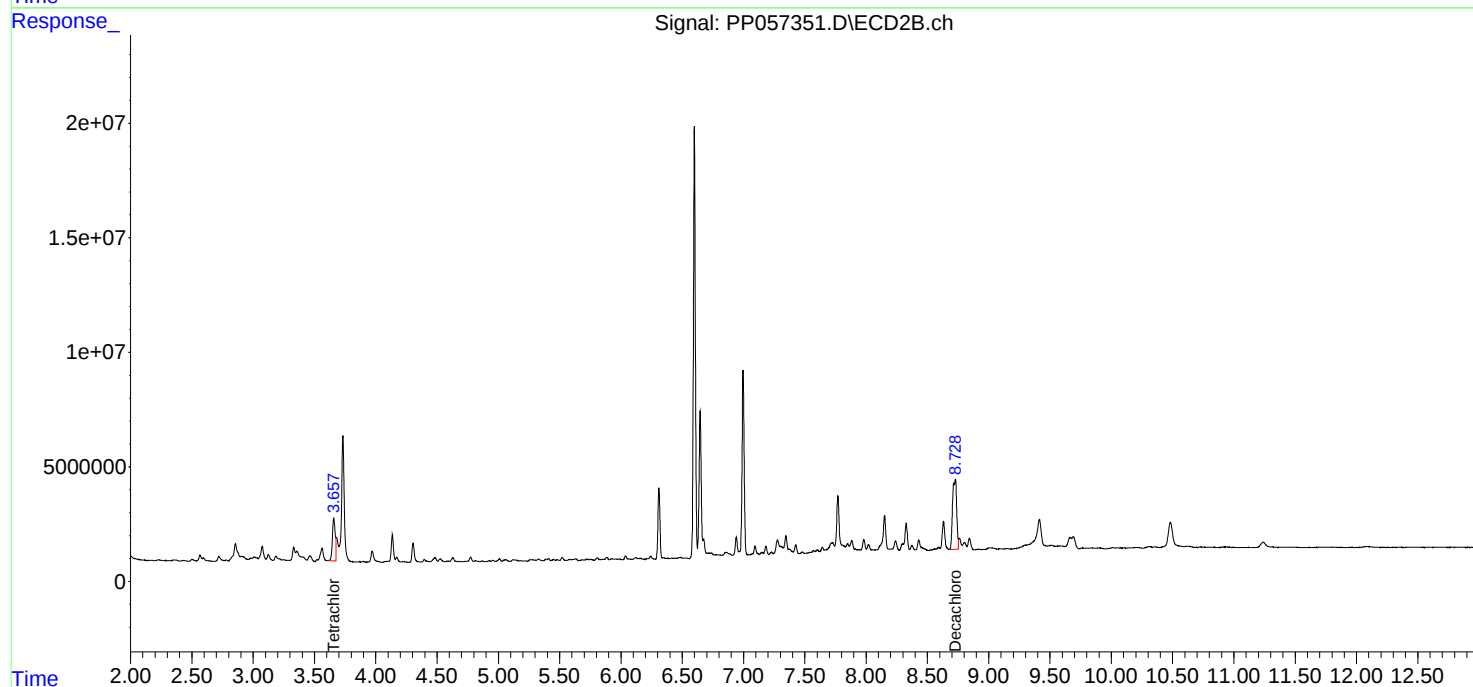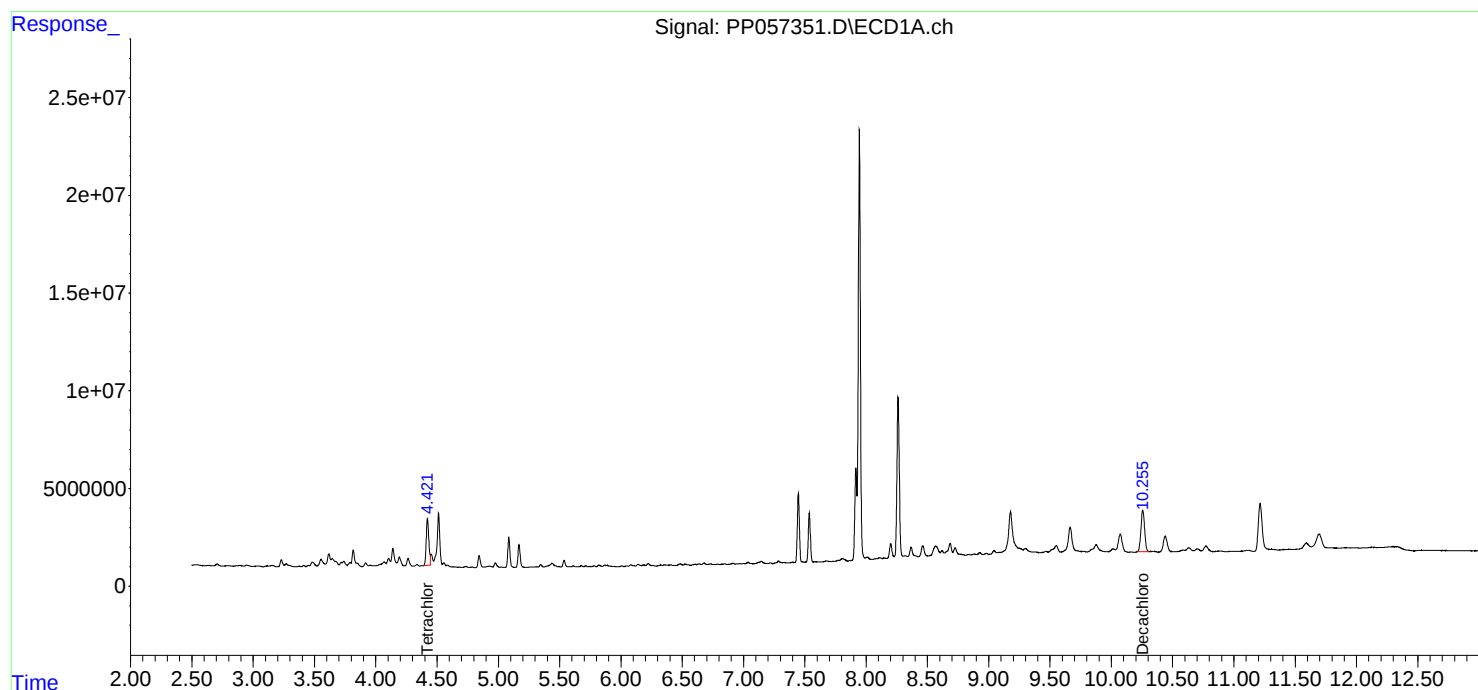

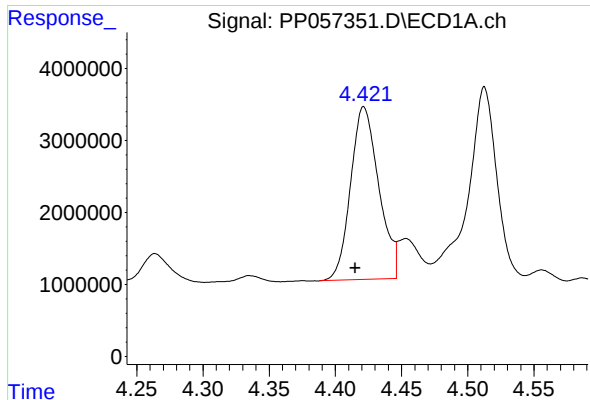


#1 Tetrachloro-m-xylene

R.T.: 4.421 min
Delta R.T.: 0.006 min
Response: 35742979
Conc: 15.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
011


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/02/2023
Supervised By :Ankita Jodhani 05/02/2023

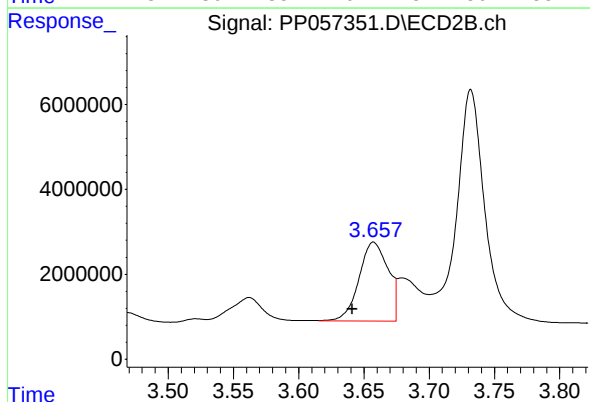


#1 Tetrachloro-m-xylene

R.T.: 3.657 min
Delta R.T.: 0.016 min
Response: 29246558
Conc: 16.50 ng/ml m

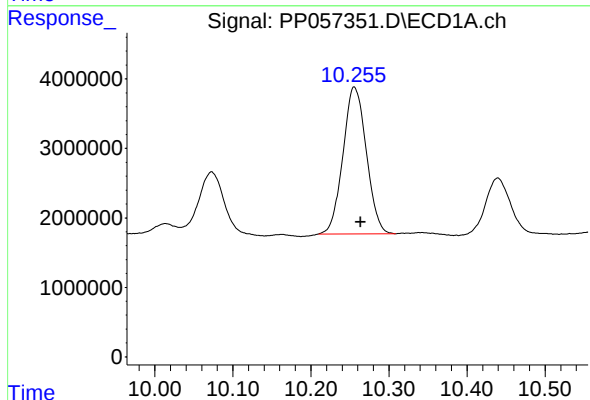

#2 Decachlorobiphenyl

R.T.: 10.255 min
Delta R.T.: -0.008 min
Response: 44006444
Conc: 26.67 ng/ml

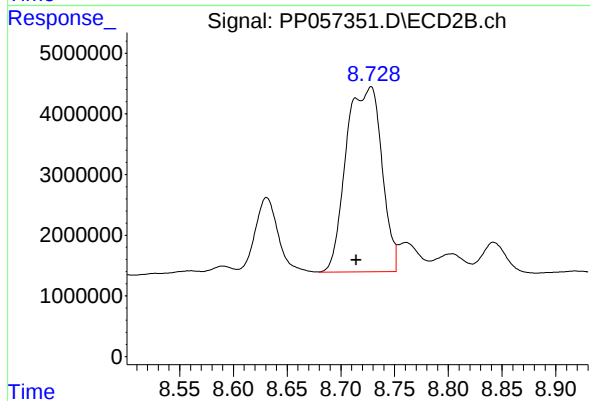

#2 Decachlorobiphenyl

R.T.: 8.728 min
Delta R.T.: 0.014 min
Response: 70135043
Conc: 35.74 ng/ml m