

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050222\
 Data File : PP046915.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 May 2022 22:25
 Operator : YP\AJ
 Sample : N2633-01 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 GROUP-1-A-4-29-2022

Manual Integrations
 APPROVED

Reviewed By :Yogesh
 Patel

05/03/2022
 Supervised By :mohammad
 ahmed

05/03/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 04:26:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 22 19:00:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.859	3.125	3763059	6690188	1.559	2.039 #
2) SA Decachlor...	9.931	8.439	3307984	4453004	2.248m	1.867

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050222\
Data File : PP046915.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 May 2022 22:25
Operator : YP\AJ
Sample : N2633-01 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
GROUP-1-A-4-29-2022

Manual Integrations
APPROVED



Reviewed By :Yogesh
Patel


05/03/2022
Supervised By :mohammad
ahmed

05/03/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 04:26:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 22 19:00:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

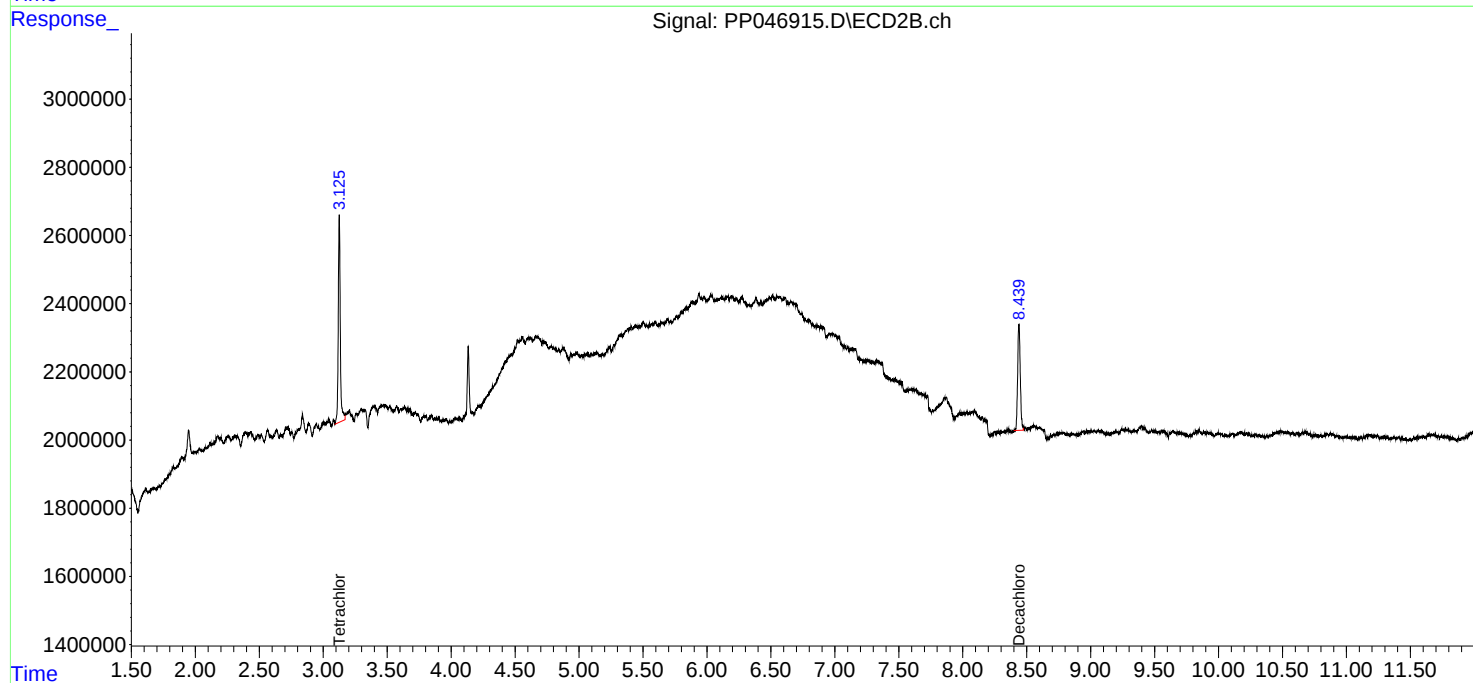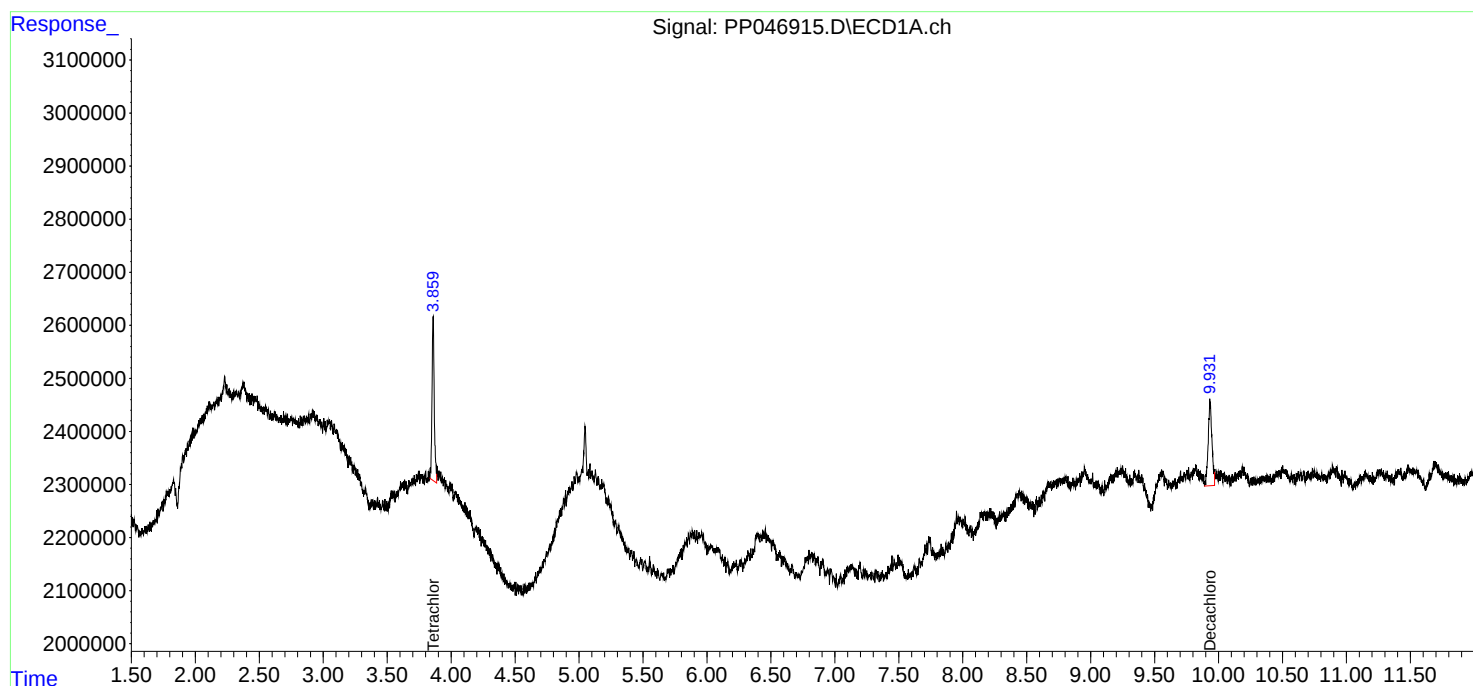

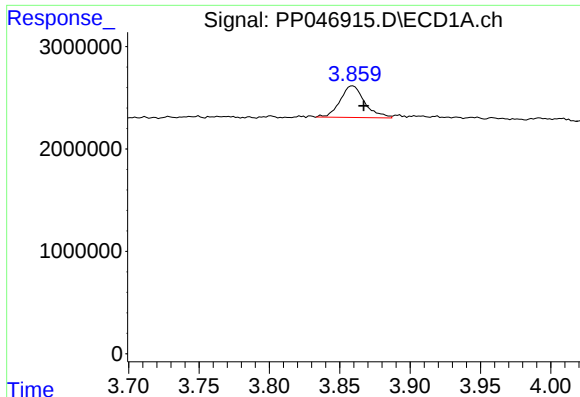

#1 Tetrachloro-m-xylene

R.T.: 3.859 min
Delta R.T.: -0.008 min
Response: 3763059
Conc: 1.56 ng/ml


Instrument :
ECD_P
ClientSampleId :
GROUP-1-A-4-29-2022

Manual Integrations
APPROVED

Reviewed By :Yogesh
Patel


05/03/2022
Supervised By :mohammad
ahmed

05/03/2022

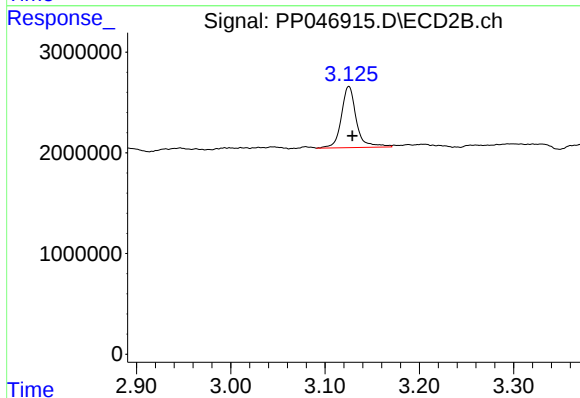


#1 Tetrachloro-m-xylene

R.T.: 3.125 min
Delta R.T.: -0.004 min
Response: 6690188
Conc: 2.04 ng/ml

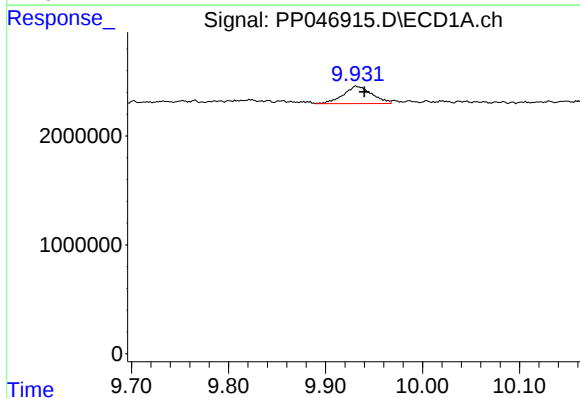

#2 Decachlorobiphenyl

R.T.: 9.931 min
Delta R.T.: -0.009 min
Response: 3307984
Conc: 2.25 ng/ml m

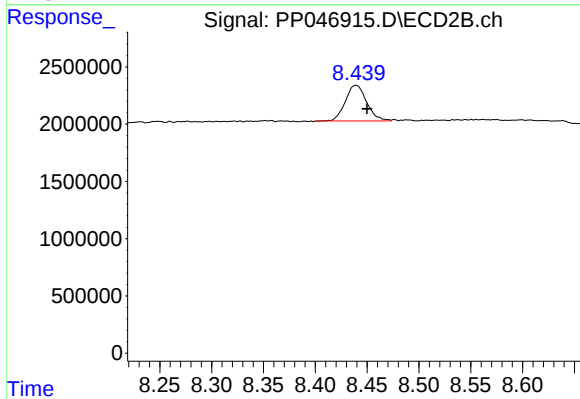

#2 Decachlorobiphenyl

R.T.: 8.439 min
Delta R.T.: -0.011 min
Response: 4453004
Conc: 1.87 ng/ml