

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050222\
 Data File : PP046917.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 May 2022 22:55
 Operator : YP\AJ
 Sample : N2633-03 10X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 GROUP-1-C-4-29-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 04:26:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 22 19:00:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.859	3.125	3459871	5880428	1.433	1.793 #
2) SA Decachlor...	9.932	8.440	3216414	4246831	2.186	1.780

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050222\
Data File : PP046917.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 May 2022 22:55
Operator : YP\AJ
Sample : N2633-03 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
GROUP-1-C-4-29-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 04:26:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 22 19:00:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

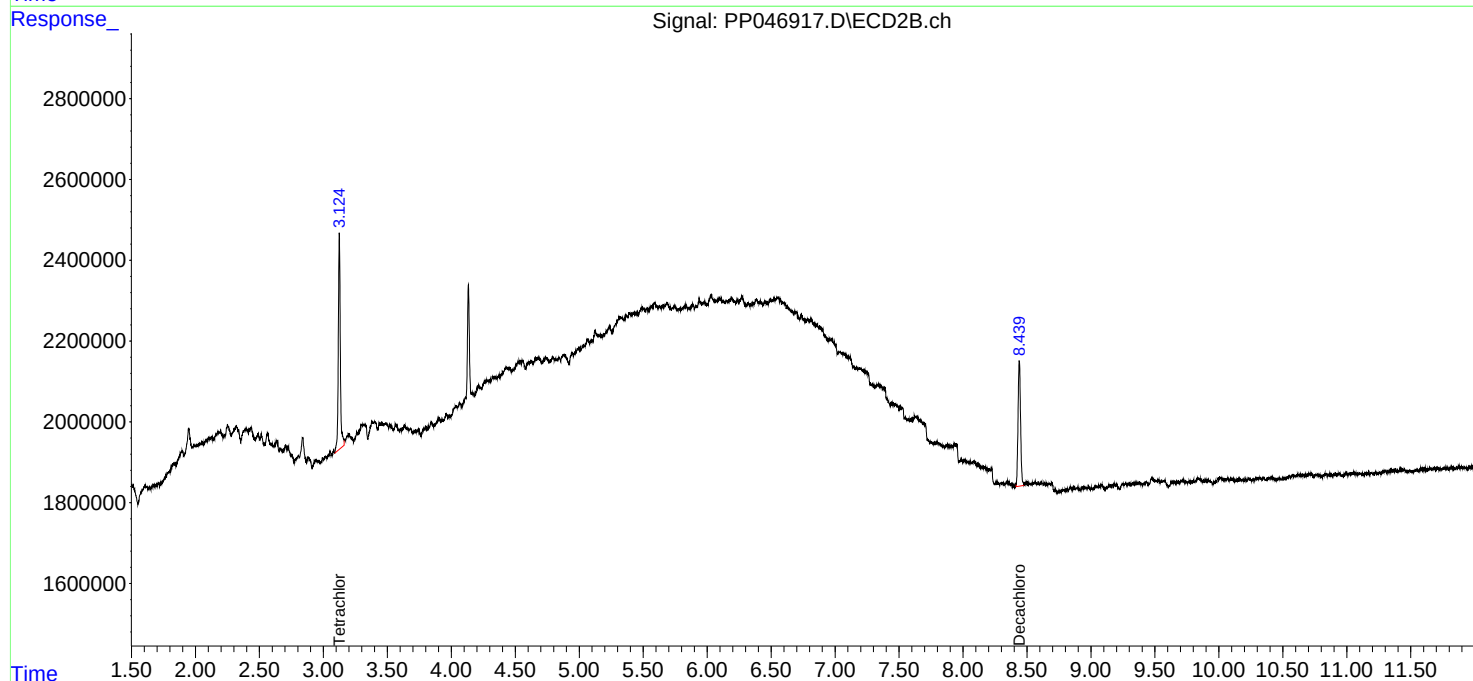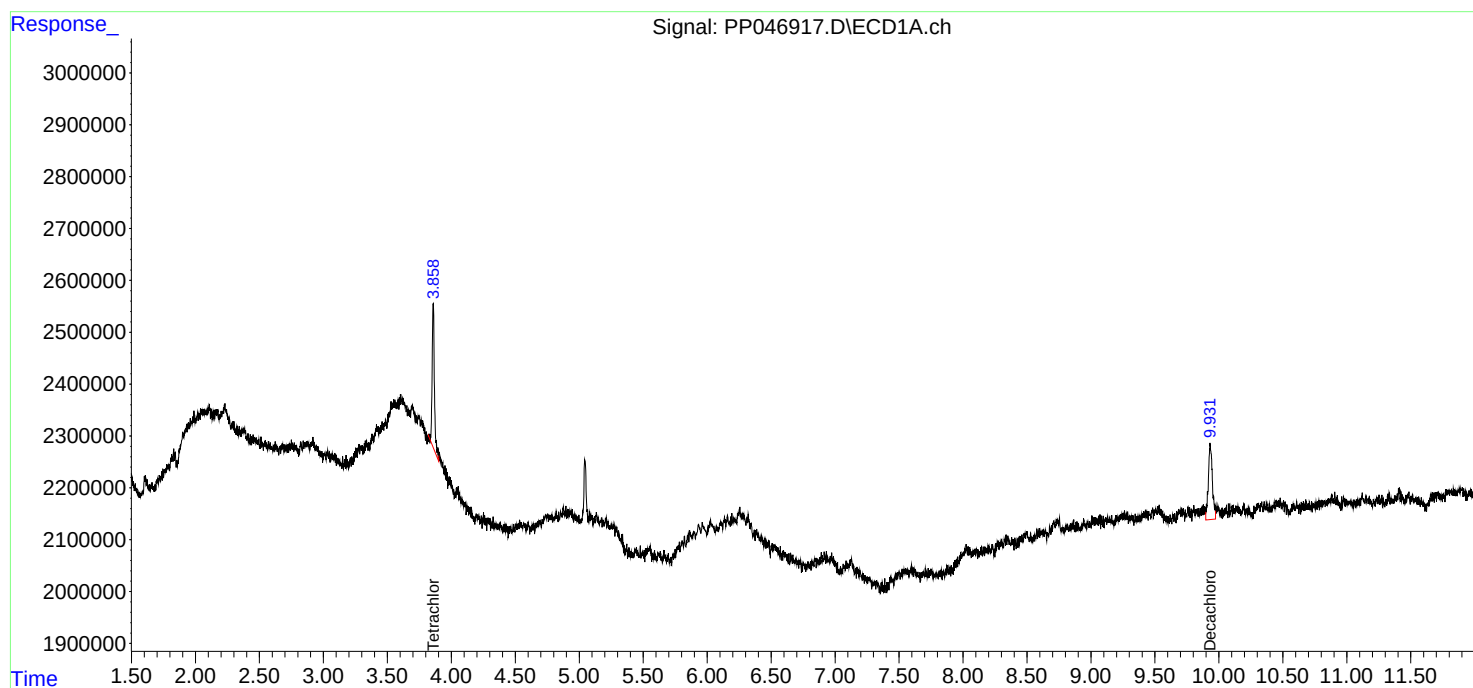


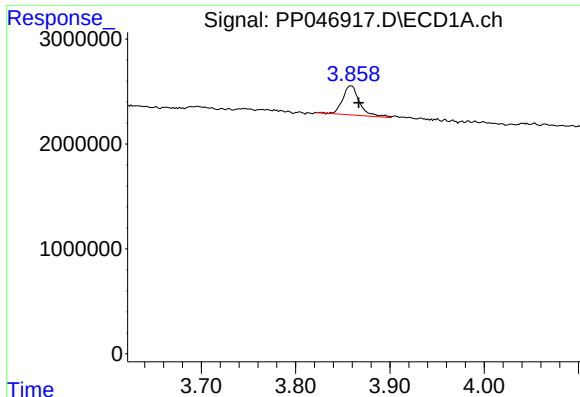

#1 Tetrachloro-m-xylene


R.T.: 3.859 min
Delta R.T.: -0.008 min
Response: 3459871
Conc: 1.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
GROUP-1-C-4-29-2022

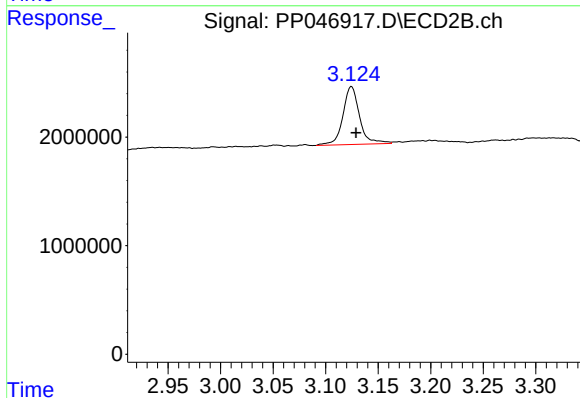


#1 Tetrachloro-m-xylene

R.T.: 3.125 min
Delta R.T.: -0.005 min
Response: 5880428
Conc: 1.79 ng/ml

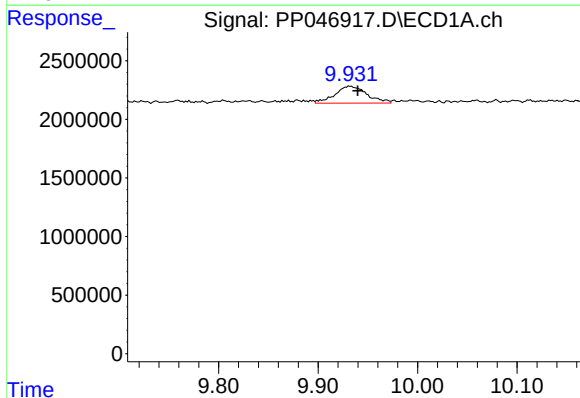

#2 Decachlorobiphenyl

R.T.: 9.932 min
Delta R.T.: -0.008 min
Response: 3216414
Conc: 2.19 ng/ml

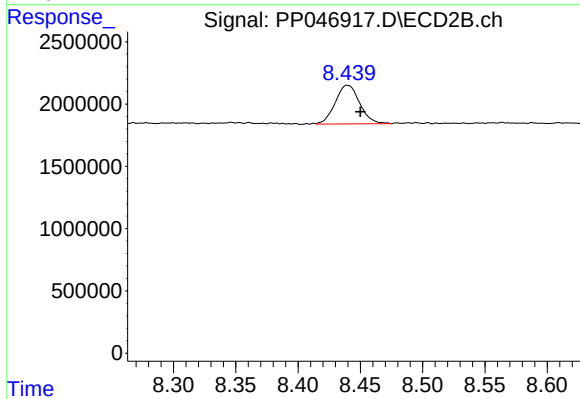

#2 Decachlorobiphenyl

R.T.: 8.440 min
Delta R.T.: -0.010 min
Response: 4246831
Conc: 1.78 ng/ml