

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050222\
 Data File : PP046921.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 May 2022 23:56
 Operator : YP\AJ
 Sample : N2633-07 10X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KMH325Y-END-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/03/2022
 Supervised By :mohammad ahmed 05/03/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 04:28:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 22 19:00:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.858	3.125	4017199	3809898	1.664	1.161 #
2) SA Decachlor...	9.932	8.436	2840126	3830411	1.930	1.606m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050222\
Data File : PP046921.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 May 2022 23:56
Operator : YP\AJ
Sample : N2633-07 10X
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KMH325Y-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/03/2022
Supervised By :mohammad ahmed 05/03/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 04:28:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042222.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 22 19:00:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

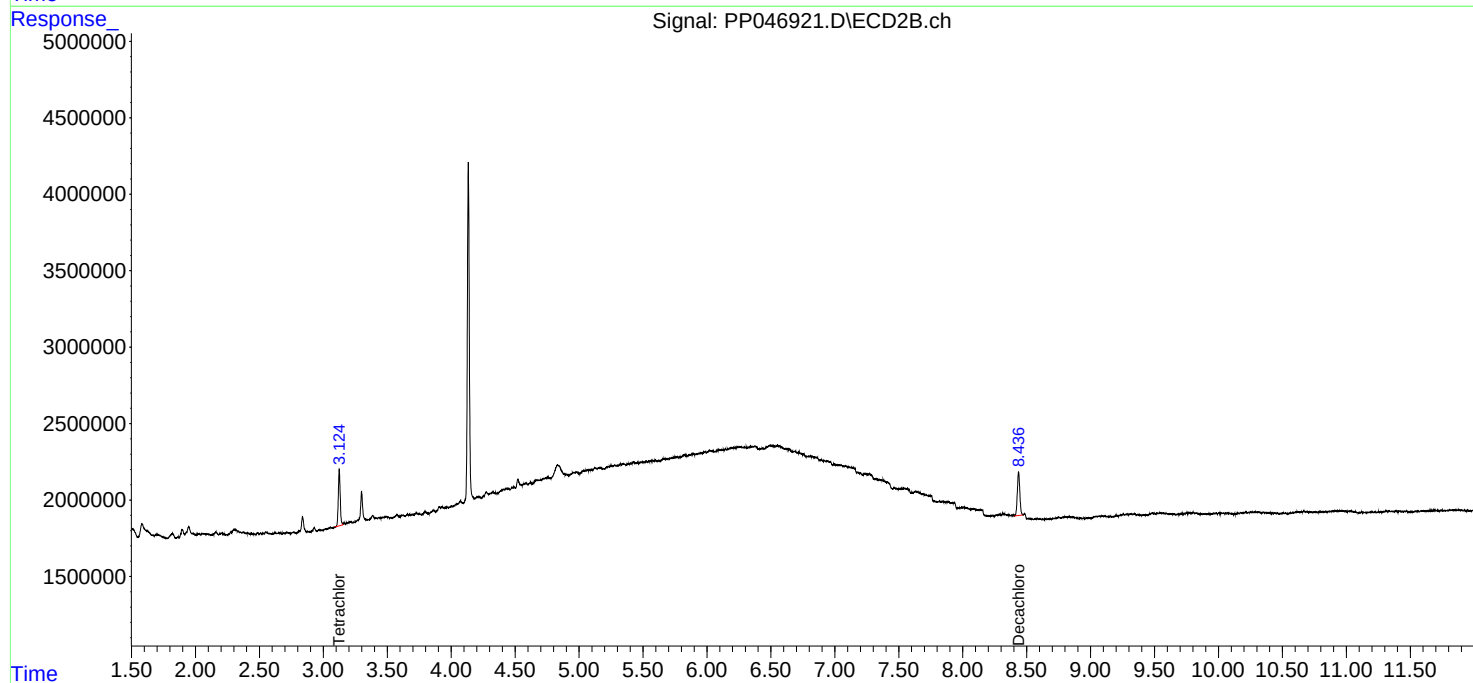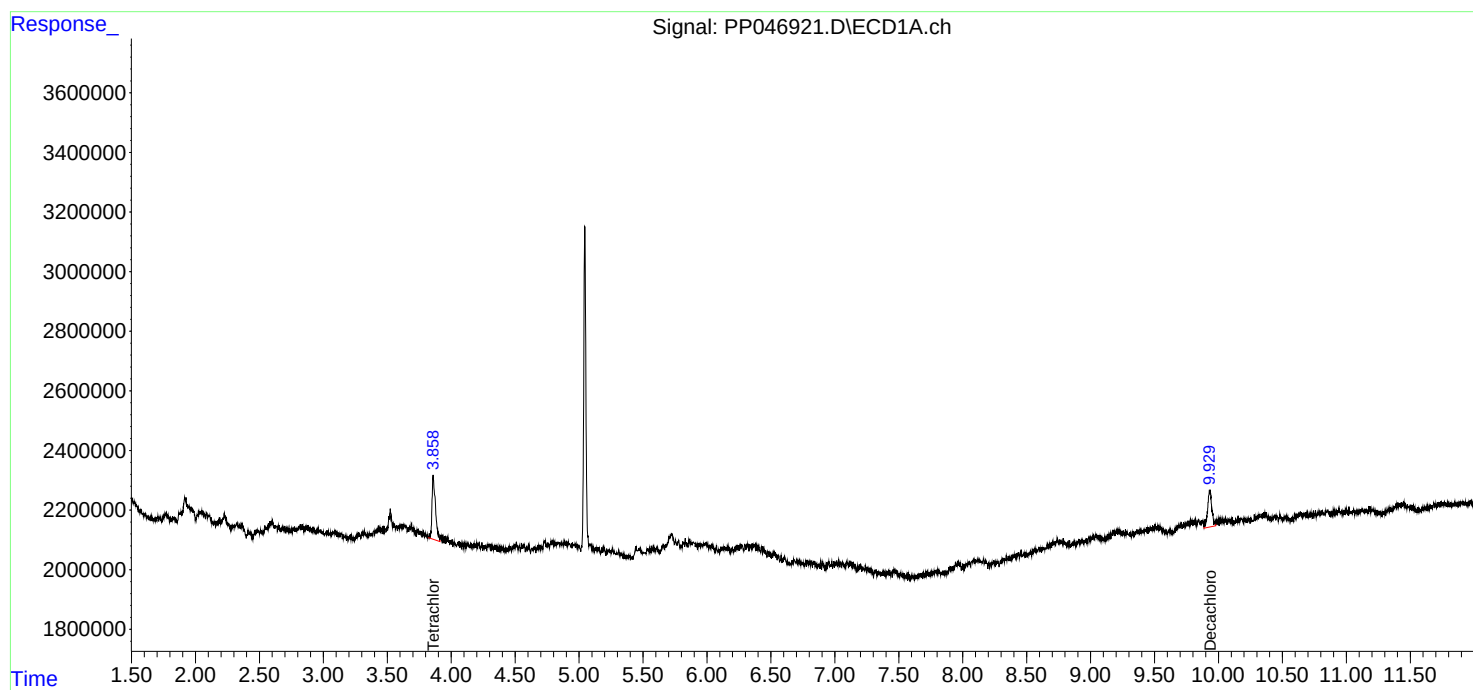

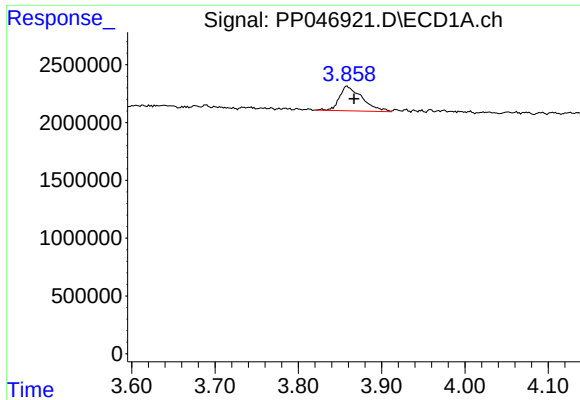


#1 Tetrachloro-m-xylene

R.T.: 3.858 min
Delta R.T.: -0.009 min
Response: 4017199
Conc: 1.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
KMH325Y-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/03/2022
Supervised By :mohammad ahmed 05/03/2022

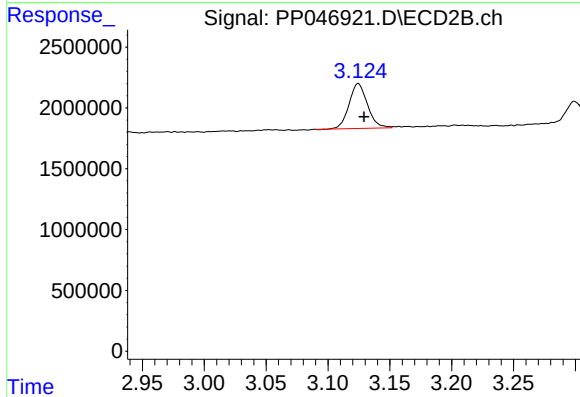


#1 Tetrachloro-m-xylene

R.T.: 3.125 min
Delta R.T.: -0.005 min
Response: 3809898
Conc: 1.16 ng/ml

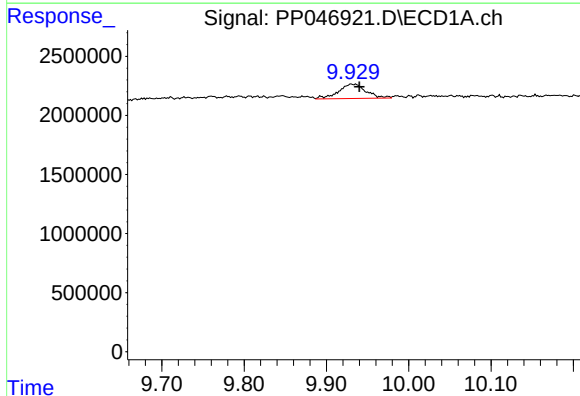

#2 Decachlorobiphenyl

R.T.: 9.932 min
Delta R.T.: -0.008 min
Response: 2840126
Conc: 1.93 ng/ml

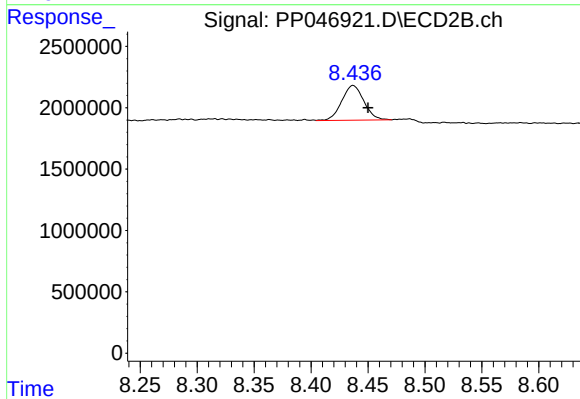

#2 Decachlorobiphenyl

R.T.: 8.436 min
Delta R.T.: -0.014 min
Response: 3830411
Conc: 1.61 ng/ml m