

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050223\
 Data File : PP057423.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 May 2023 22:32
 Operator : YP\AJ
 Sample : 02572-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RBR-251671

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/03/2023
 Supervised By :Ankita Jodhani 05/03/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 04:46:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 01 18:39:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.413	3.640	44727511	34522284	18.992m	19.471
2) SA Decachlor...	10.260	8.714	94729283	87890231	57.421m	44.786m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050223\
Data File : PP057423.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 May 2023 22:32
Operator : YP\AJ
Sample : 02572-01
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
RBR-251671


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/03/2023
Supervised By :Ankita Jodhani 05/03/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 04:46:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050123.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 01 18:39:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

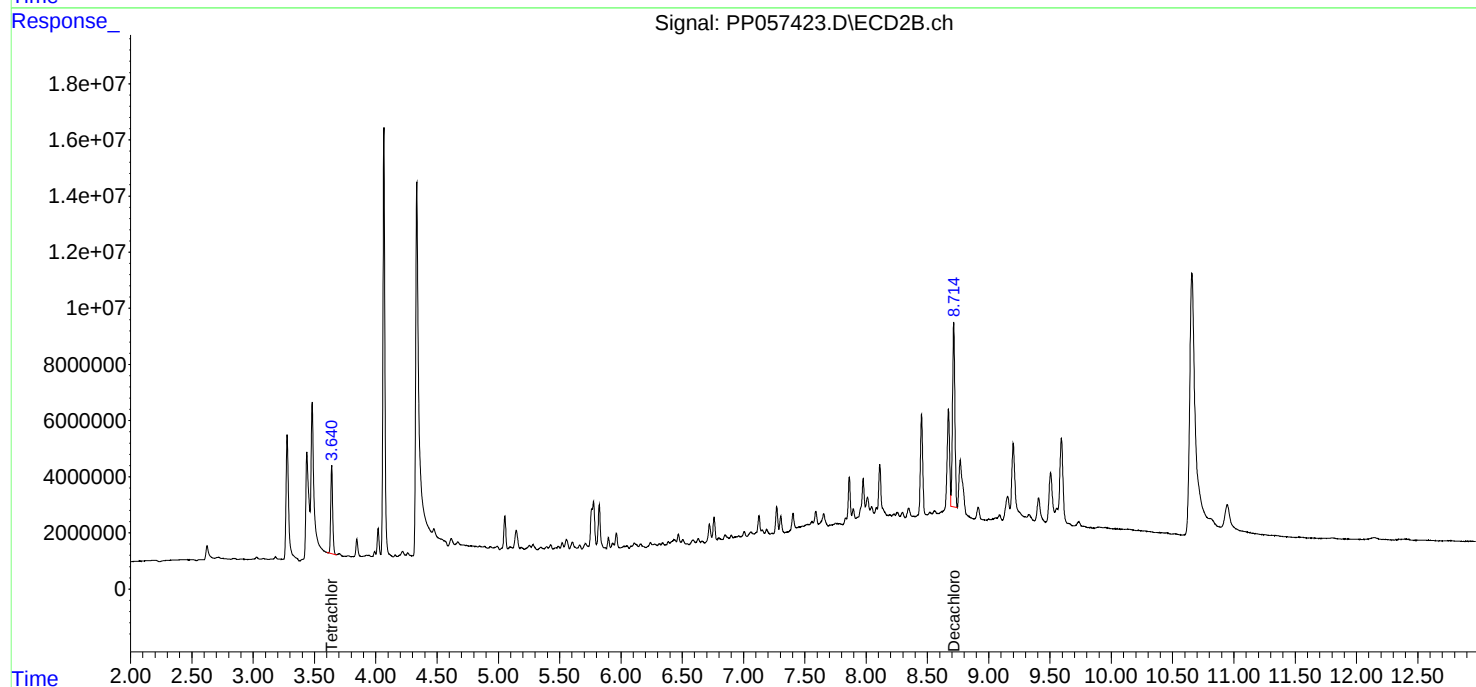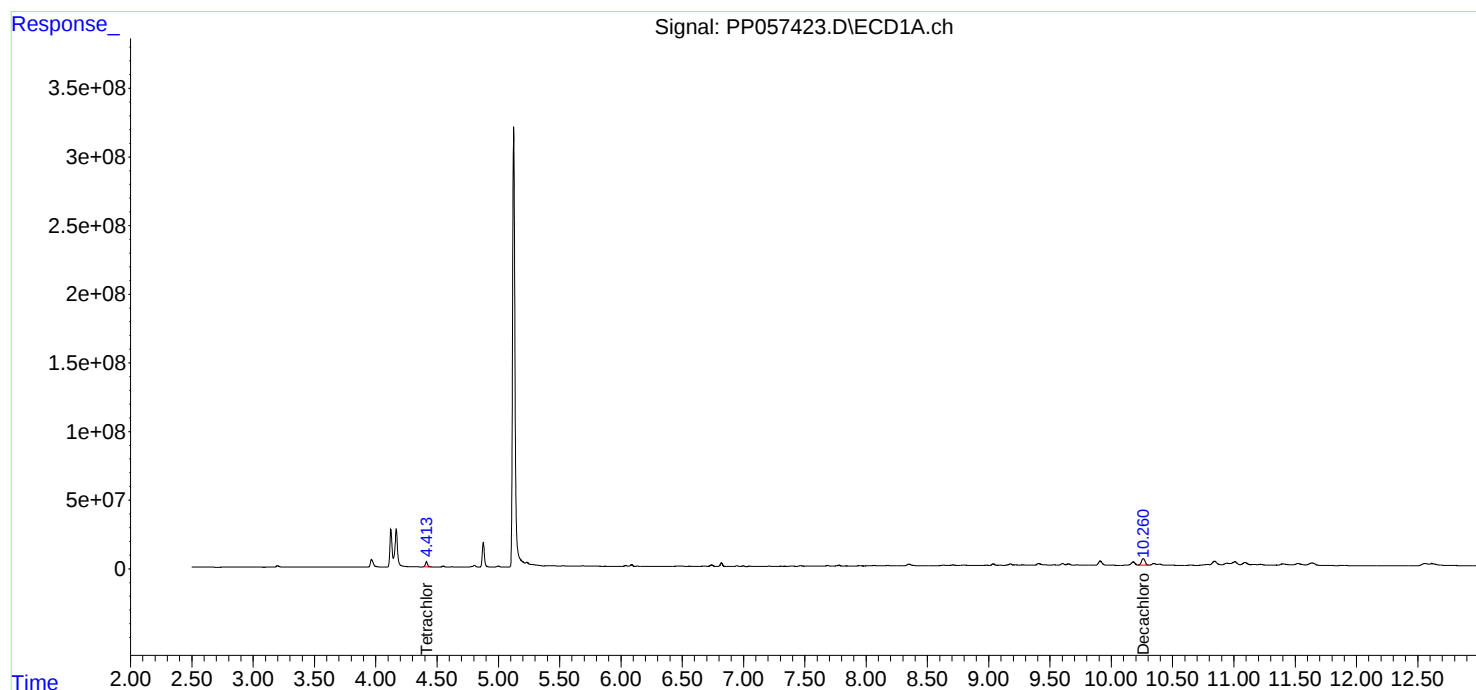

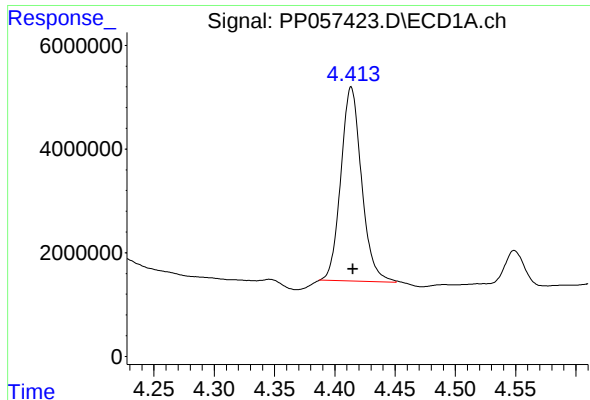


#1 Tetrachloro-m-xylene

R.T.: 4.413 min
Delta R.T.: -0.002 min
Response: 44727511
Conc: 18.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
RBR-251671


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/03/2023
Supervised By :Ankita Jodhani 05/03/2023

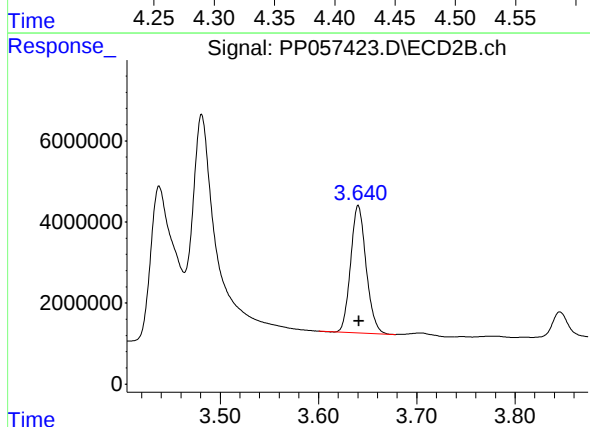


#1 Tetrachloro-m-xylene

R.T.: 3.640 min
Delta R.T.: 0.000 min
Response: 34522284
Conc: 19.47 ng/ml

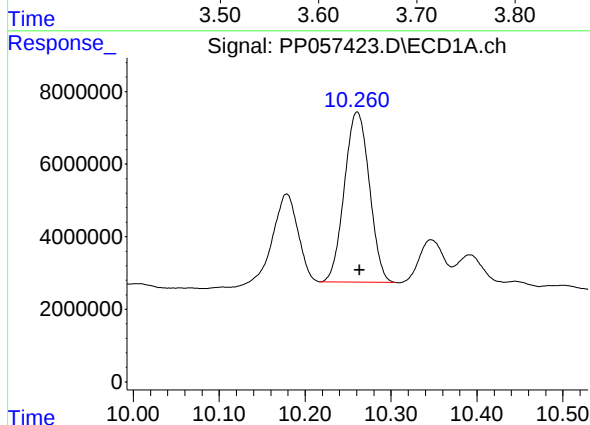

#2 Decachlorobiphenyl

R.T.: 10.260 min
Delta R.T.: -0.003 min
Response: 94729283
Conc: 57.42 ng/ml m

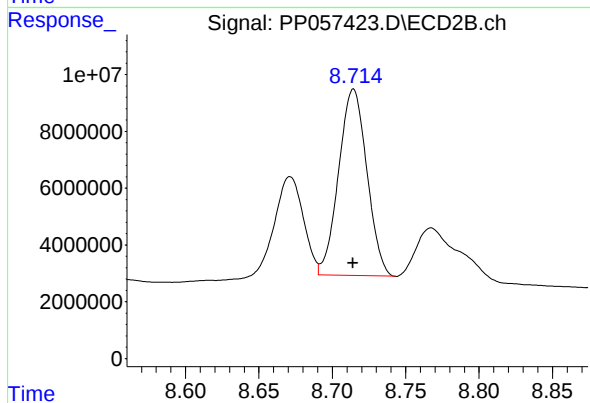

#2 Decachlorobiphenyl

R.T.: 8.714 min
Delta R.T.: 0.000 min
Response: 87890231
Conc: 44.79 ng/ml m