

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050223\
 Data File : PP057424.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 May 2023 22:49
 Operator : YP\AJ
 Sample : 02572-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RT2343

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/03/2023
 Supervised By :Ankita Jodhani 05/03/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 04:47:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 01 18:39:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.414	3.641	45548037	36444176	19.341	20.555
2) SA Decachlor...	10.261	8.714	29716997	30043750	18.013	15.309m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050223\
Data File : PP057424.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 May 2023 22:49
Operator : YP\AJ
Sample : 02572-03
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
RT2343


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/03/2023
Supervised By :Ankita Jodhani 05/03/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 04:47:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050123.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 01 18:39:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

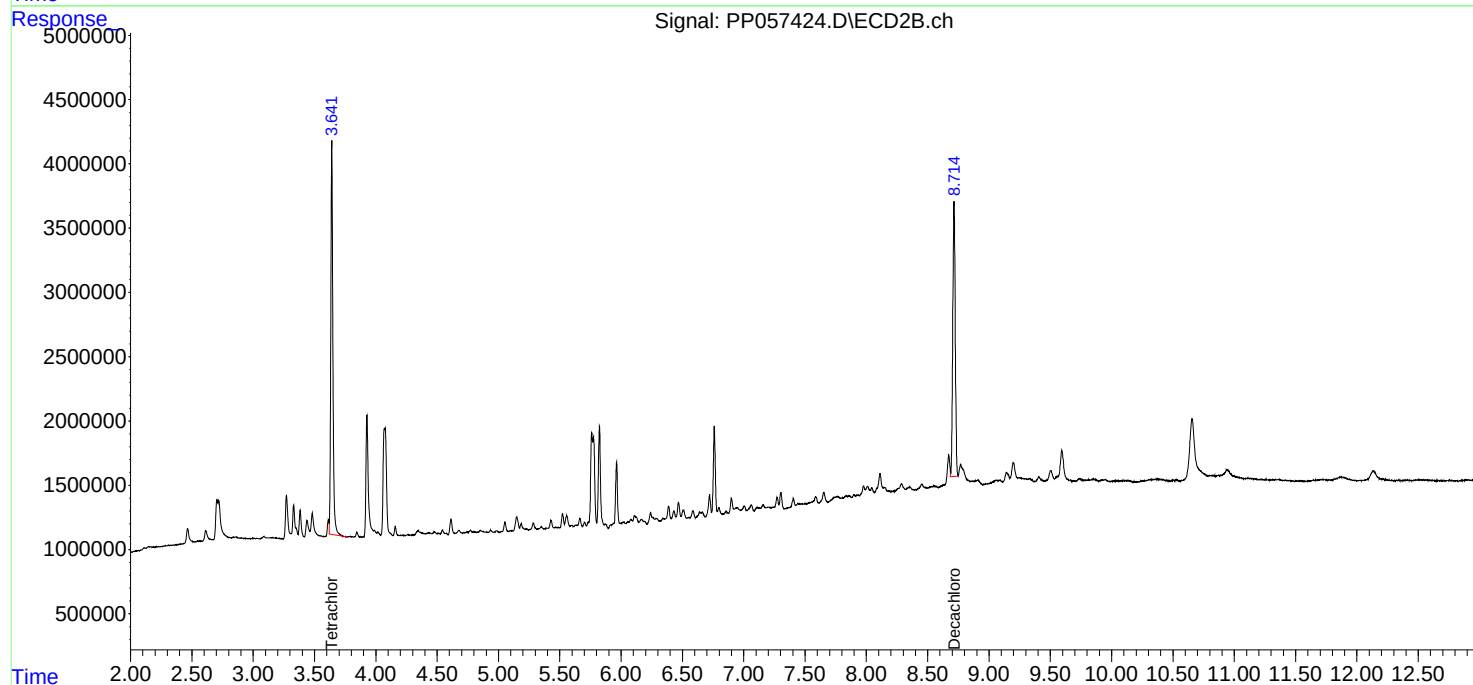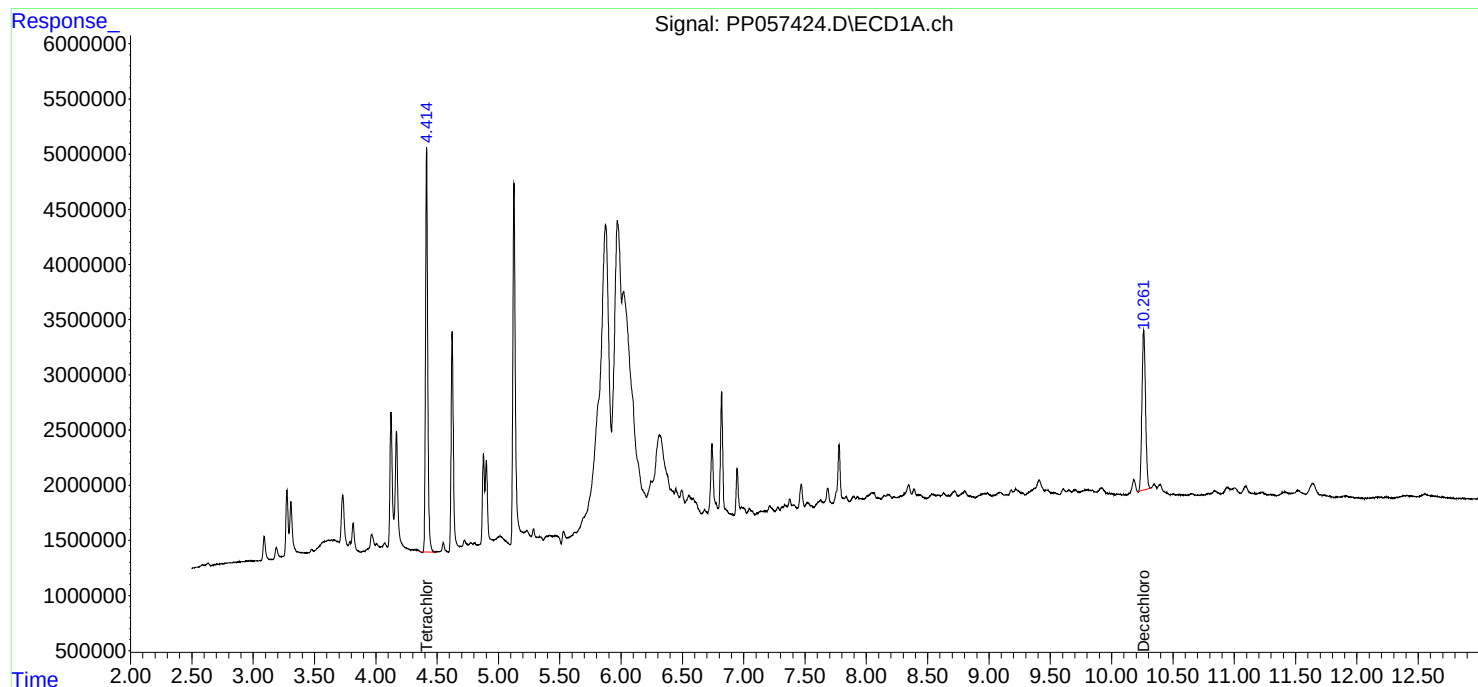

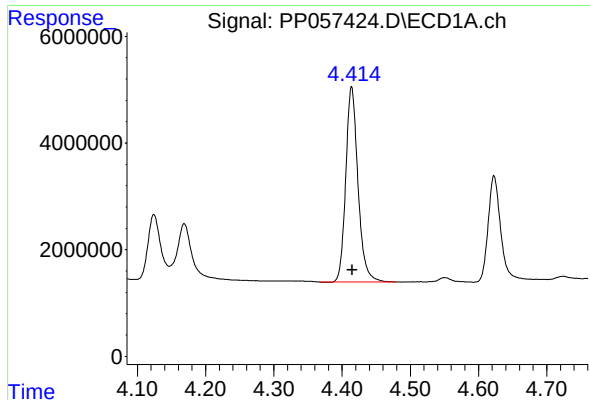


#1 Tetrachloro-m-xylene

R.T.: 4.414 min
Delta R.T.: 0.000 min
Response: 45548037
Conc: 19.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
RT2343


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/03/2023
Supervised By :Ankita Jodhani 05/03/2023

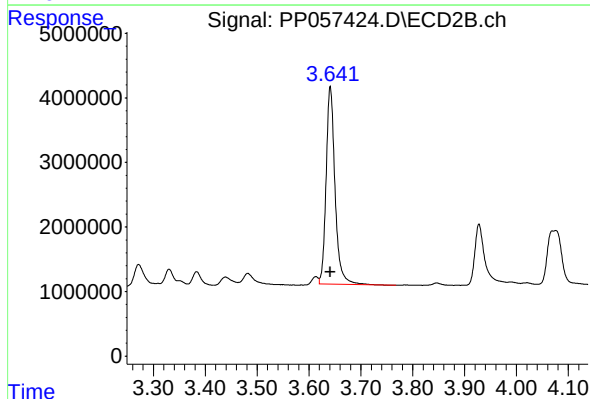


#1 Tetrachloro-m-xylene

R.T.: 3.641 min
Delta R.T.: 0.000 min
Response: 36444176
Conc: 20.55 ng/ml

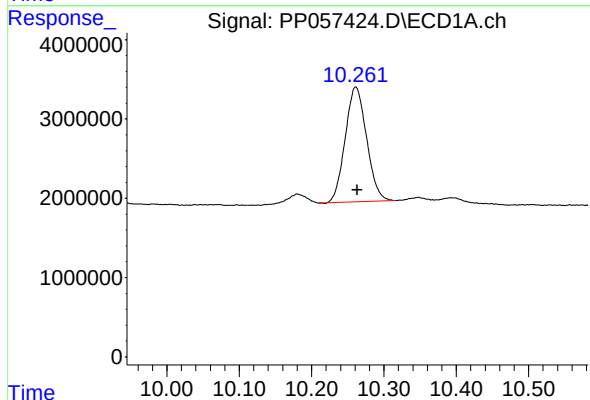

#2 Decachlorobiphenyl

R.T.: 10.261 min
Delta R.T.: -0.003 min
Response: 29716997
Conc: 18.01 ng/ml

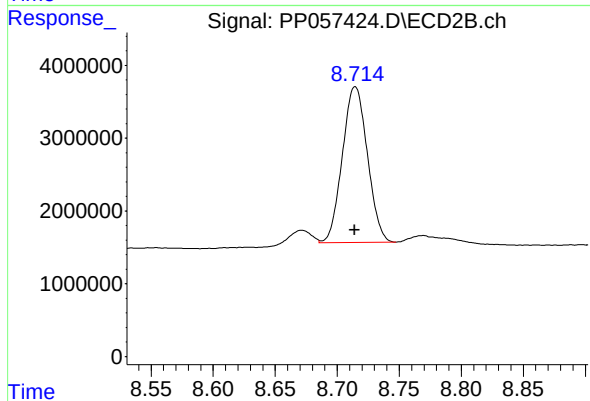

#2 Decachlorobiphenyl

R.T.: 8.714 min
Delta R.T.: 0.000 min
Response: 30043750
Conc: 15.31 ng/ml m