

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050224\
 Data File : PP064645.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 May 2024 14:21
 Operator : YP\AJ
 Sample : P2346-02 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 Y2308-0022-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/03/2024
 Supervised By :Ankita Jodhani 05/06/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 02 16:01:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP043024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 01 05:01:39 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.445	2165395	3661323	1.230m	1.553m#
2) SA Decachlor...	10.078	8.360	1590700	2622394	1.788	1.406

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050224\
Data File : PP064645.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 May 2024 14:21
Operator : YP\AJ
Sample : P2346-02 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
Y2308-0022-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/03/2024
Supervised By :Ankita Jodhani 05/06/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 02 16:01:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP043024.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 01 05:01:39 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

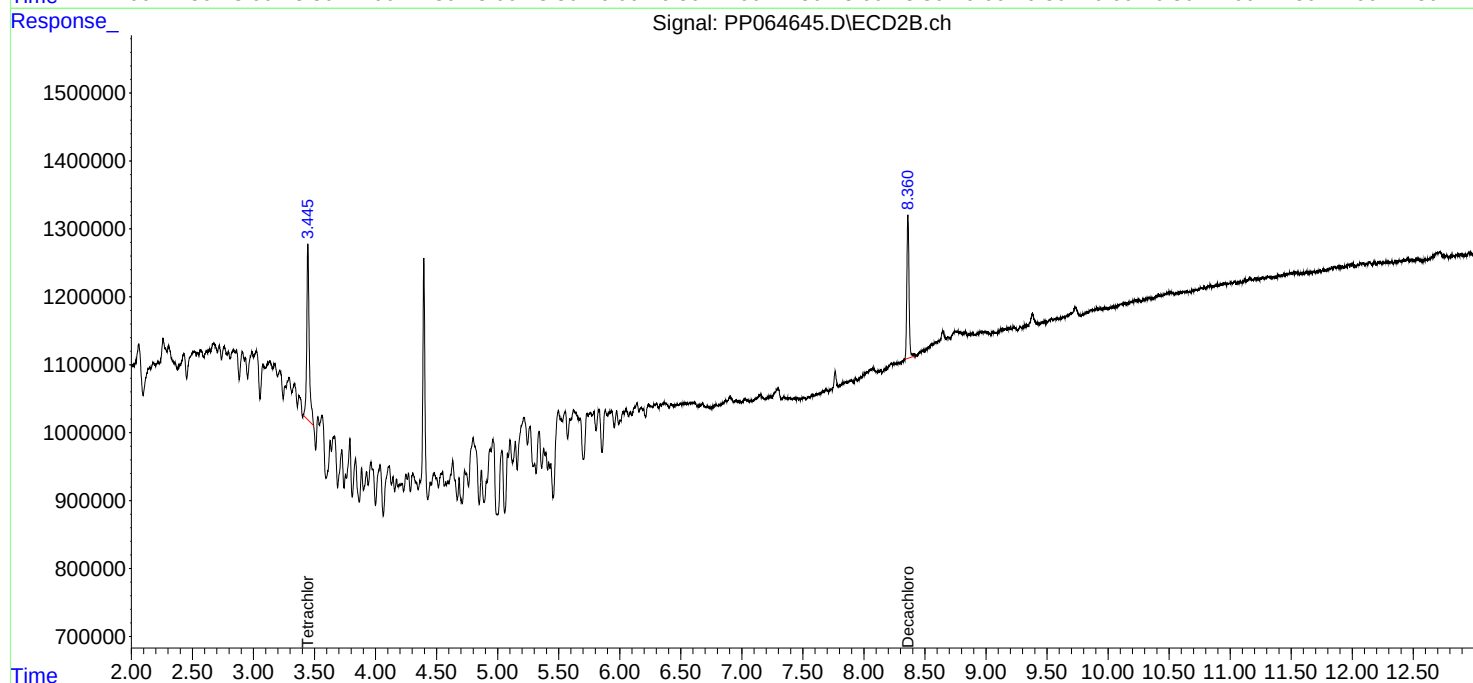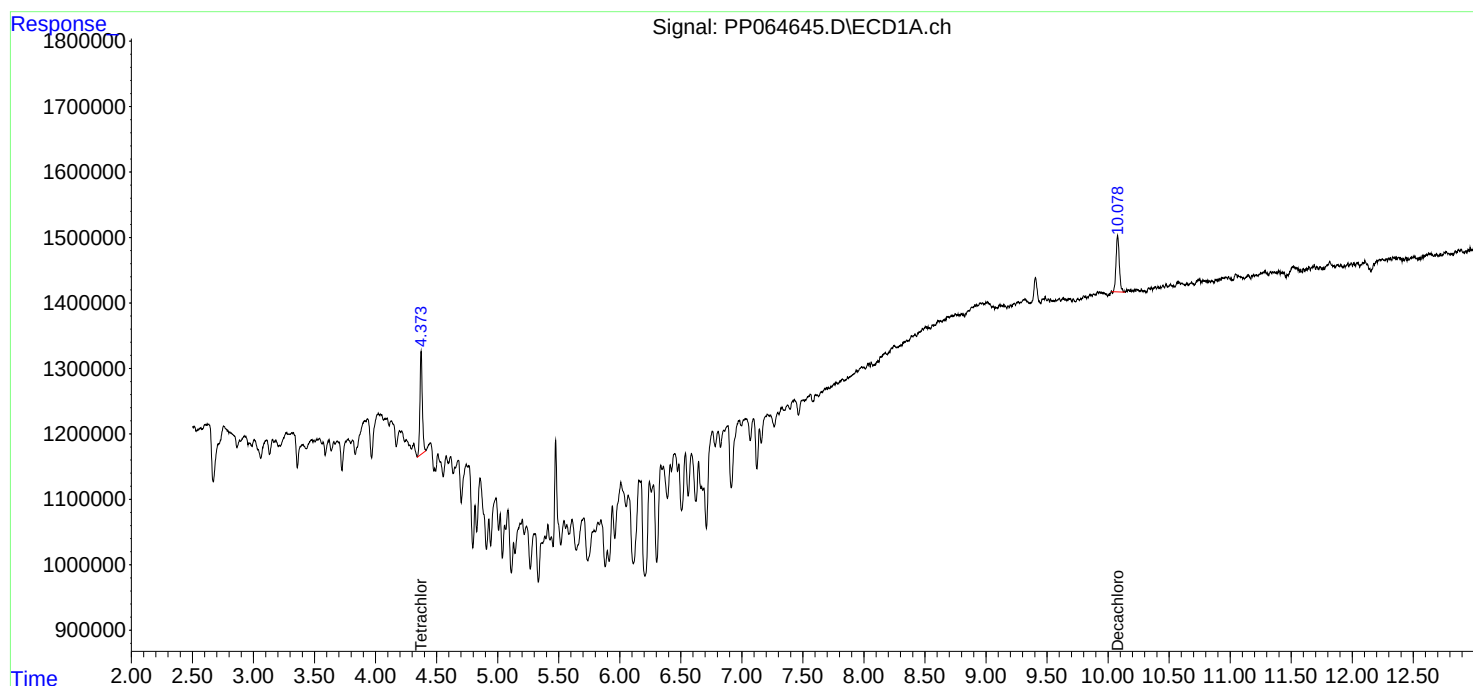

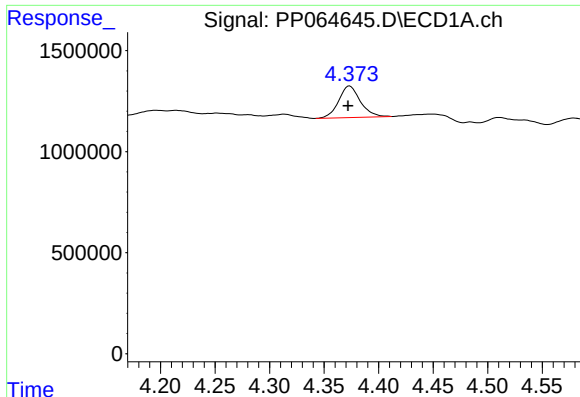


#1 Tetrachloro-m-xylene

R.T.: 4.373 min
Delta R.T.: 0.000 min
Response: 2165395
Conc: 1.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
Y2308-0022-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/03/2024
Supervised By :Ankita Jodhani 05/06/2024

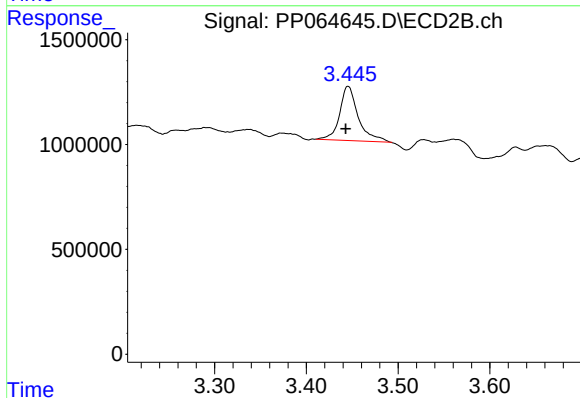


#1 Tetrachloro-m-xylene

R.T.: 3.445 min
Delta R.T.: 0.002 min
Response: 3661323
Conc: 1.55 ng/ml m

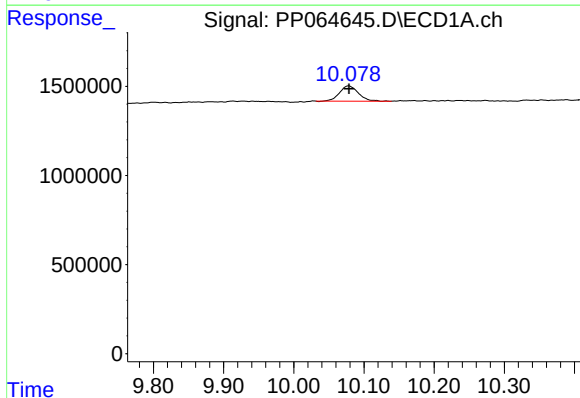

#2 Decachlorobiphenyl

R.T.: 10.078 min
Delta R.T.: 0.000 min
Response: 1590700
Conc: 1.79 ng/ml

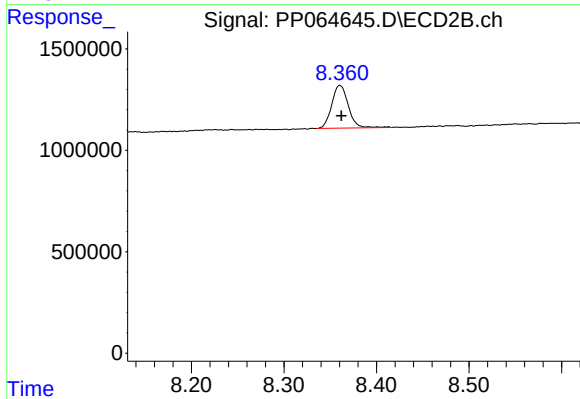

#2 Decachlorobiphenyl

R.T.: 8.360 min
Delta R.T.: -0.002 min
Response: 2622394
Conc: 1.41 ng/ml