

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050224\
 Data File : PP064673.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2024 00:30
 Operator : YP\AJ
 Sample : P2330-07
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 H-1(0.5-1.5)

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/03/2024
 Supervised By :Ankita Jodhani 05/06/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 01:50:42 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP043024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 01 05:01:39 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.442	31681324	36664656	18.000	15.551m
2) SA Decachlor...	10.073	8.357	19980090	33341269	22.457	17.874

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050224\
Data File : PP064673.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2024 00:30
Operator : YP\AJ
Sample : P2330-07
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
H-1(0.5-1.5)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/03/2024
Supervised By :Ankita Jodhani 05/06/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 01:50:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP043024.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 01 05:01:39 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

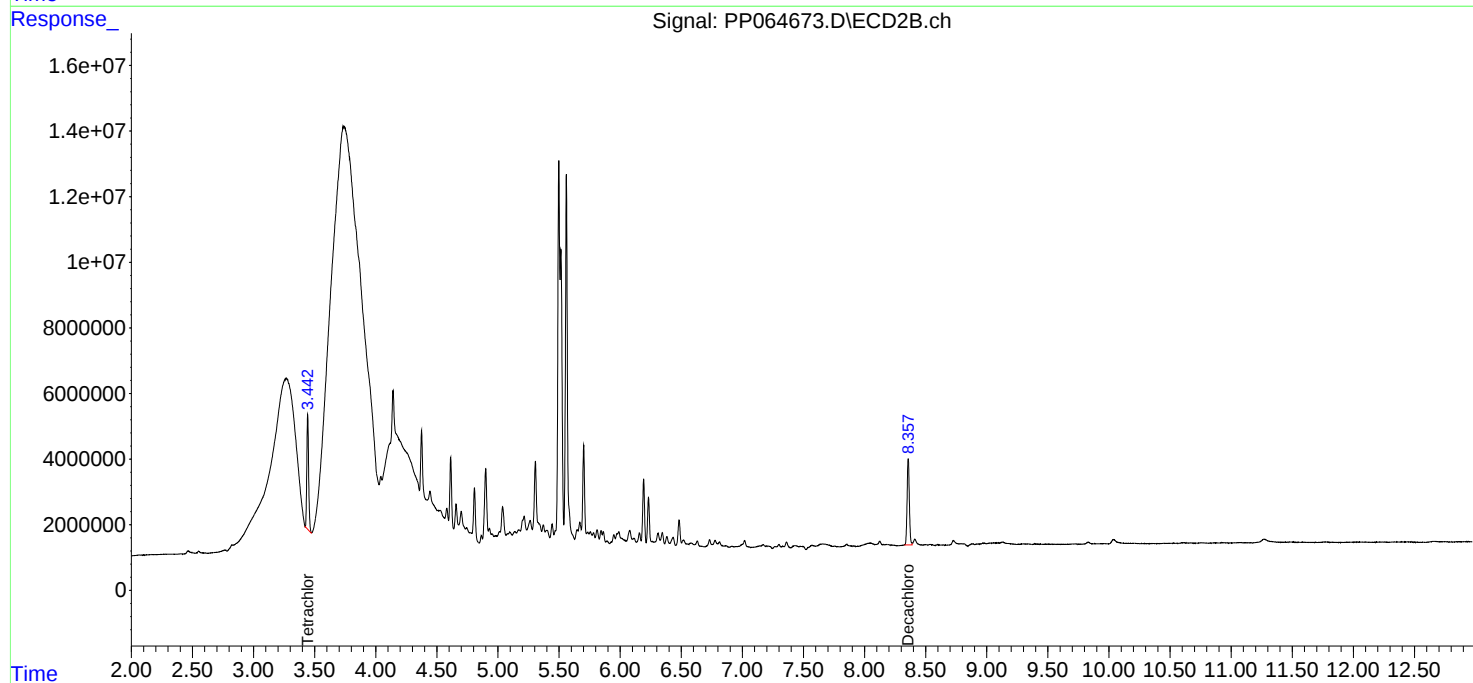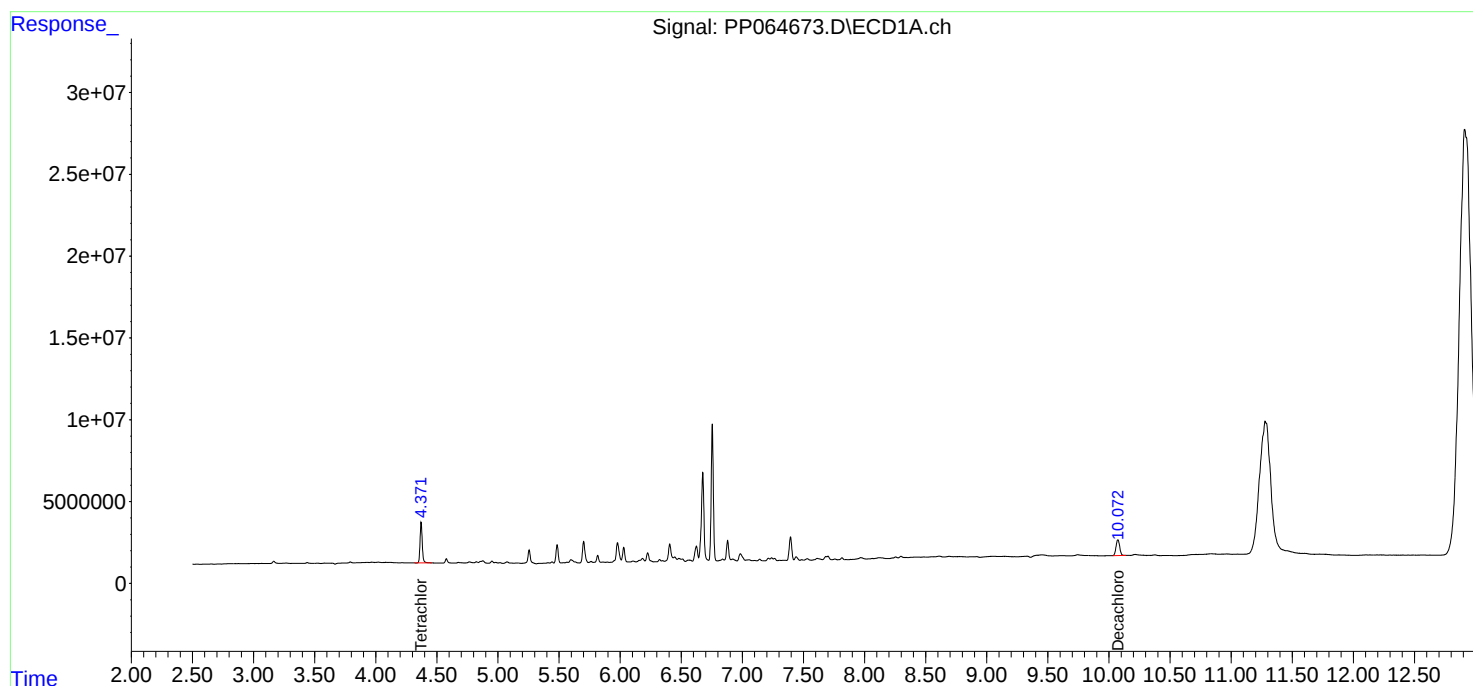

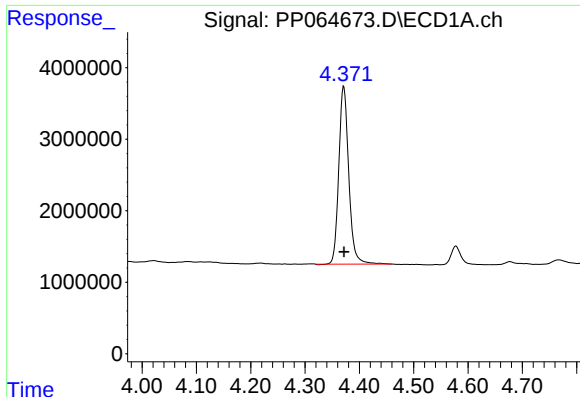


#1 Tetrachloro-m-xylene

R.T.: 4.371 min
Delta R.T.: 0.000 min
Response: 31681324
Conc: 18.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
H-1(0.5-1.5)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/03/2024
Supervised By :Ankita Jodhani 05/06/2024

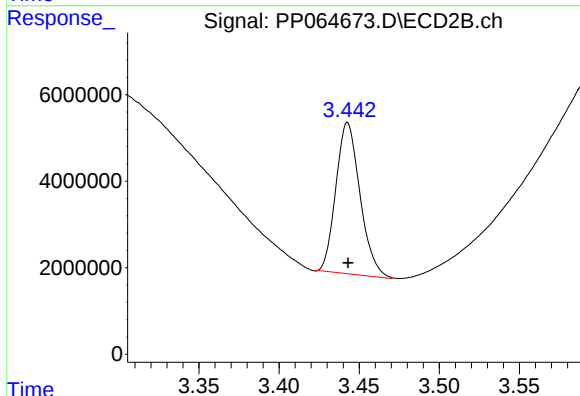


#1 Tetrachloro-m-xylene

R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 36664656
Conc: 15.55 ng/ml m

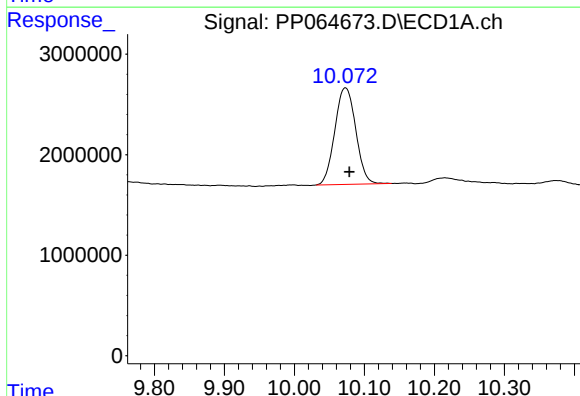

#2 Decachlorobiphenyl

R.T.: 10.073 min
Delta R.T.: -0.006 min
Response: 19980090
Conc: 22.46 ng/ml

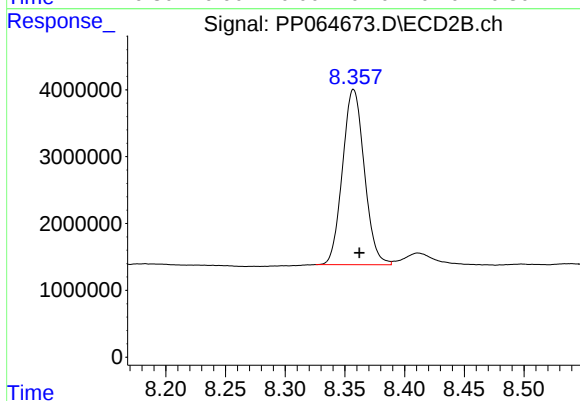

#2 Decachlorobiphenyl

R.T.: 8.357 min
Delta R.T.: -0.005 min
Response: 33341269
Conc: 17.87 ng/ml