

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050224\
 Data File : PP064691.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2024 06:28
 Operator : YP\AJ
 Sample : P2339-01 10X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 D3479

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/03/2024
 Supervised By :Ankita Jodhani 05/06/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 06:48:25 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP043024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 01 05:01:39 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.368	3.450	4591075	3968342	2.608m	1.683 #
2) SA Decachlor...	10.071	8.355	2939493	4788342	3.304	2.567

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050224\
Data File : PP064691.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2024 06:28
Operator : YP\AJ
Sample : P2339-01 10X
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
D3479


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/03/2024
Supervised By :Ankita Jodhani 05/06/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 06:48:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP043024.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 01 05:01:39 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

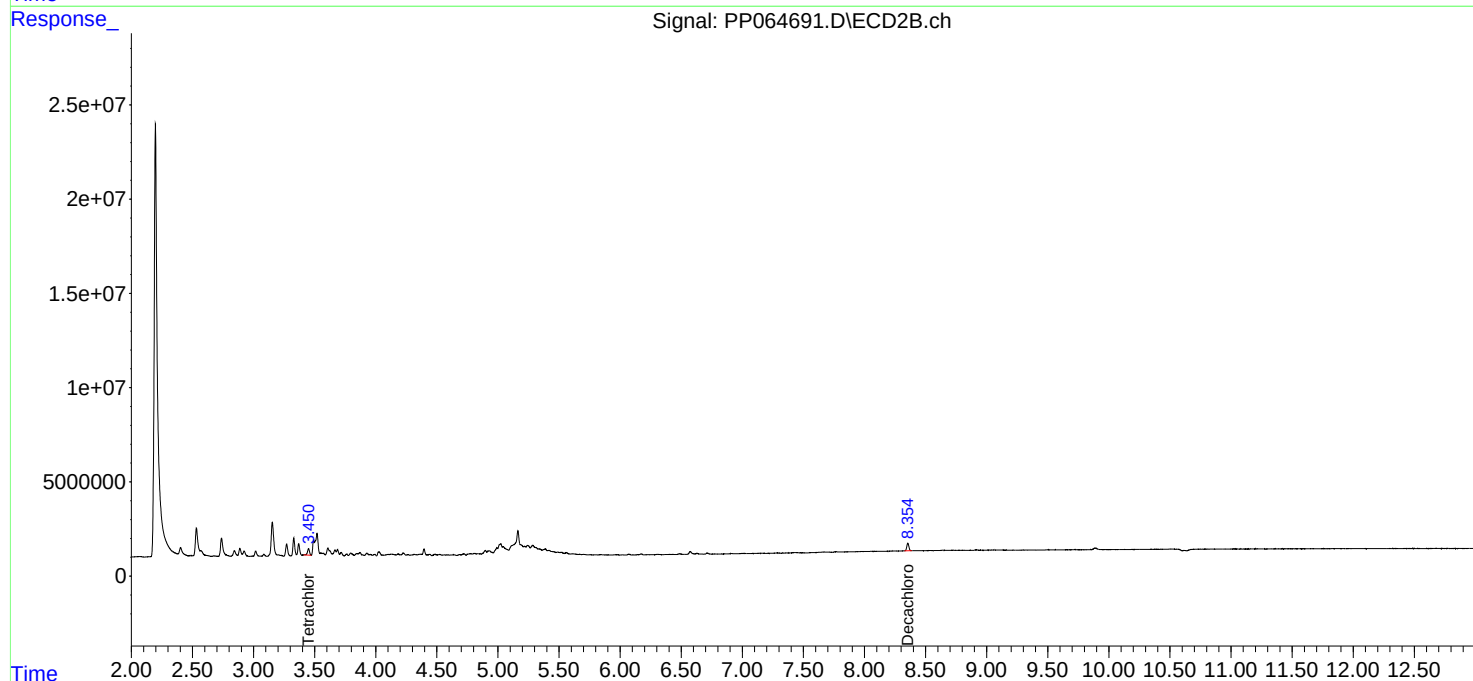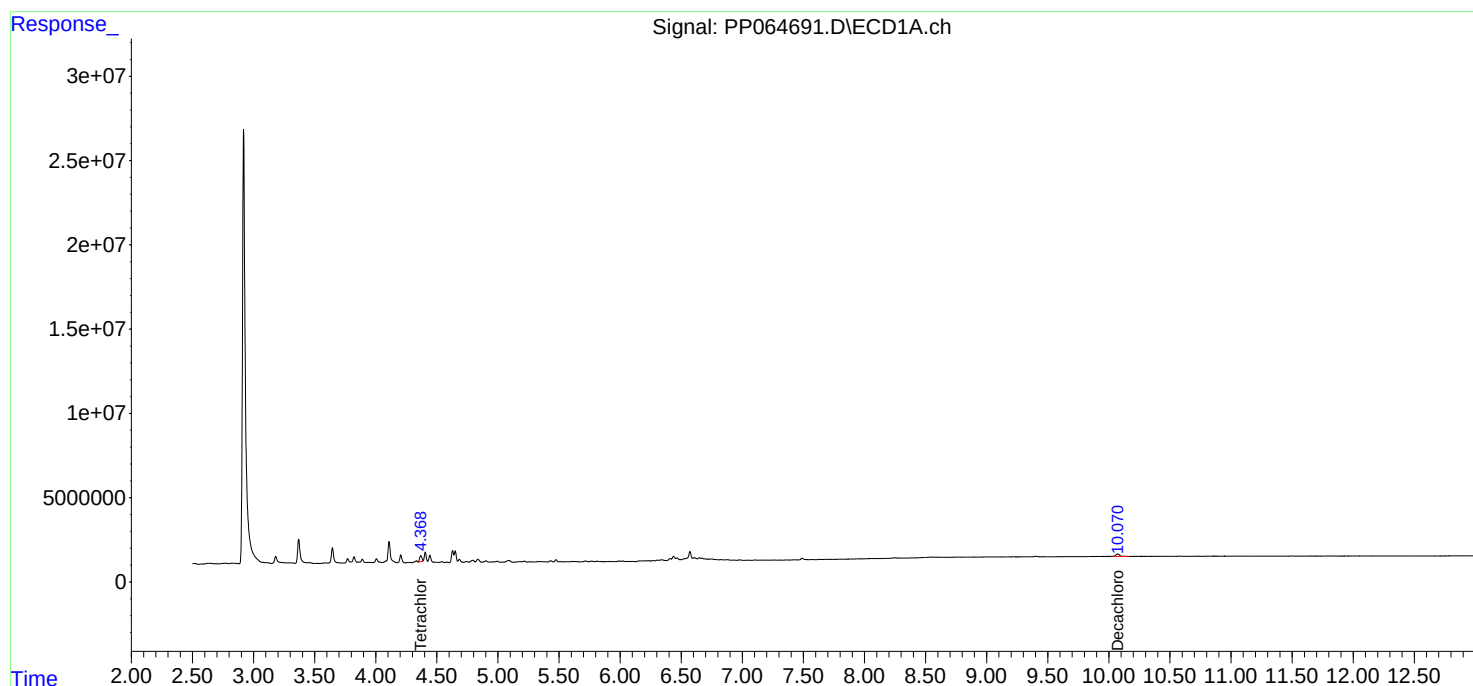

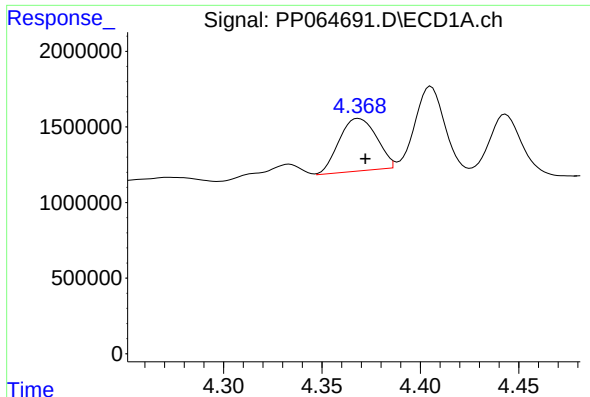

#1 Tetrachloro-m-xylene

R.T.: 4.368 min
Delta R.T.: -0.004 min
Response: 4591075
Conc: 2.61 ng/ml


Instrument :

ECD_P

ClientSampleId :
D3479


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/03/2024
Supervised By :Ankita Jodhani 05/06/2024

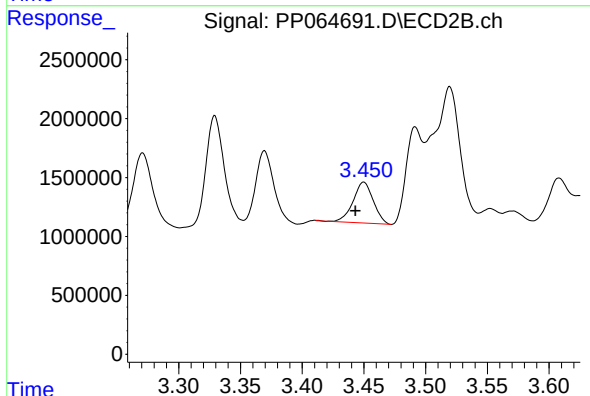


#1 Tetrachloro-m-xylene

R.T.: 3.450 min
Delta R.T.: 0.007 min
Response: 3968342
Conc: 1.68 ng/ml

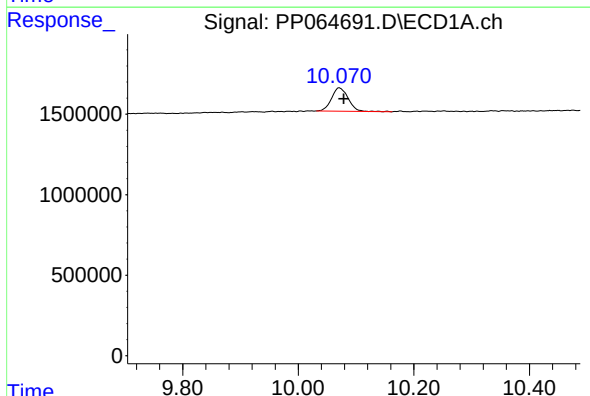

#2 Decachlorobiphenyl

R.T.: 10.071 min
Delta R.T.: -0.007 min
Response: 2939493
Conc: 3.30 ng/ml

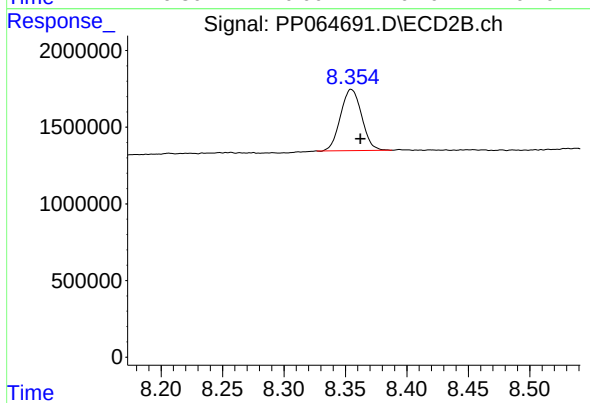

#2 Decachlorobiphenyl

R.T.: 8.355 min
Delta R.T.: -0.007 min
Response: 4788342
Conc: 2.57 ng/ml