

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050225\
 Data File : PP071759.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 May 2025 20:42
 Operator : YP\AJ
 Sample : Q1913-03DL 10X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WC-13-S-202504DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/05/2025
 Supervised By :mohammad ahmed 05/06/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 00:26:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042225.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 23 05:02:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.500	3.808	5304010	1505206	2.675m	1.069m#
2) SA Decachlor...	10.222	8.839	6248188	1899420	4.315m	2.166 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050225\
Data File : PP071759.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 May 2025 20:42
Operator : YP\AJ
Sample : Q1913-03DL 10X
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
WC-13-S-202504DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/05/2025
Supervised By :mohammad ahmed 05/06/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 00:26:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042225.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 23 05:02:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

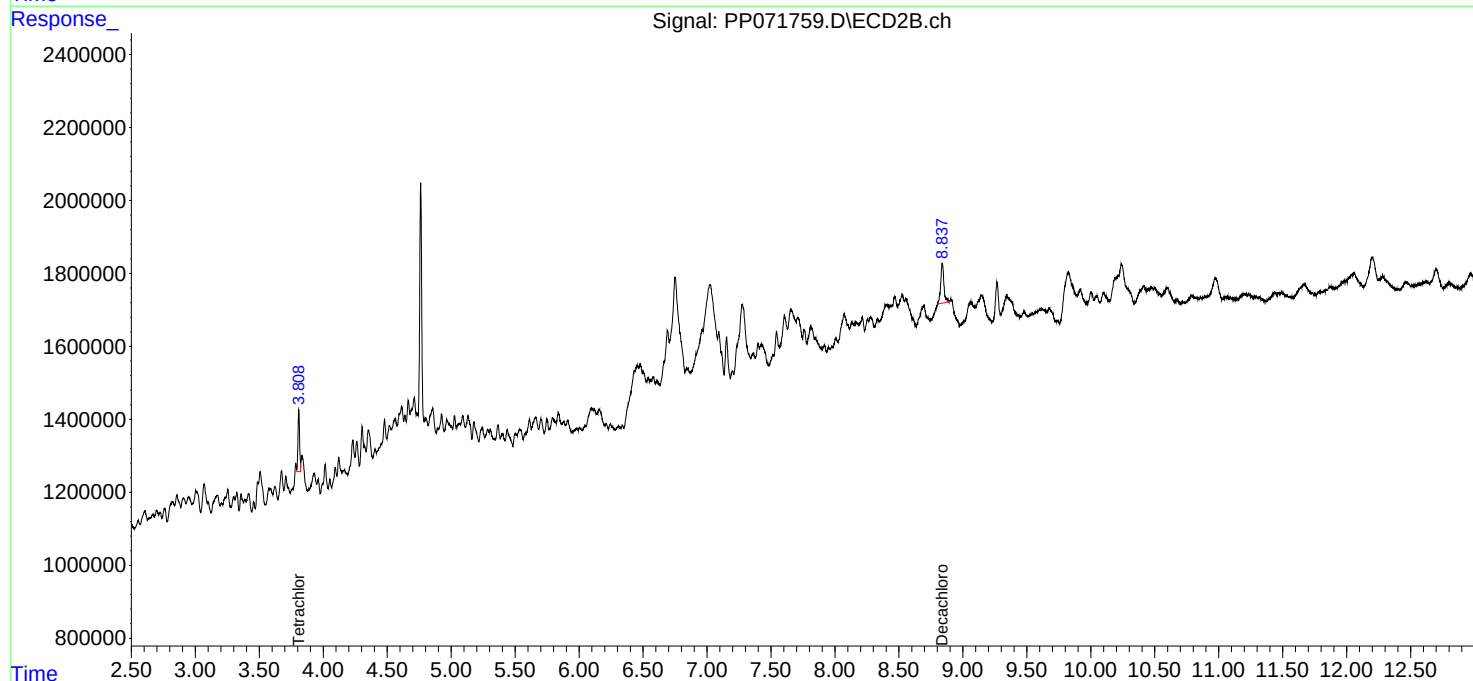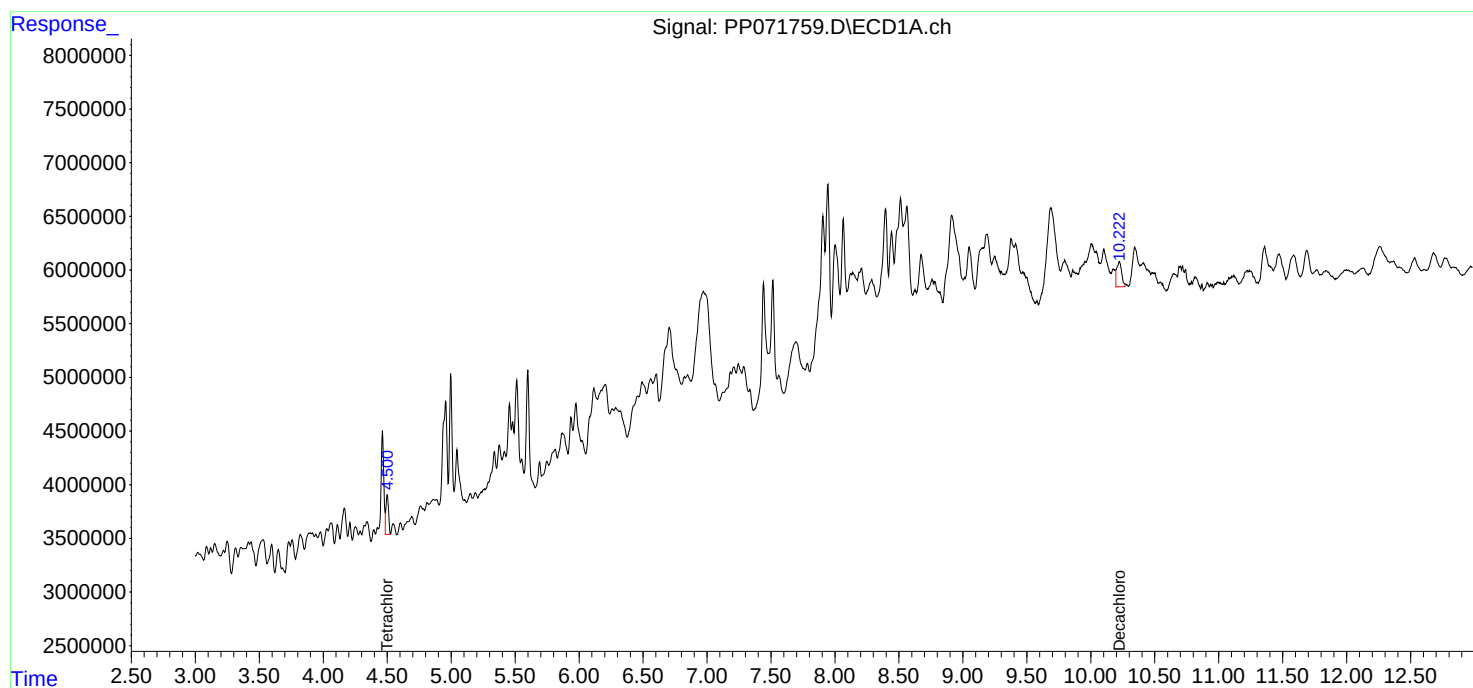

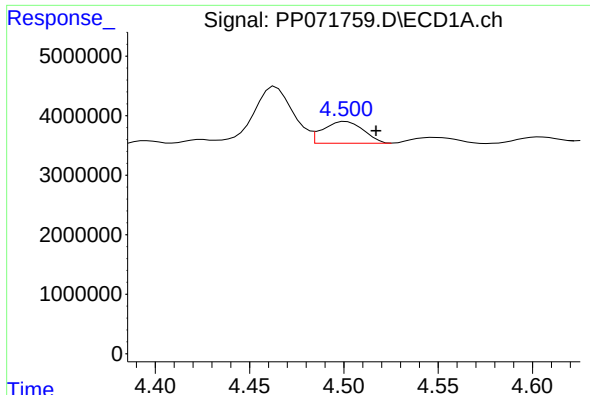


#1 Tetrachloro-m-xylene

R.T.: 4.500 min
Delta R.T.: -0.017 min
Response: 5304010
Conc: 2.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
WC-13-S-202504DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/05/2025
Supervised By :mohammad ahmed 05/06/2025

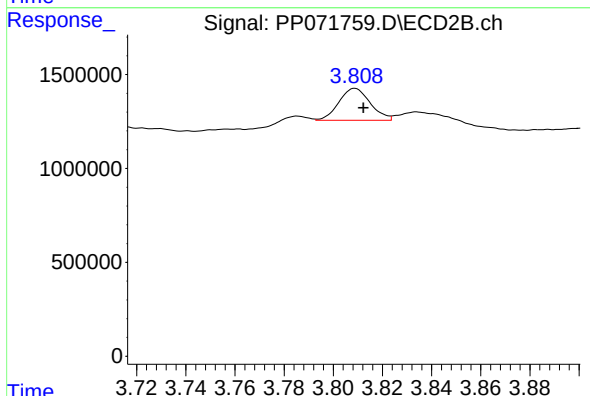


#1 Tetrachloro-m-xylene

R.T.: 3.808 min
Delta R.T.: -0.004 min
Response: 1505206
Conc: 1.07 ng/ml m

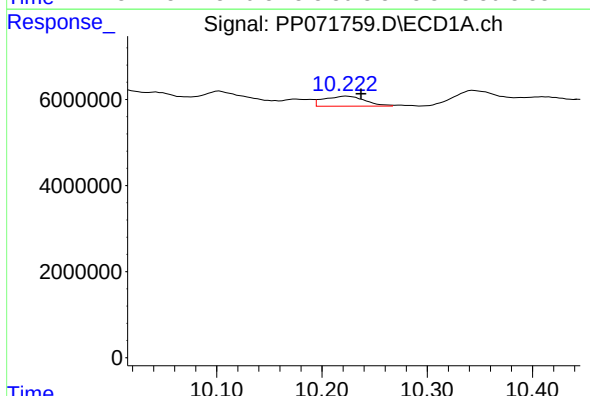

#2 Decachlorobiphenyl

R.T.: 10.222 min
Delta R.T.: -0.015 min
Response: 6248188
Conc: 4.32 ng/ml m

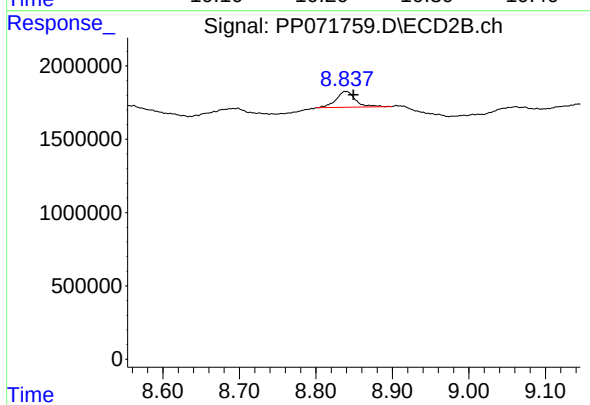

#2 Decachlorobiphenyl

R.T.: 8.839 min
Delta R.T.: -0.010 min
Response: 1899420
Conc: 2.17 ng/ml