

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050321\
 Data File : PP035460.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 May 2021 9:31
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 17:04:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 03 09:49:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
25)	L5	AR-1248-5	0.000	6.356	0	417329 N.D. 437.467 #
27)	L6	AR-1254-2	0.000	6.492f	0	260484 N.D. 196.742 #
28)	L6	AR-1254-3	0.000	6.887	0	286659 N.D. 141.262 #
32)	L7	AR-1260-2	0.000	7.216	0	46194 N.D. 27.511 #
40)	L8	AR-1262-5	0.000	8.923f	0	137363 N.D. 136.949 #
43)	L9	AR-1268-3	0.000	8.618f	0	91170 N.D. 33.726 #
44)	L9	AR-1268-4	0.000	8.923	0	137363 N.D. 121.355 #
45)	L9	AR-1268-5	0.000	9.247f	0	140910 N.D. 18.285 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050321\
Data File : PP035460.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 May 2021 9:31
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 17:04:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 03 09:49:05 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

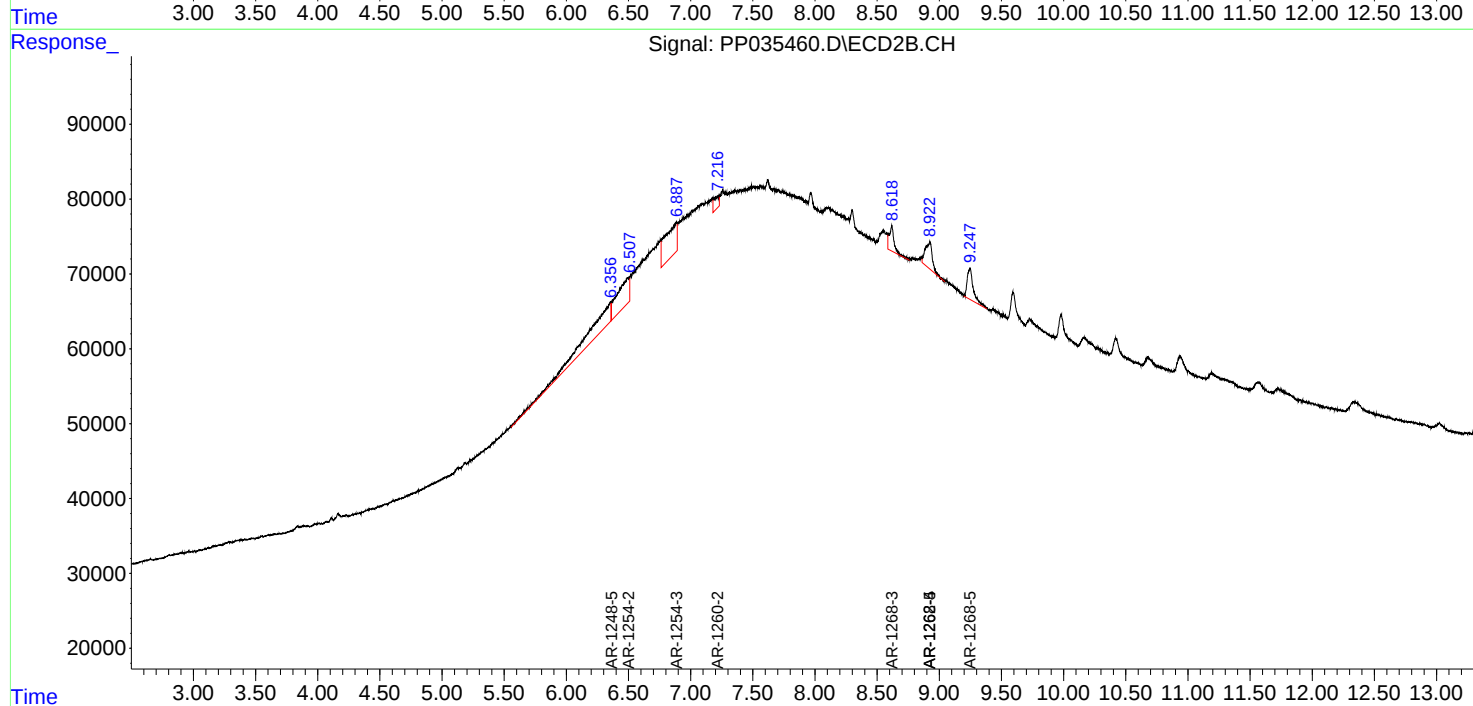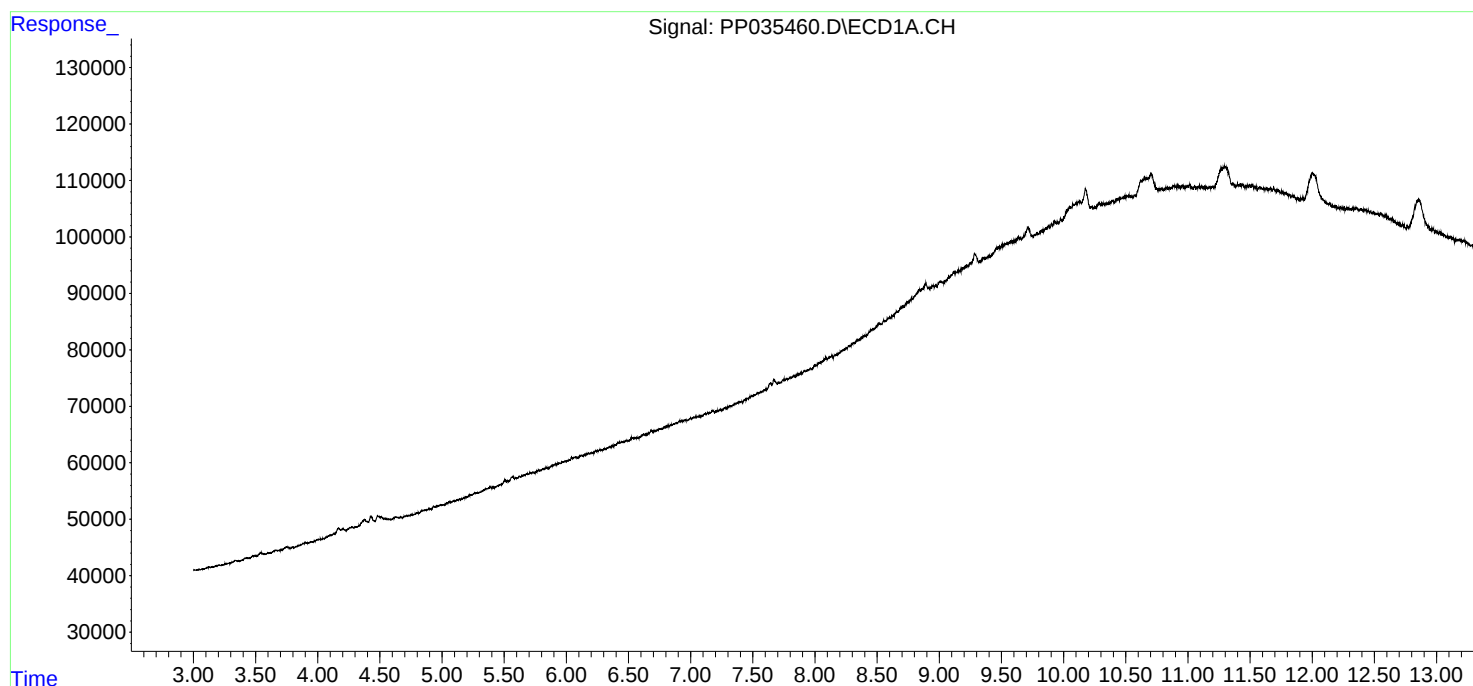


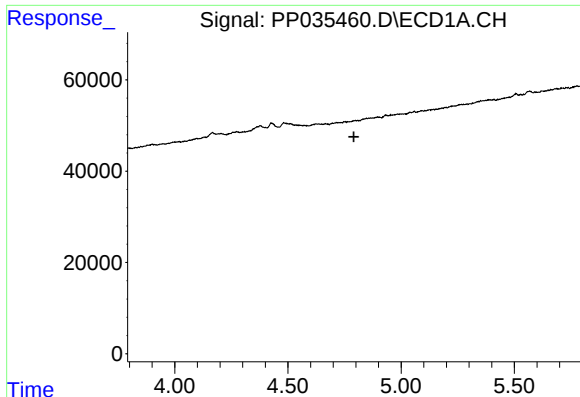

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.791 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

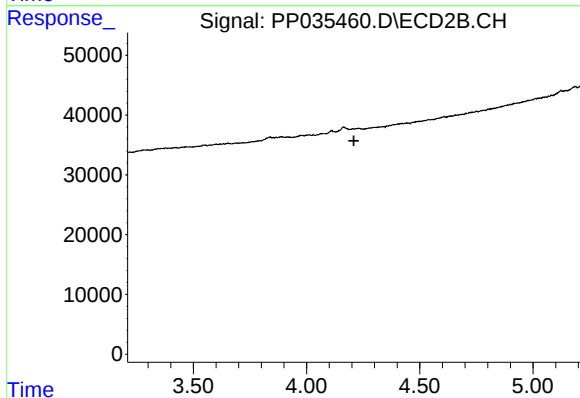


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.209 min
Response: 0
Conc: N.D.

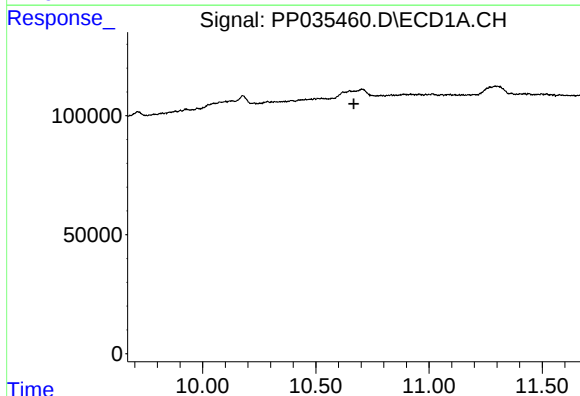


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.668 min
Response: 0
Conc: N.D.

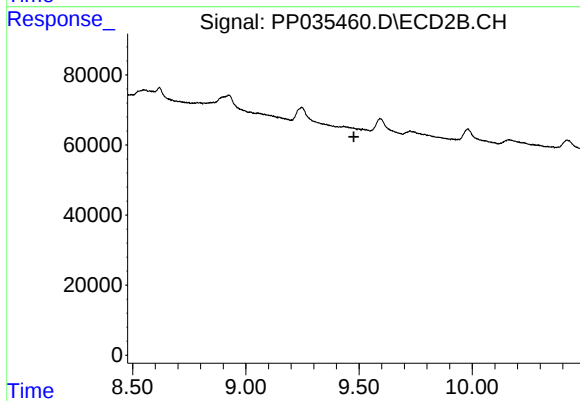

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.477 min
Response: 0
Conc: N.D.

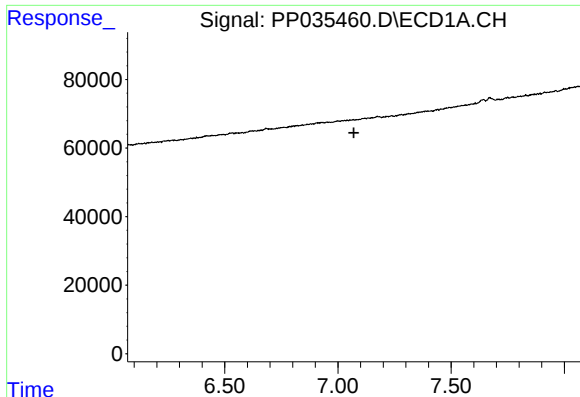

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 7.070 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

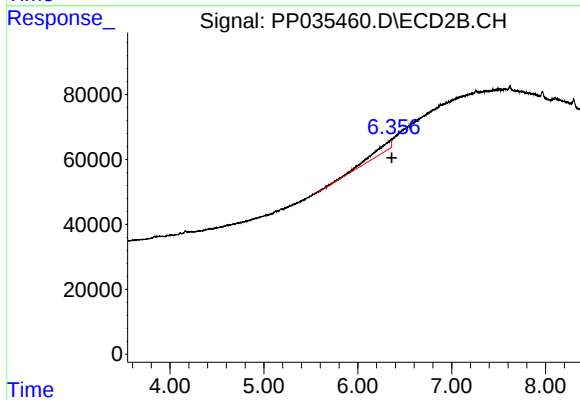


#25 AR-1248-5

R.T.: 6.356 min
Delta R.T.: -0.005 min
Response: 417329
Conc: 437.47 ng/ml

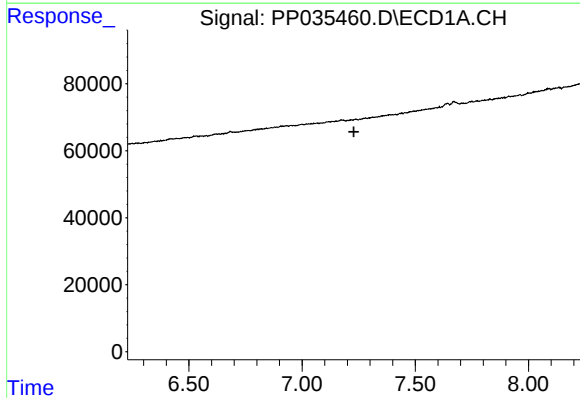


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T.: 7.229 min
Response: 0
Conc: N.D.

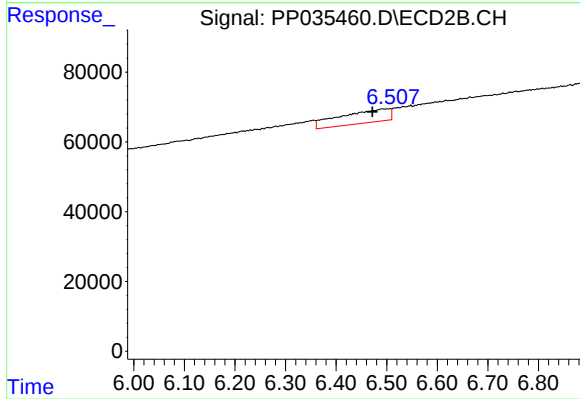

#27 AR-1254-2


R.T.: 6.492 min
Delta R.T.: 0.020 min
Response: 260484
Conc: 196.74 ng/ml

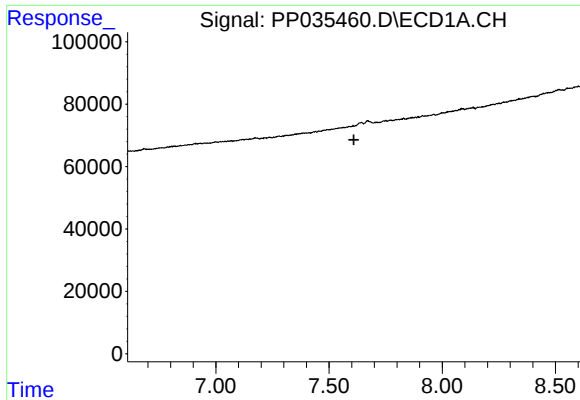

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 7.610 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

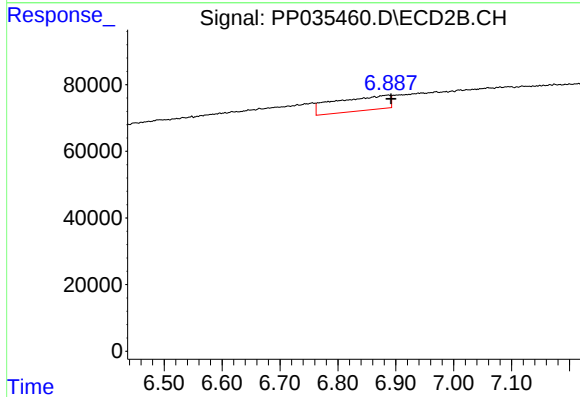


#28 AR-1254-3

R.T.: 6.887 min
Delta R.T.: -0.005 min
Response: 286659
Conc: 141.26 ng/ml

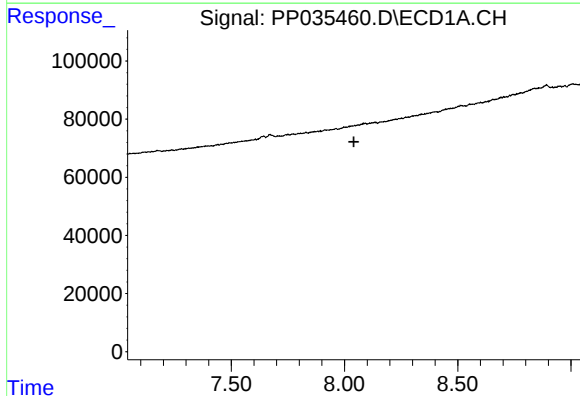


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 8.041 min
Response: 0
Conc: N.D.

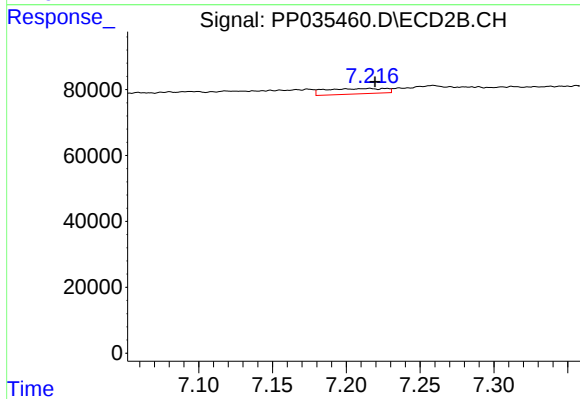

#32 AR-1260-2


R.T.: 7.216 min
Delta R.T.: -0.004 min
Response: 46194
Conc: 27.51 ng/ml

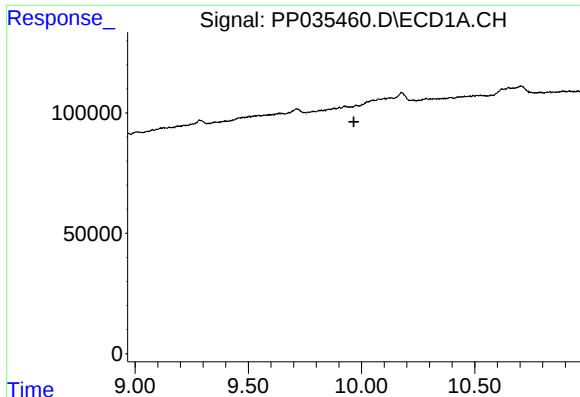

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 9.966 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

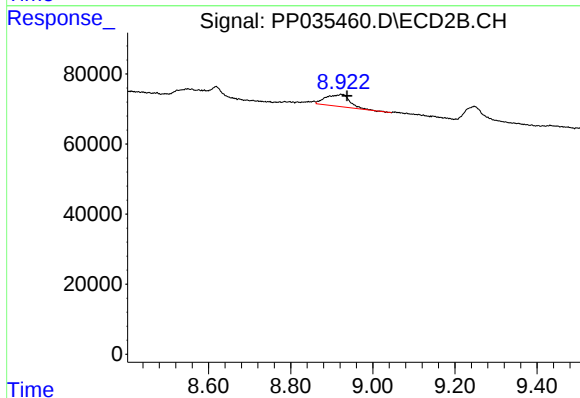


#40 AR-1262-5

R.T.: 8.923 min
Delta R.T.: -0.015 min
Response: 137363
Conc: 136.95 ng/ml

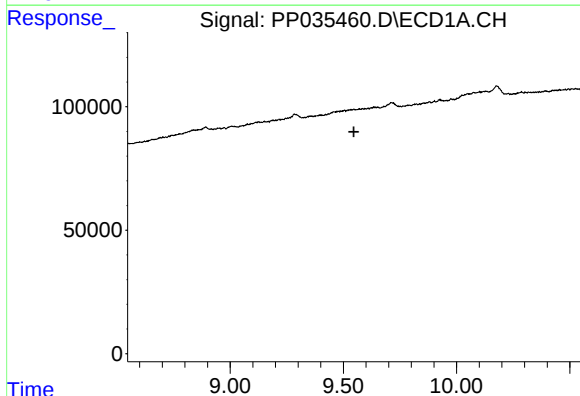


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 9.547 min
Response: 0
Conc: N.D.

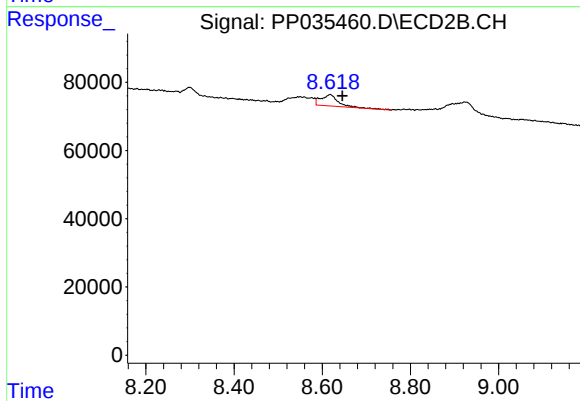

#43 AR-1268-3


R.T.: 8.618 min
Delta R.T.: -0.028 min
Response: 91170
Conc: 33.73 ng/ml

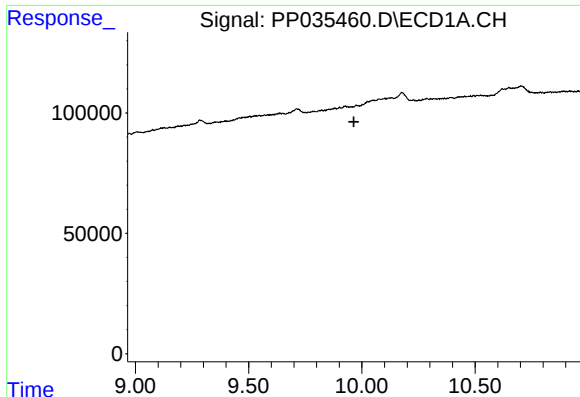

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 9.965 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

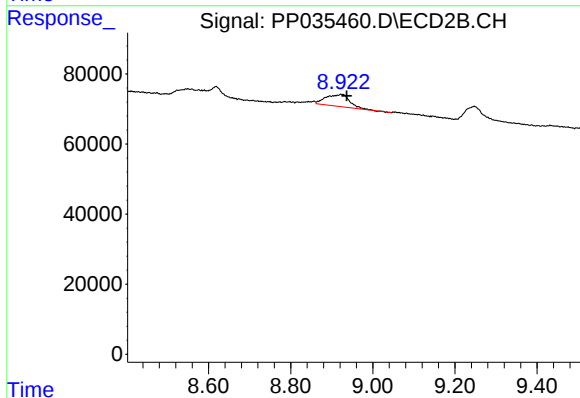


#44 AR-1268-4

R.T.: 8.923 min
Delta R.T.: -0.014 min
Response: 137363
Conc: 121.36 ng/ml

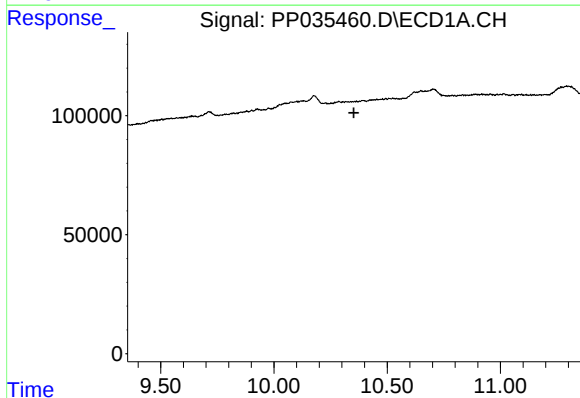

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 10.353 min
Response: 0
Conc: N.D.

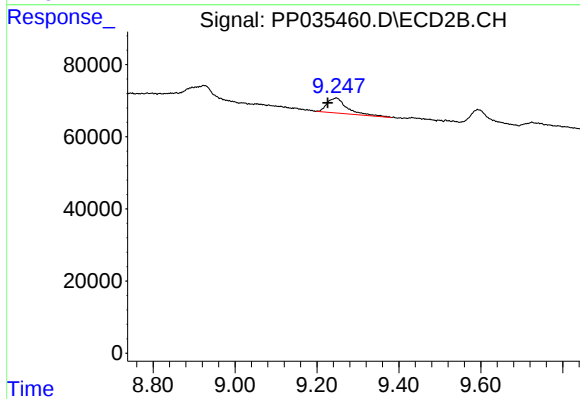

#45 AR-1268-5

R.T.: 9.247 min
Delta R.T.: 0.021 min
Response: 140910
Conc: 18.29 ng/ml