

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050321\
 Data File : PP035470.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 May 2021 12:56
 Operator : DD\AJ
 Sample : M2230-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 JTY3-WC-S-1

Manual Integrations
 APPROVED

Ankita
 5/4/2021 9:56:09 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 03:44:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 03 09:49:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.792	4.210	1023950	704189	20.167	20.684
2) SA Decachlor...	10.649	9.463	869098	411415	21.401m	21.231

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP050321\
Data File : PP035470.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 May 2021 12:56
Operator : DD\AJ
Sample : M2230-02
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
JTY3-WC-S-1


Manual Integrations
APPROVED

Ankita
5/4/2021 9:56:09 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 03:44:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042921.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 03 09:49:05 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

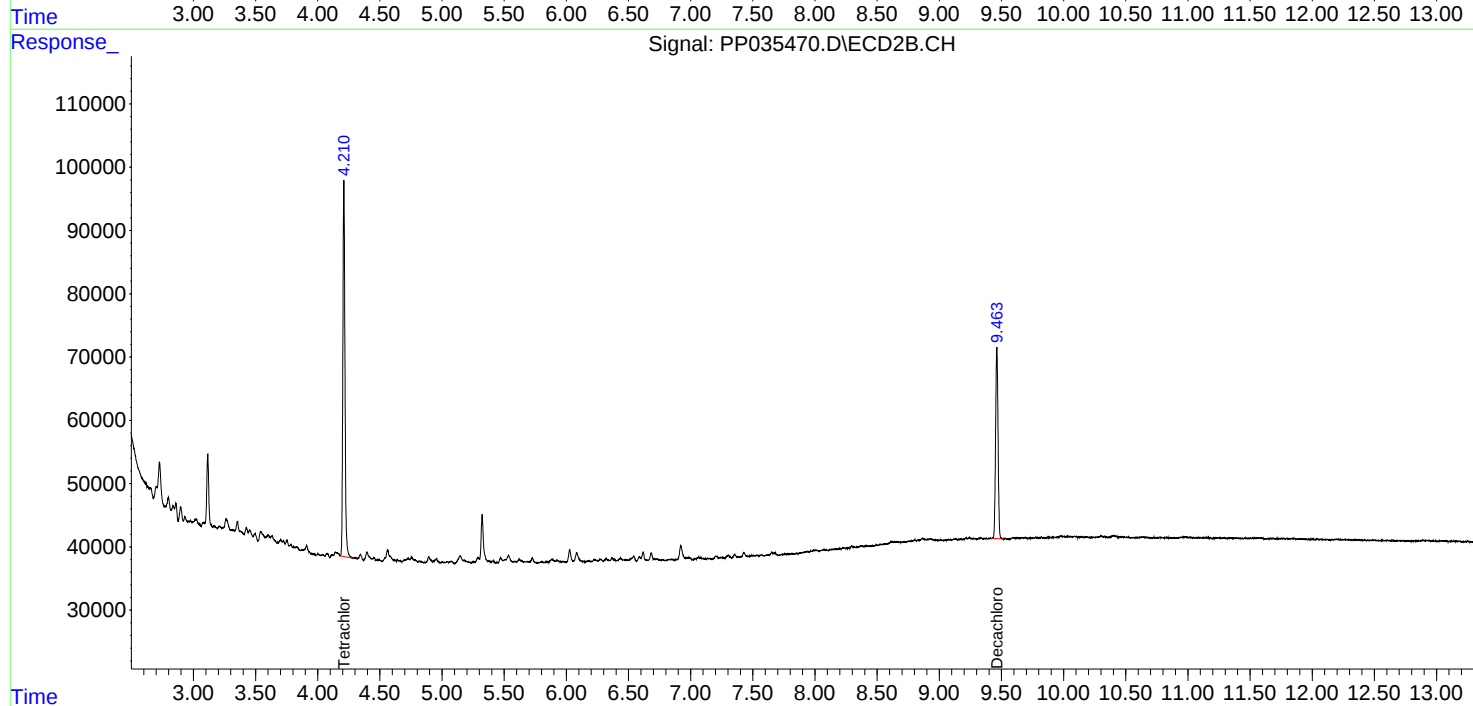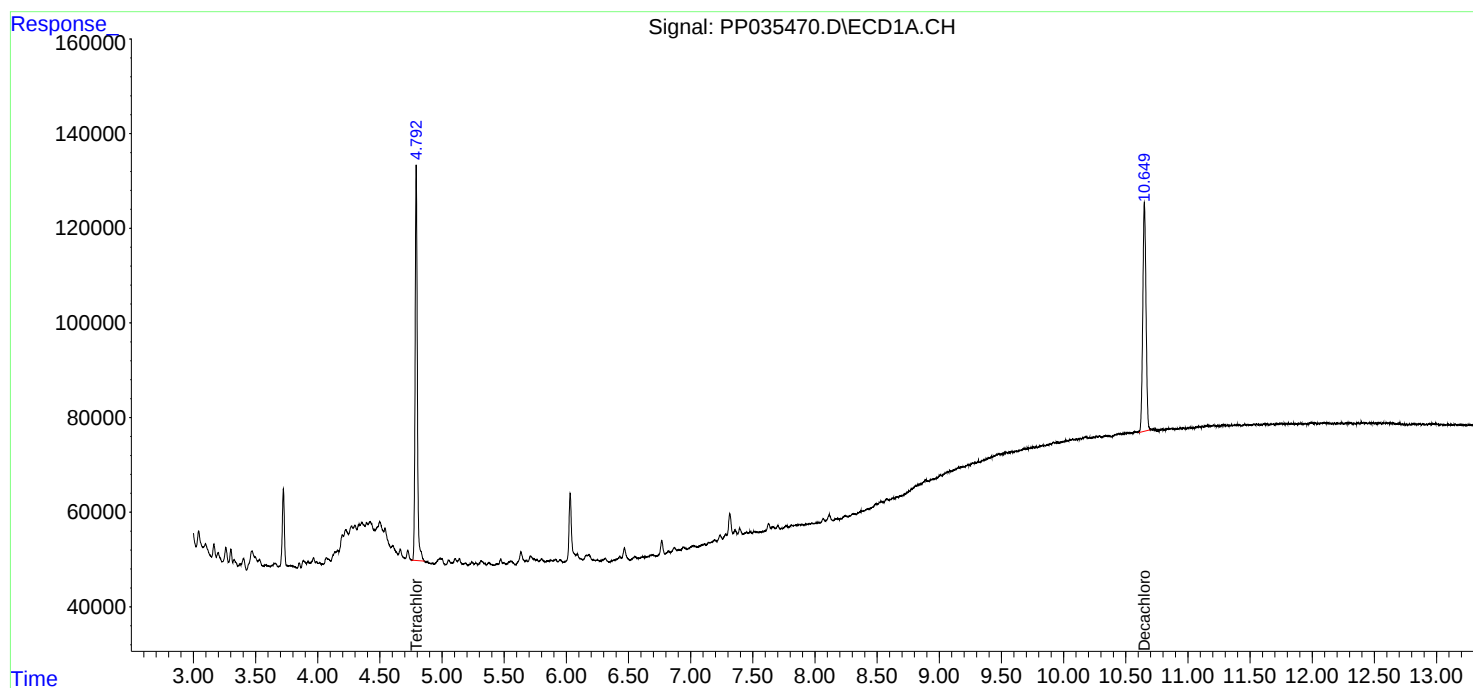

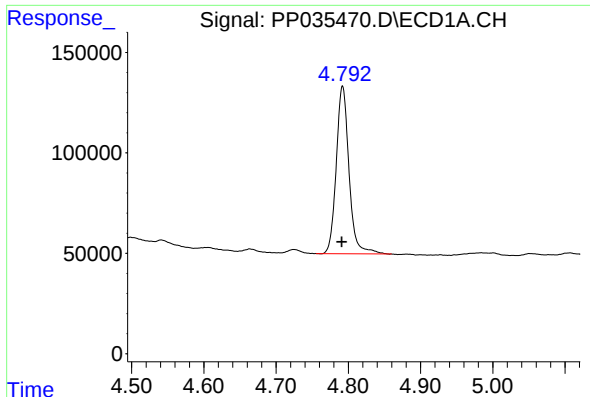


#1 Tetrachloro-m-xylene

R.T.: 4.792 min
Delta R.T.: 0.000 min
Response: 1023950
Conc: 20.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
JTY3-WC-S-1


Manual Integrations
APPROVED

Ankita
5/4/2021 9:56:09 AM

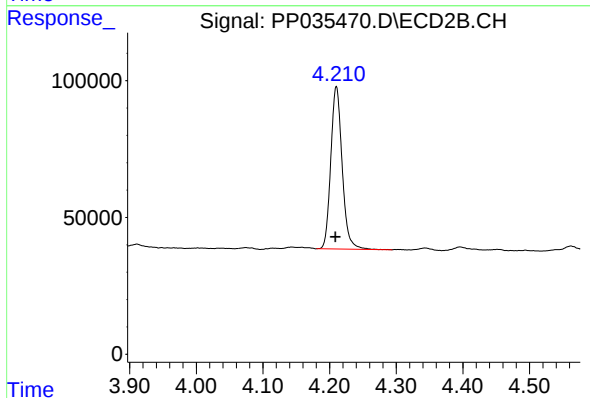


#1 Tetrachloro-m-xylene

R.T.: 4.210 min
Delta R.T.: 0.002 min
Response: 704189
Conc: 20.68 ng/ml

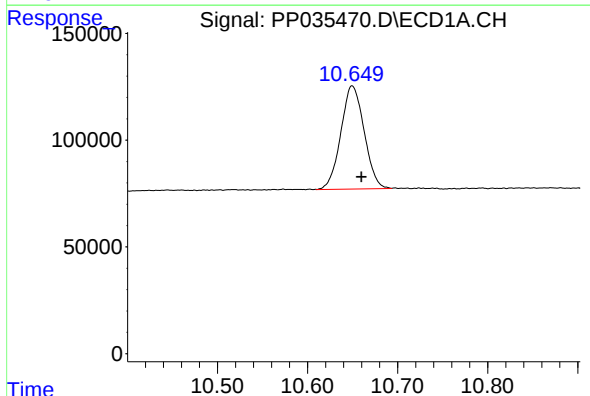

#2 Decachlorobiphenyl

R.T.: 10.649 min
Delta R.T.: -0.011 min
Response: 869098
Conc: 21.40 ng/ml m

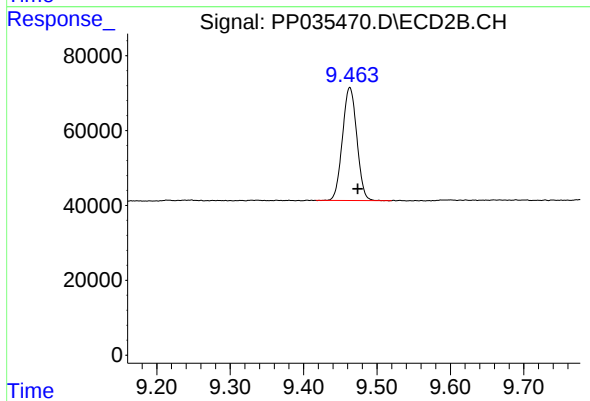

#2 Decachlorobiphenyl

R.T.: 9.463 min
Delta R.T.: -0.011 min
Response: 411415
Conc: 21.23 ng/ml